

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
 Data File : P0078173.D
 Signal(s) : ECD2B.CH
 Acq On : 5/26/2021 04:46:30 PM
 Operator : DD\AJ
 Sample : M2518-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 118-119

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:12:01 PM

Integration File: autoint1.e
 Quant Time: May 26 18:32:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.622	1226326	610441	16.593	20.202m
2) SA Decachlor...	9.958	8.812	620416	353494	12.549	12.157

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078173.D
Signal(s) : ECD2B.CH
Acq On : 5/26/2021 04:46:30 PM
Operator : DD\AJ
Sample : M2518-05
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
118-119


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:01 PM

Integration File: autoint1.e
Quant Time: May 26 18:32:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

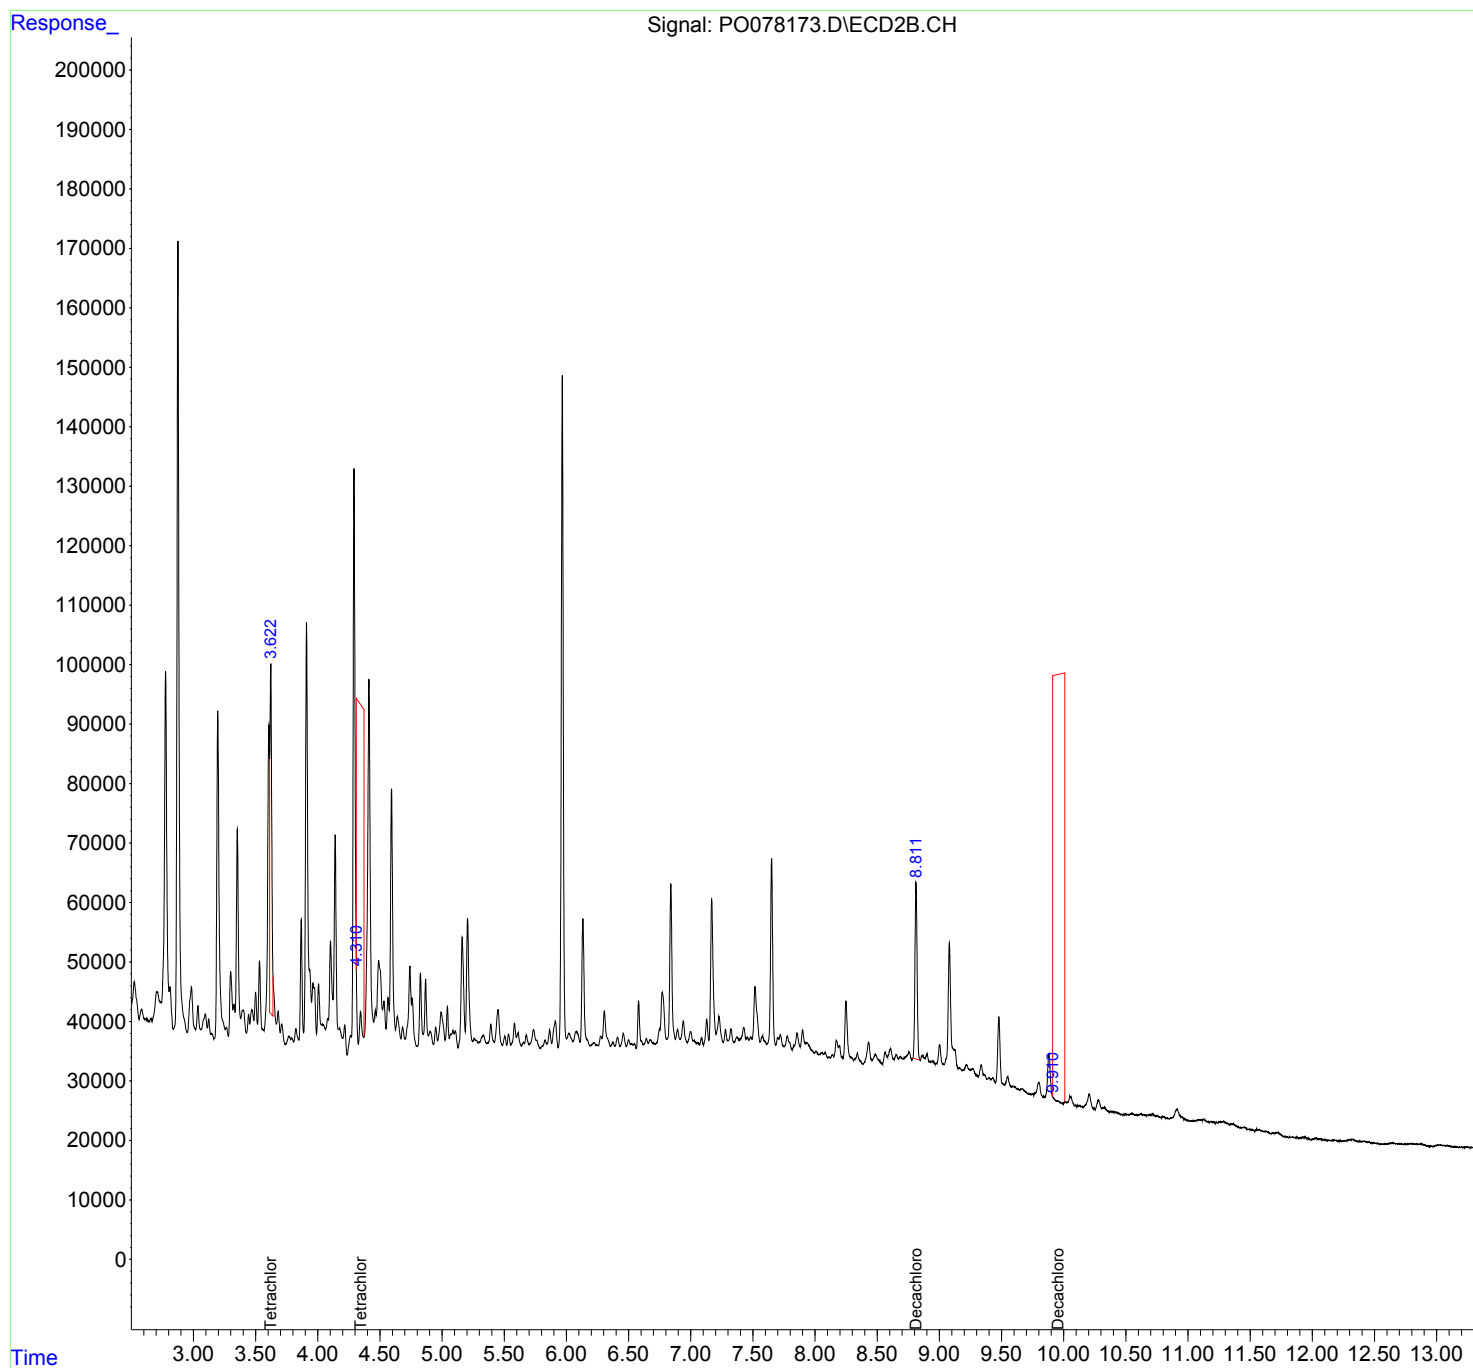

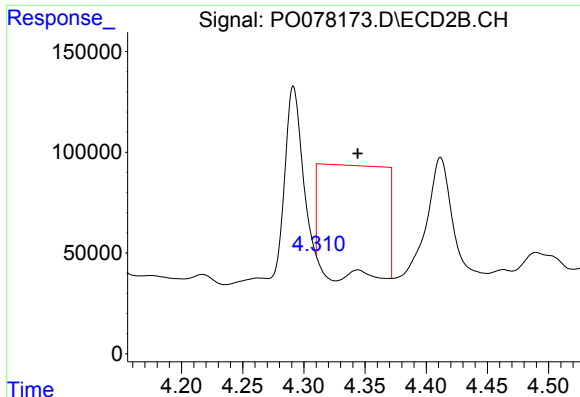


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 1226326
Conc: 16.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
118-119


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:01 PM

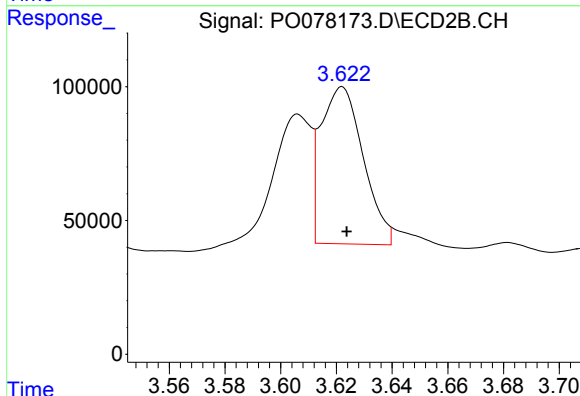


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.002 min
Response: 610441
Conc: 20.20 ng/ml m

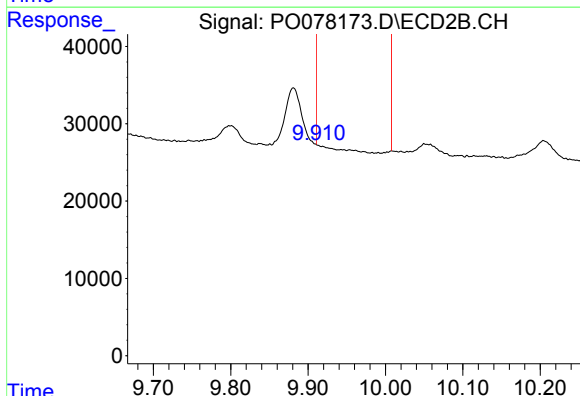

#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.003 min
Response: 620416
Conc: 12.55 ng/ml

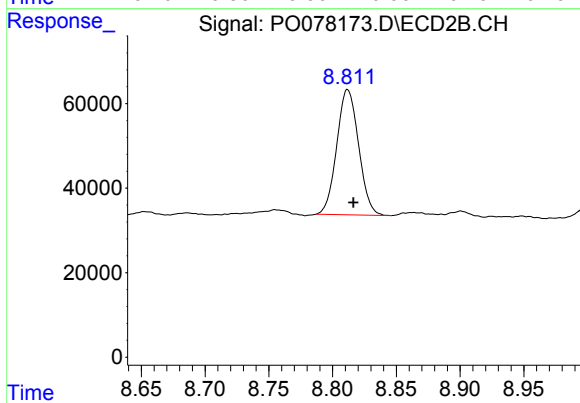

#2 Decachlorobiphenyl

R.T.: 8.812 min
Delta R.T.: -0.005 min
Response: 353494
Conc: 12.16 ng/ml