

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
 Data File : P0078178.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2021 18:12
 Operator : DD\AJ
 Sample : M2518-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 115

Manual Integrations
 APPROVED

Ankita
 5/27/2021 2:12:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 26 18:35:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.621	1699133	740429	22.990	24.504
2) SA Decachlor...	9.956	8.809	1149876	1253033	23.258m	43.093m#
Target Compounds						
26) L6 AR-1254-1	6.533	5.706	145713	84725	58.708m	49.127
27) L6 AR-1254-2	6.760	5.865	245809	70150	63.344	43.763 #
28) L6 AR-1254-3	7.135	6.278	437693	177003	111.561	74.161 #
29) L6 AR-1254-4	7.428	6.515	176006	74367	64.811	51.222
30) L6 AR-1254-5	7.851	6.939	537032	436811	183.633	192.179

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052621\
Data File : P0078178.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2021 18:12
Operator : DD\AJ
Sample : M2518-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
115


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 26 18:35:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

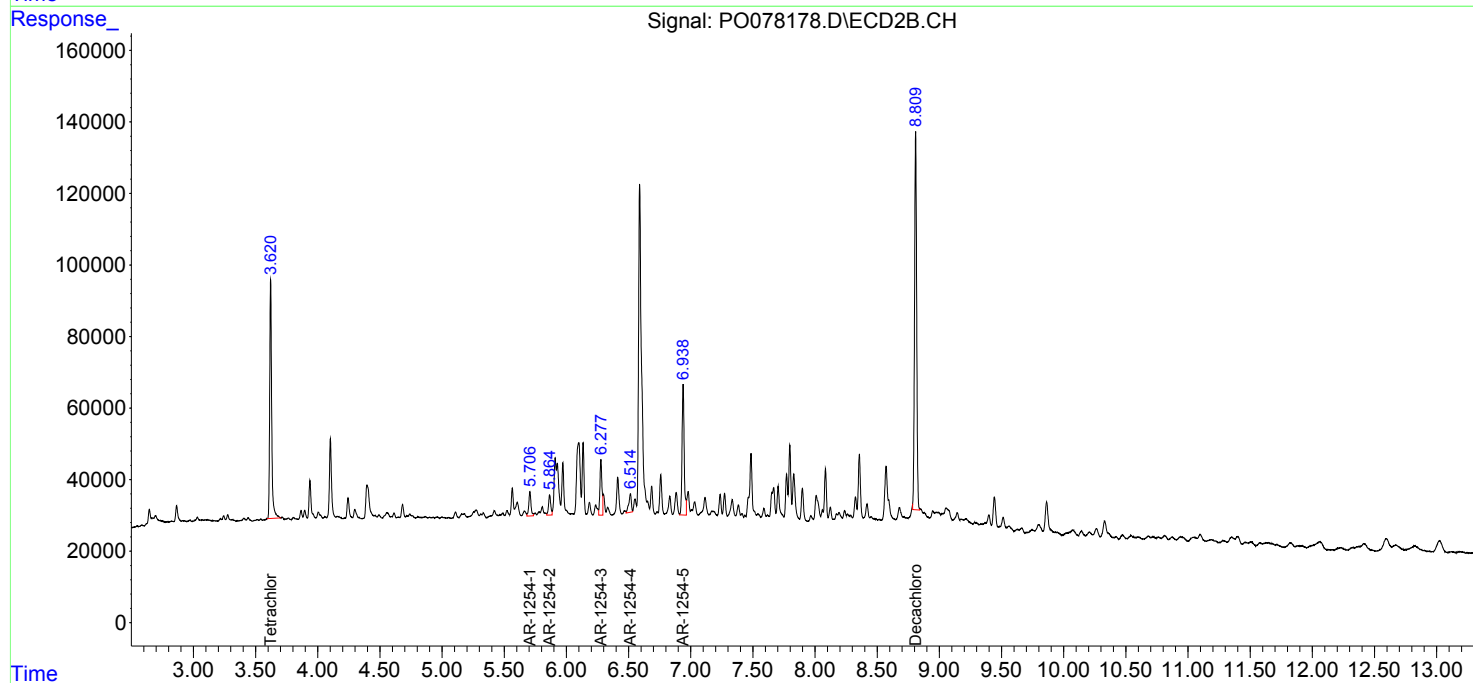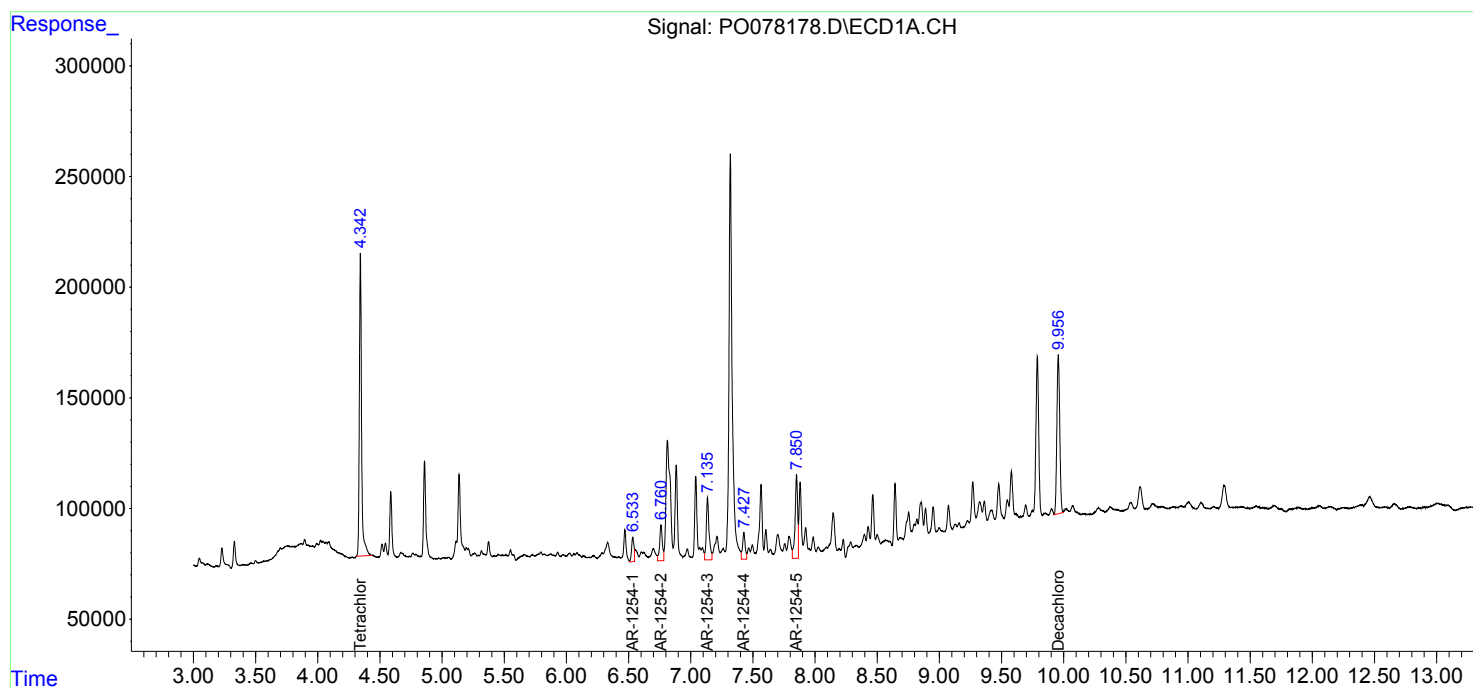

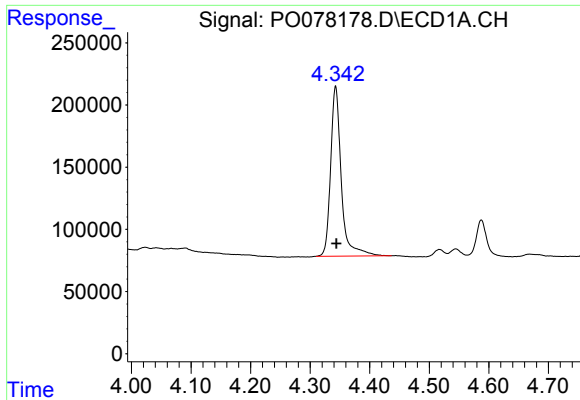


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1699133
Conc: 22.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
115


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:02 PM

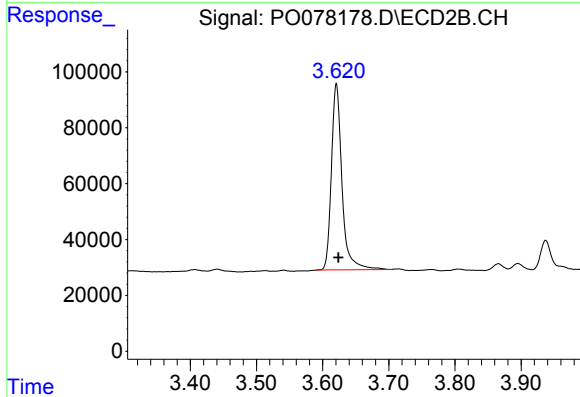


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 740429
Conc: 24.50 ng/ml

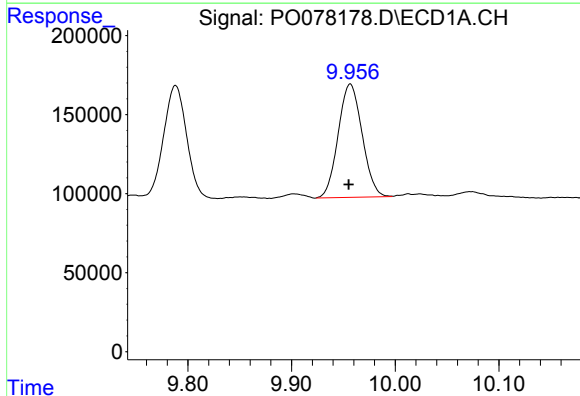


#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: 0.001 min
Response: 1149876
Conc: 23.26 ng/ml m

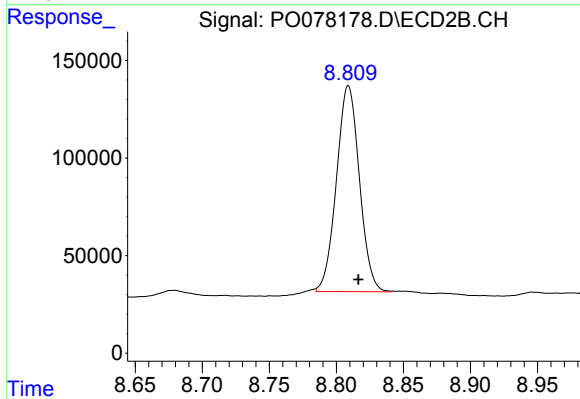

#2 Decachlorobiphenyl

R.T.: 8.809 min
Delta R.T.: -0.008 min
Response: 1253033
Conc: 43.09 ng/ml m

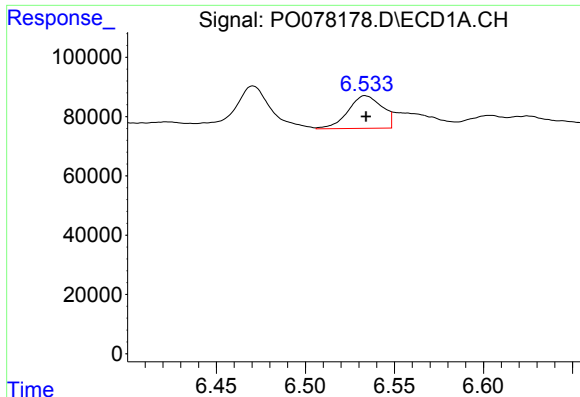


#26 AR-1254-1

R.T.: 6.533 min
Delta R.T.: -0.001 min
Response: 145713
Conc: 58.71 ng/ml m

Instrument :
ECD_O
ClientSampleId :
115


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:02 PM

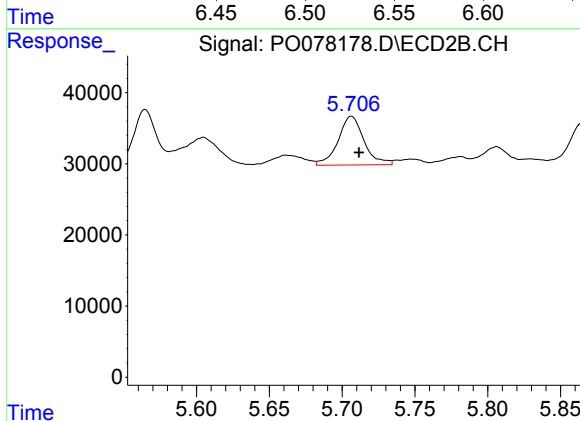


#26 AR-1254-1

R.T.: 5.706 min
Delta R.T.: -0.005 min
Response: 84725
Conc: 49.13 ng/ml

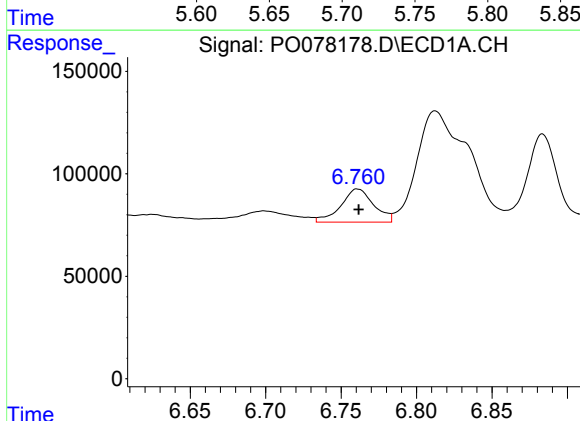


#27 AR-1254-2

R.T.: 6.760 min
Delta R.T.: -0.001 min
Response: 245809
Conc: 63.34 ng/ml

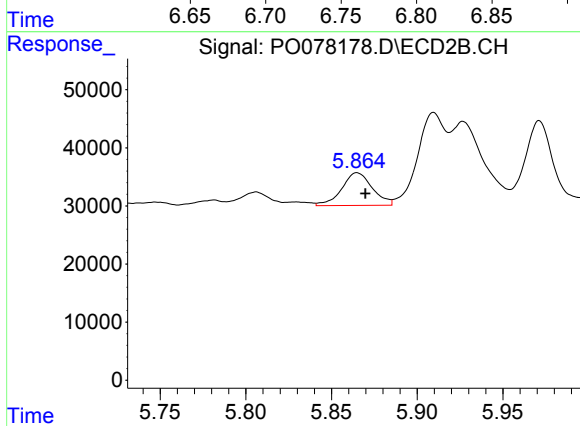

#27 AR-1254-2

R.T.: 5.865 min
Delta R.T.: -0.005 min
Response: 70150
Conc: 43.76 ng/ml

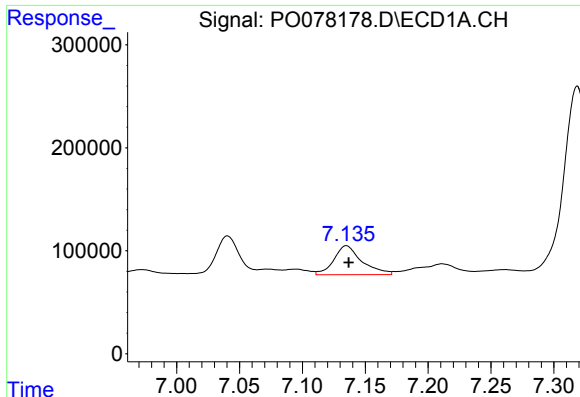


#28 AR-1254-3

R.T.: 7.135 min
Delta R.T.: -0.002 min
Response: 437693
Conc: 111.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
115


Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:02 PM

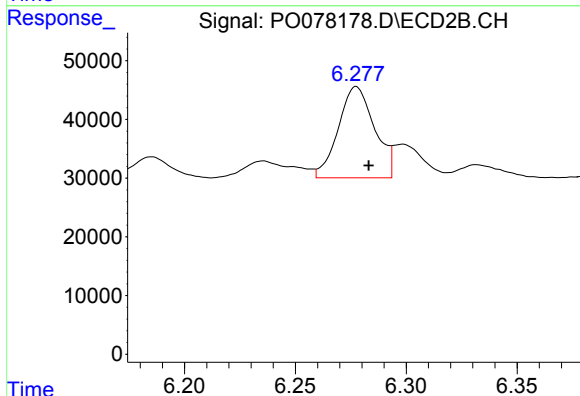


#28 AR-1254-3

R.T.: 6.278 min
Delta R.T.: -0.006 min
Response: 177003
Conc: 74.16 ng/ml

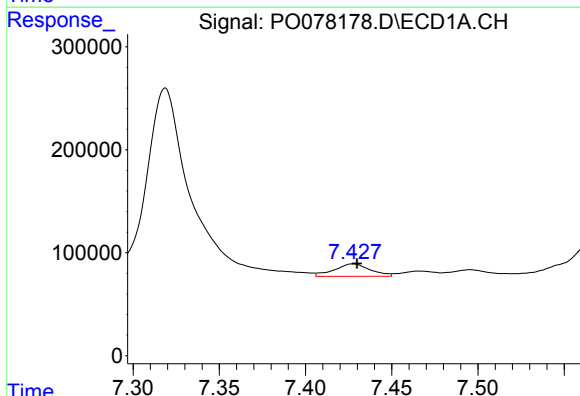


#29 AR-1254-4

R.T.: 7.428 min
Delta R.T.: -0.002 min
Response: 176006
Conc: 64.81 ng/ml

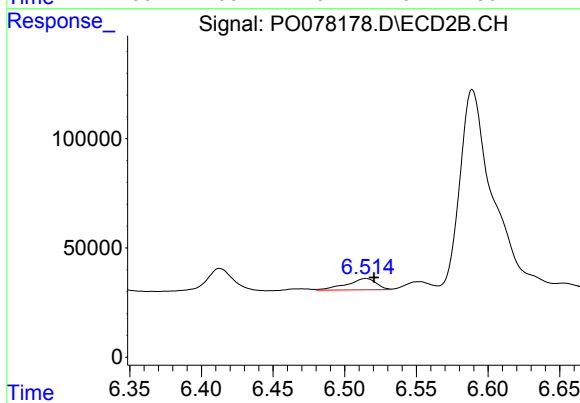

#29 AR-1254-4

R.T.: 6.515 min
Delta R.T.: -0.006 min
Response: 74367
Conc: 51.22 ng/ml

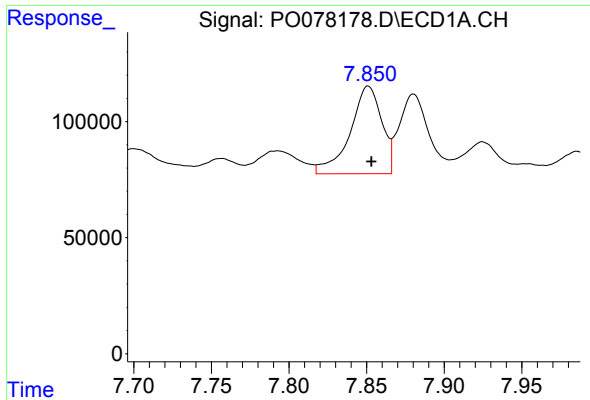


#30 AR-1254-5

R.T.: 7.851 min
Delta R.T.: -0.002 min
Response: 537032
Conc: 183.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
115

Manual Integrations
APPROVED

Ankita
5/27/2021 2:12:02 PM

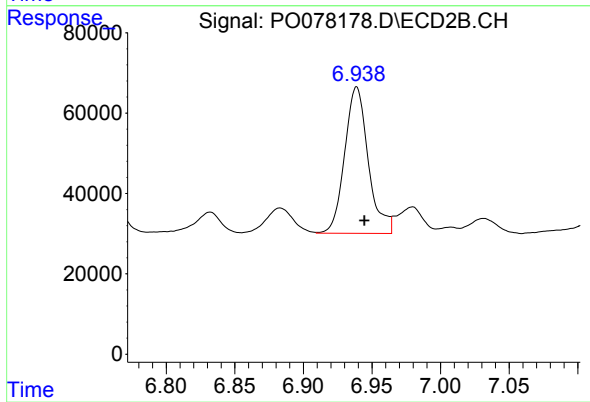

#30 AR-1254-5

R.T.: 6.939 min
Delta R.T.: -0.006 min
Response: 436811
Conc: 192.18 ng/ml