

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0052622\
 Data File : P0086613.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2022 11:36
 Operator : YP\AJ
 Sample : N2893-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 P004-SS003-0612-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/27/2022
 Supervised By :Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:23:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.476	3.672	2360311	969250	23.230	22.252
2) SA Decachlor...	10.323	8.719	1264950	747552	23.296	21.481
Target Compounds						
31) L7 AR-1260-1	7.275	6.263	195527	76745	64.607	39.431m#
32) L7 AR-1260-2	7.534	6.450	348759	199211	96.409	84.759m
33) L7 AR-1260-3	7.896	6.605	301526	109997	109.249	51.155m#
34) L7 AR-1260-4	8.124	7.078	274388	119757	81.325	66.508
35) L7 AR-1260-5	8.451	7.319	521687	324561	84.542	74.925

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052622\
Data File : P0086613.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2022 11:36
Operator : YP\AJ
Sample : N2893-07
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
P004-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:23:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

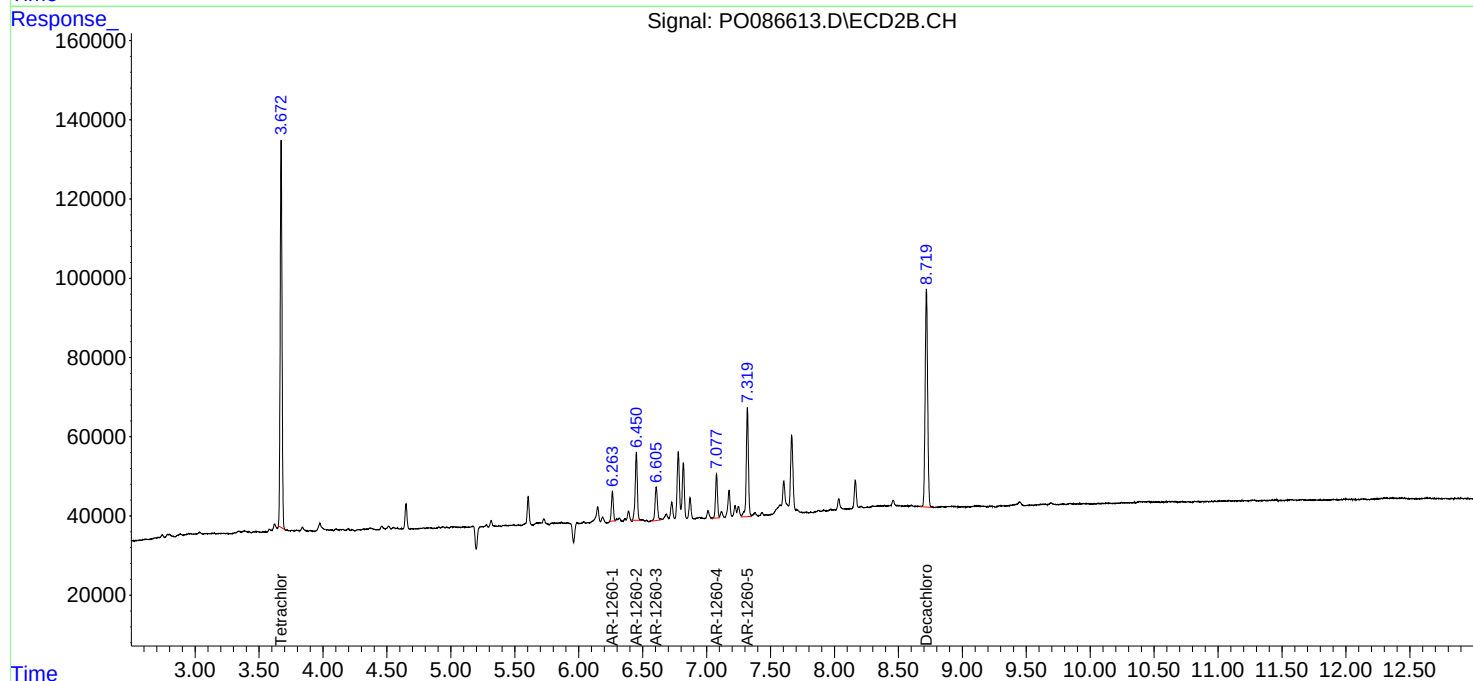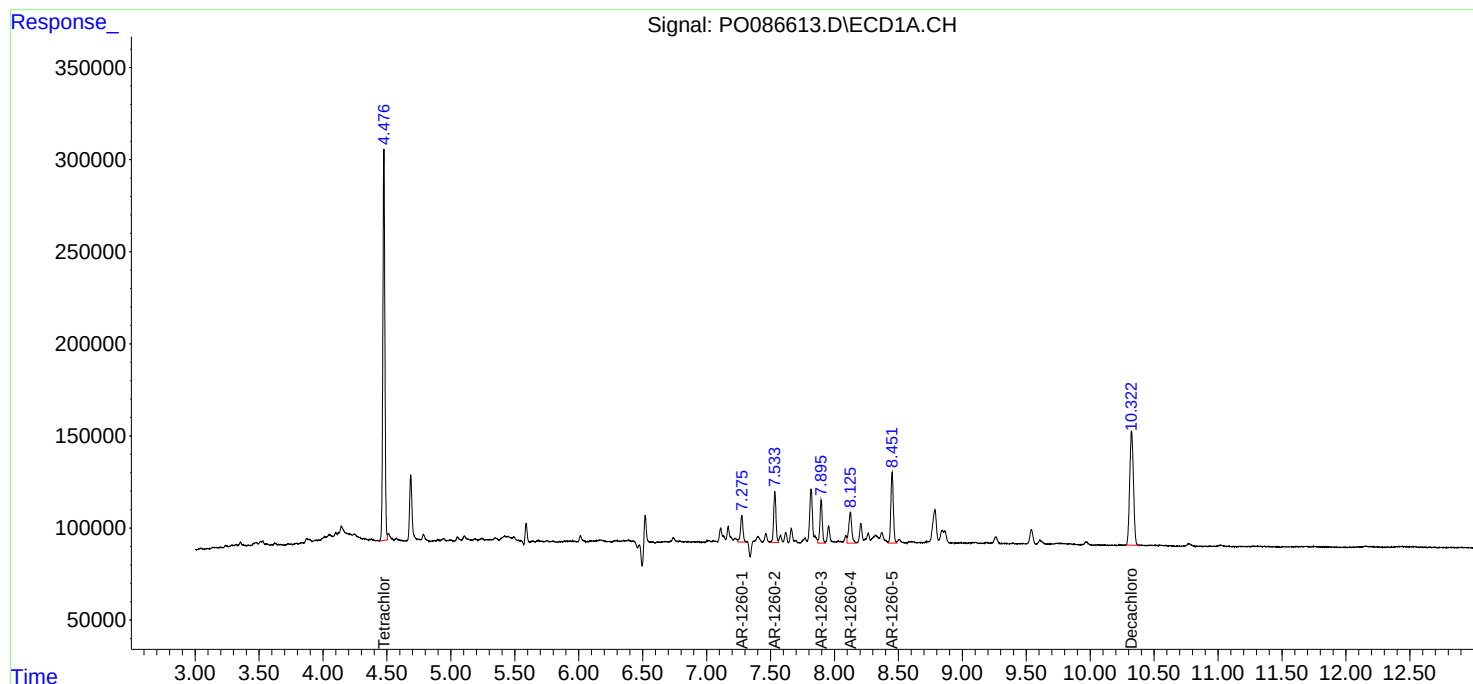

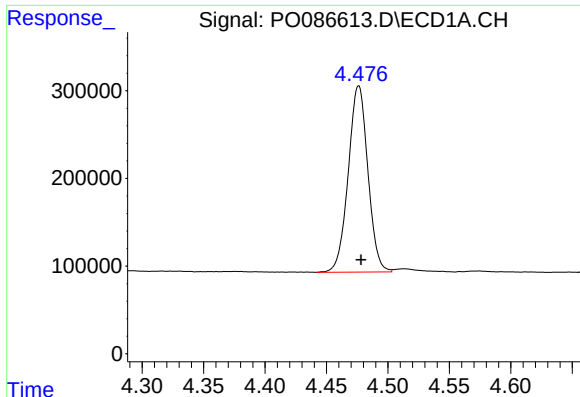


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.002 min
Response: 2360311
Conc: 23.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
P004-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

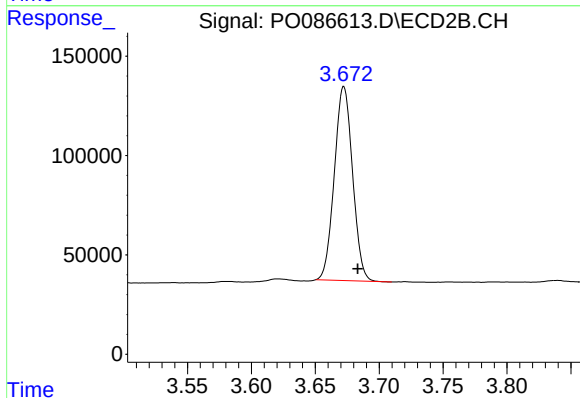


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.011 min
Response: 969250
Conc: 22.25 ng/ml

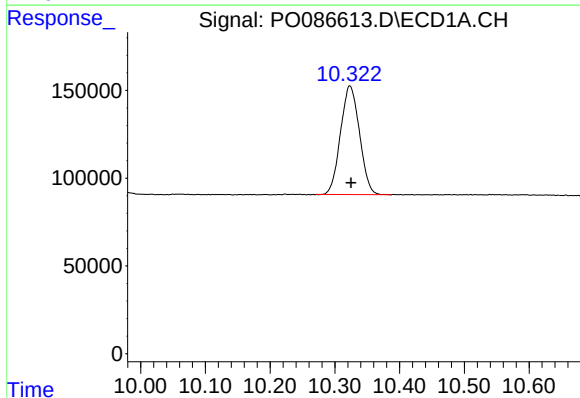


#2 Decachlorobiphenyl

R.T.: 10.323 min
Delta R.T.: -0.002 min
Response: 1264950
Conc: 23.30 ng/ml

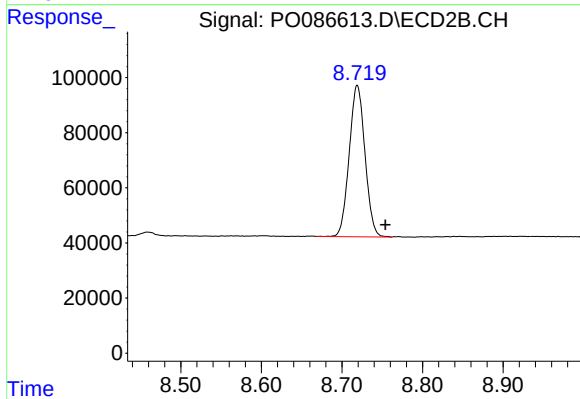

#2 Decachlorobiphenyl

R.T.: 8.719 min
Delta R.T.: -0.035 min
Response: 747552
Conc: 21.48 ng/ml

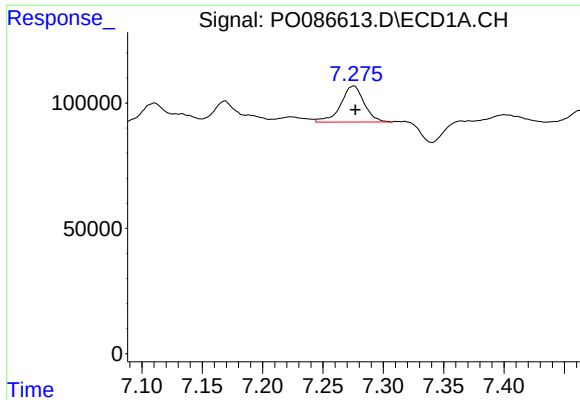


#31 AR-1260-1

R.T.: 7.275 min
Delta R.T.: -0.002 min
Response: 195527
Conc: 64.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
P004-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

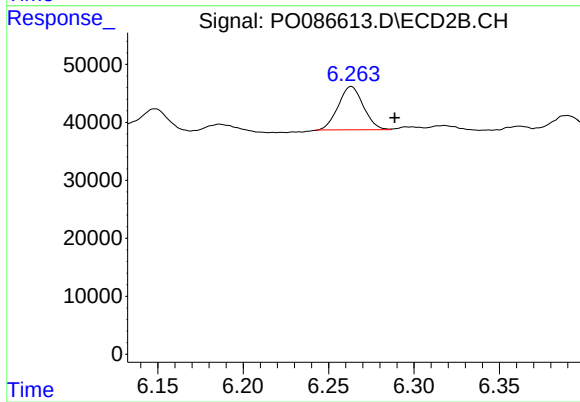


#31 AR-1260-1

R.T.: 6.263 min
Delta R.T.: -0.026 min
Response: 76745
Conc: 39.43 ng/ml m

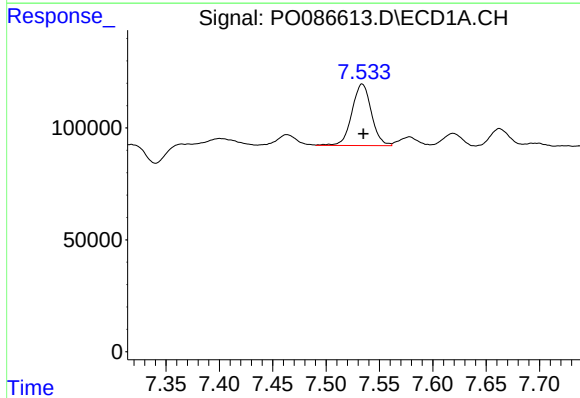


#32 AR-1260-2

R.T.: 7.534 min
Delta R.T.: 0.000 min
Response: 348759
Conc: 96.41 ng/ml

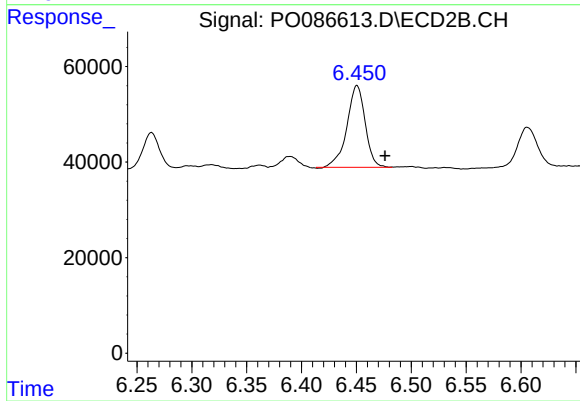

#32 AR-1260-2

R.T.: 6.450 min
Delta R.T.: -0.026 min
Response: 199211
Conc: 84.76 ng/ml m

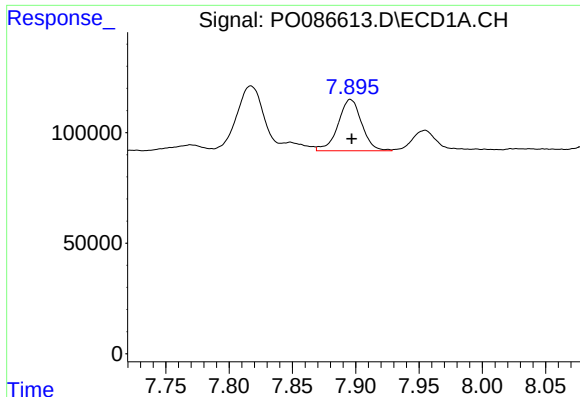


#33 AR-1260-3

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 301526
Conc: 109.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
P004-SS003-0612-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

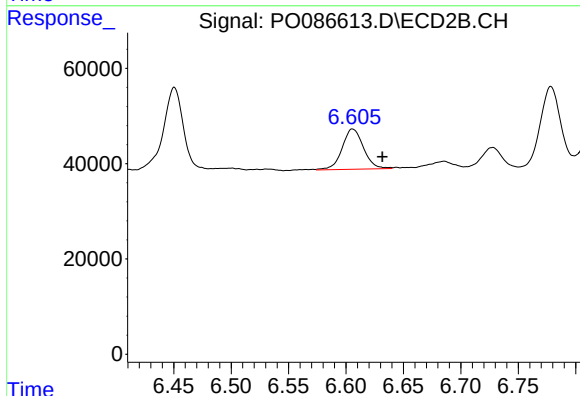


#33 AR-1260-3

R.T.: 6.605 min
Delta R.T.: -0.027 min
Response: 109997
Conc: 51.16 ng/ml m

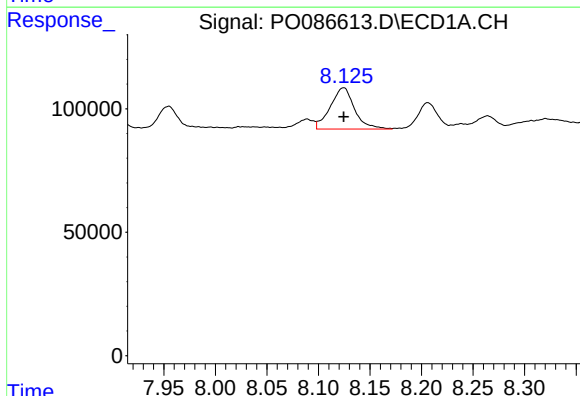


#34 AR-1260-4

R.T.: 8.124 min
Delta R.T.: 0.000 min
Response: 274388
Conc: 81.32 ng/ml

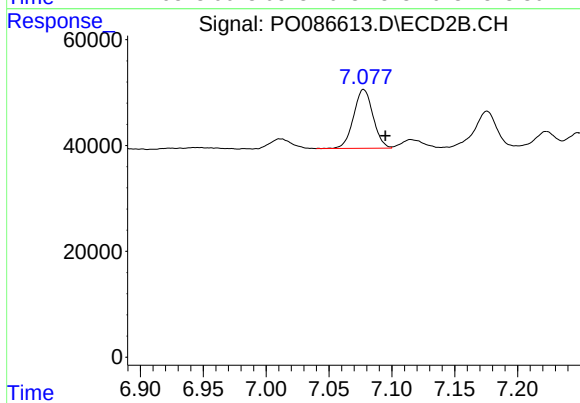

#34 AR-1260-4

R.T.: 7.078 min
Delta R.T.: -0.017 min
Response: 119757
Conc: 66.51 ng/ml

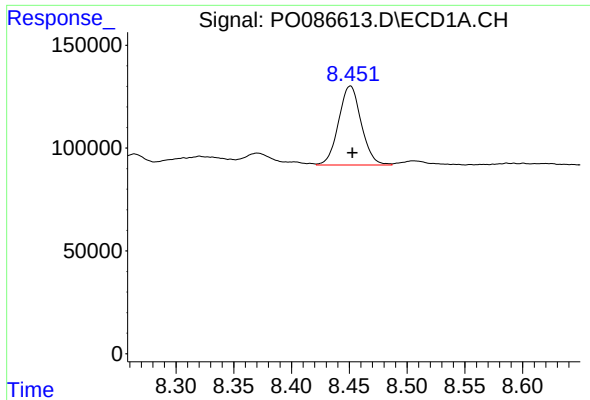


#35 AR-1260-5

R.T.: 8.451 min
Delta R.T.: -0.002 min
Response: 521687
Conc: 84.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
P004-SS003-0612-01

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/27/2022
Supervised By :Ankita Jodhani 05/27/2022

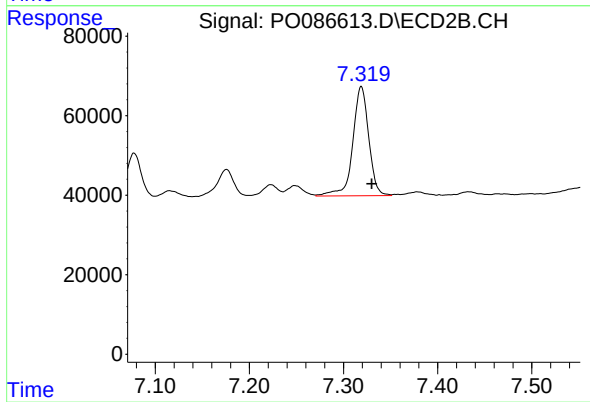

#35 AR-1260-5

R.T.: 7.319 min
Delta R.T.: -0.011 min
Response: 324561
Conc: 74.92 ng/ml