

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052622\
 Data File : P0086630.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 26 May 2022 16:14
 Operator : YP\AJ
 Sample : N3031-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-5-0524

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:37:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.477	3.672	2220399	910460	21.853	20.902
2)	SA Decachlor...	10.328	8.721	1397293	825201	25.733	23.712

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052622\
Data File : P0086630.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 May 2022 16:14
Operator : YP\AJ
Sample : N3031-01
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIPE-5-0524

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:37:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

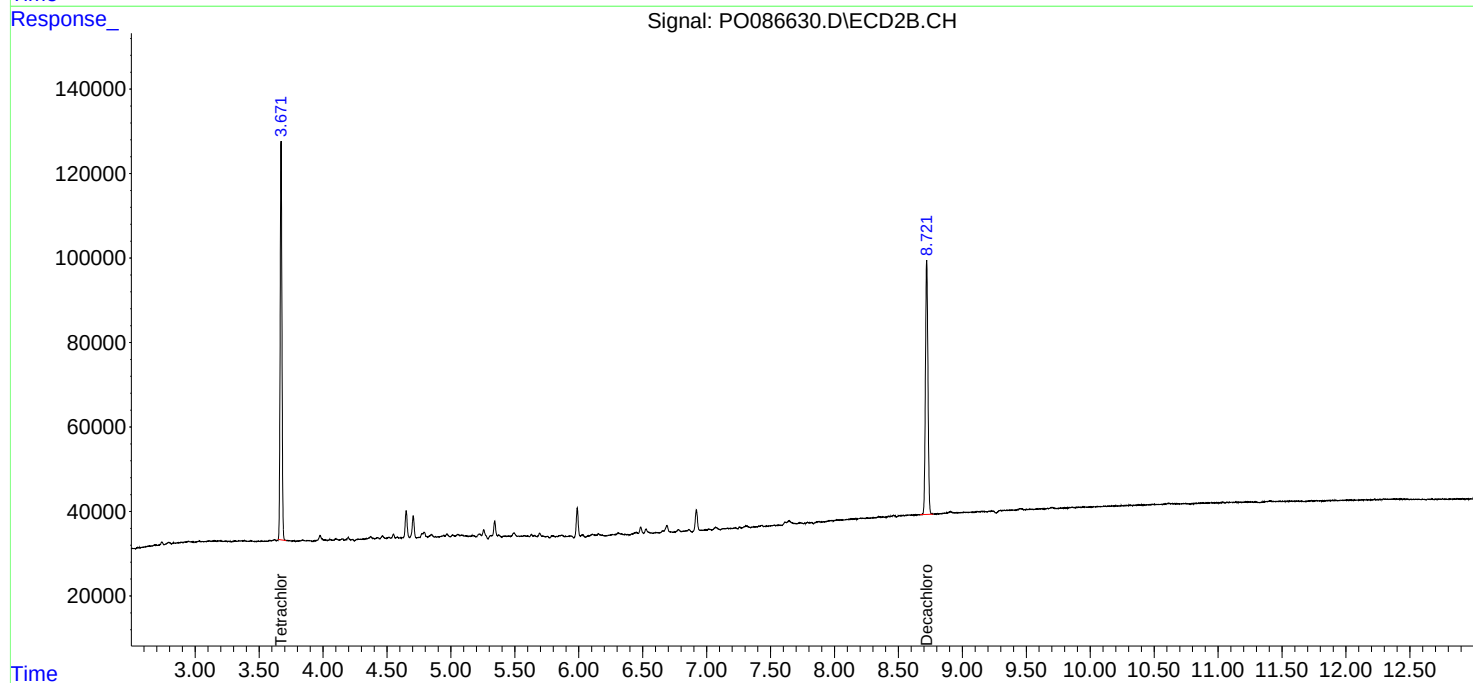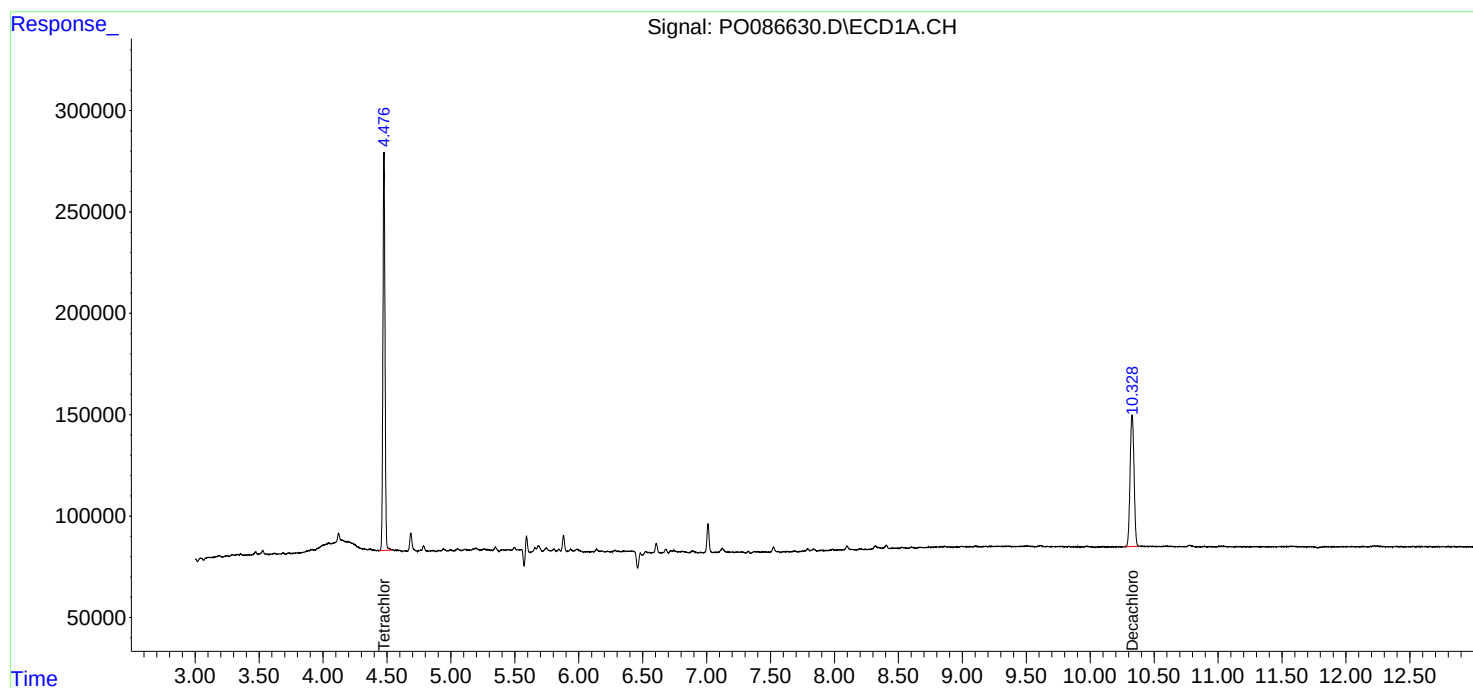


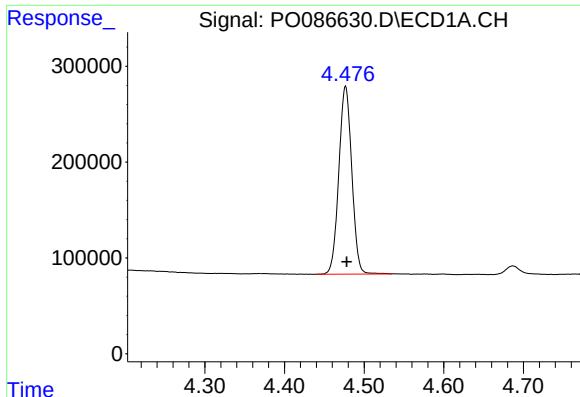

#1 Tetrachloro-m-xylene


R.T.: 4.477 min
Delta R.T.: -0.001 min
Response: 2220399
Conc: 21.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-5-0524

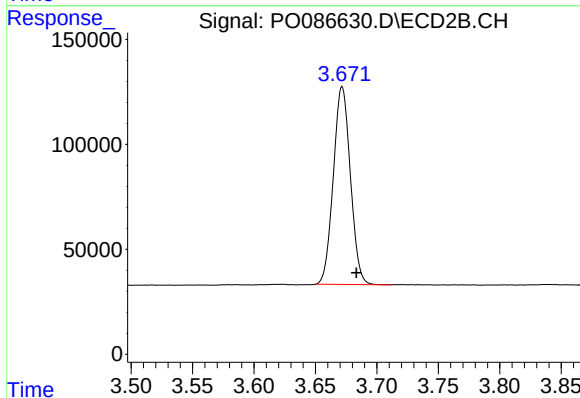


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.012 min
Response: 910460
Conc: 20.90 ng/ml

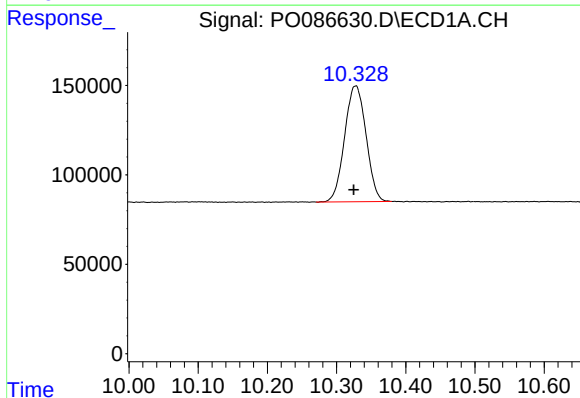

#2 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.003 min
Response: 1397293
Conc: 25.73 ng/ml

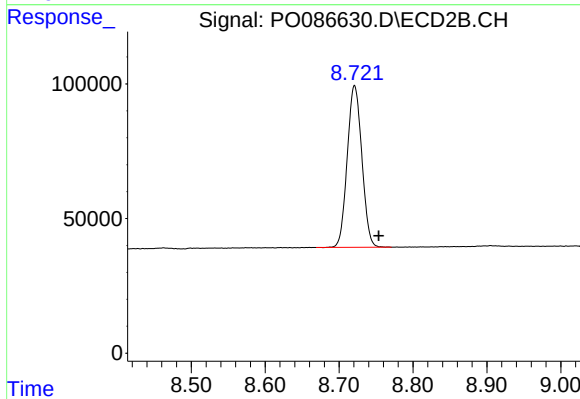

#2 Decachlorobiphenyl

R.T.: 8.721 min
Delta R.T.: -0.033 min
Response: 825201
Conc: 23.71 ng/ml