

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052624\
 Data File : P0104164.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2024 16:53
 Operator : YP/AJ
 Sample : P2615-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RBR251686

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:07:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 15:39:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.565	169.9E6	40973688	20.353m	18.379
2) SA Decachlor...	10.130	8.500	75306000	30401574	16.078	15.297

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052624\
Data File : PO104164.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2024 16:53
Operator : YP/AJ
Sample : P2615-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RBR251686


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:07:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 15:39:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

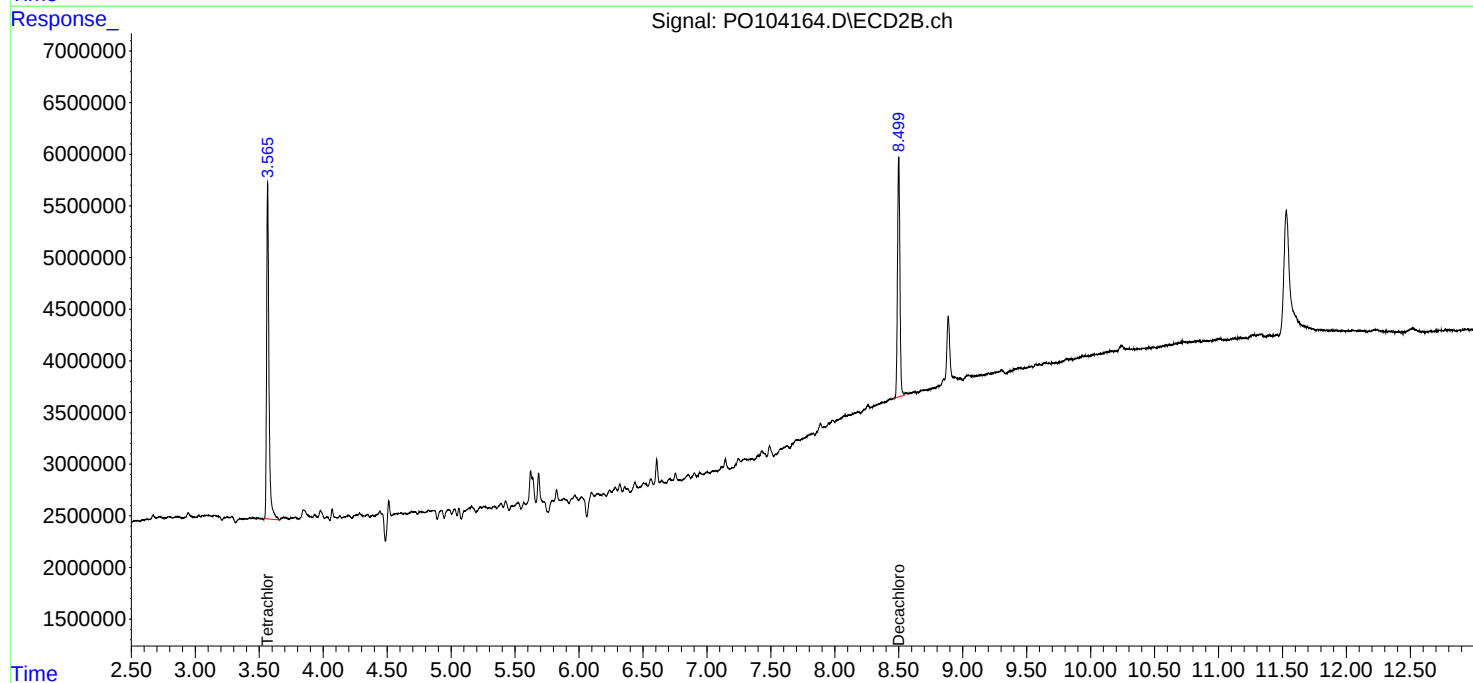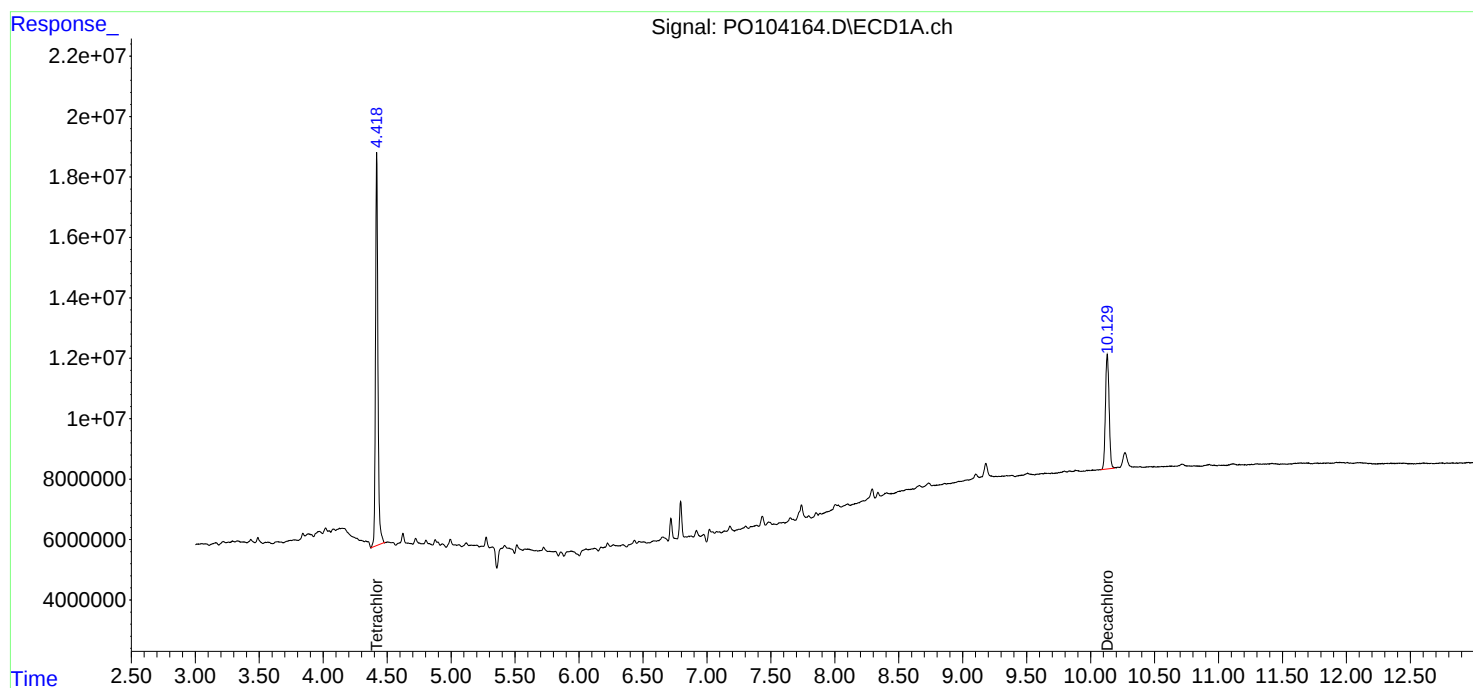

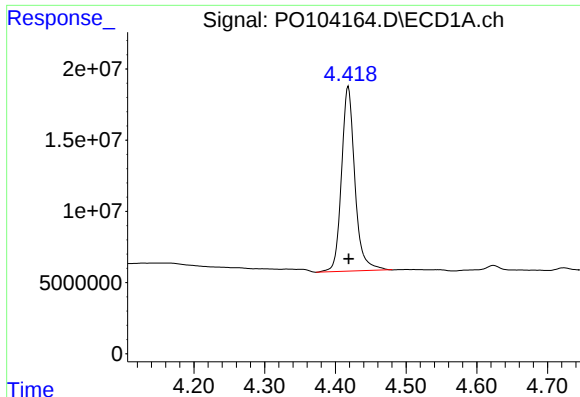


#1 Tetrachloro-m-xylene

R.T.: 4.418 min
Delta R.T.: -0.001 min
Response: 169926029
Conc: 20.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
RBR251686


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024

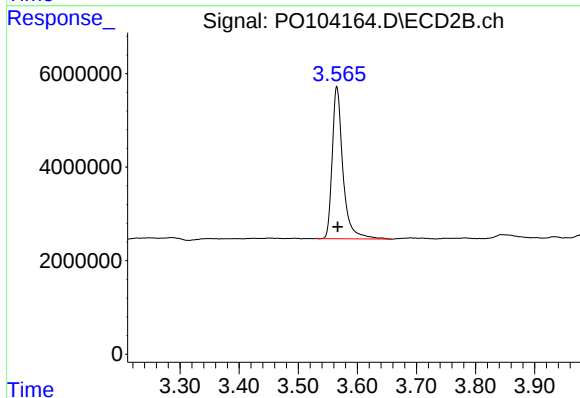


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.002 min
Response: 40973688
Conc: 18.38 ng/ml

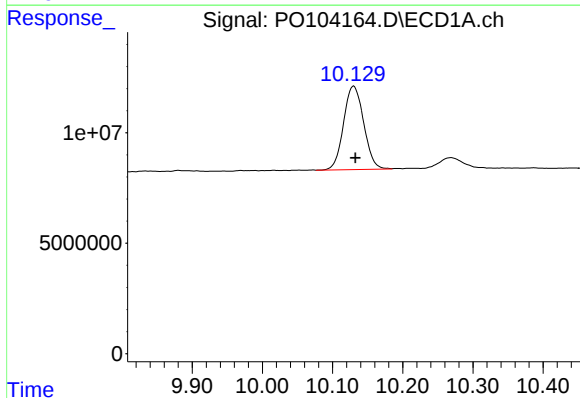

#2 Decachlorobiphenyl

R.T.: 10.130 min
Delta R.T.: -0.002 min
Response: 75306000
Conc: 16.08 ng/ml

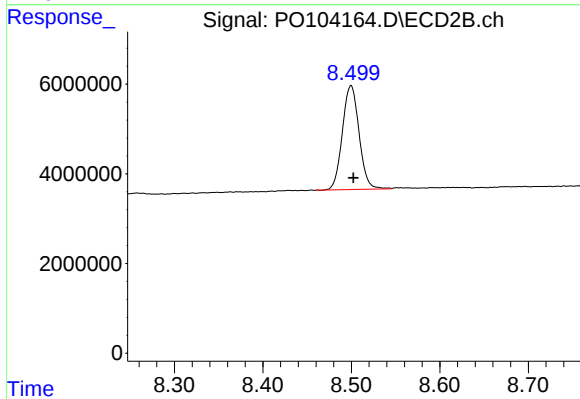

#2 Decachlorobiphenyl

R.T.: 8.500 min
Delta R.T.: -0.003 min
Response: 30401574
Conc: 15.30 ng/ml