

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052624\
 Data File : P0104166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 May 2024 17:27
 Operator : YP/AJ
 Sample : P2616-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 VNJ-206

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2024
 Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 01:07:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052424.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 15:39:50 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.566	172.5E6	43310882	20.661	19.427
2) SA Decachlor...	10.130	8.499	77390661	30284923	16.523m	15.238m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO052624\
Data File : PO104166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 May 2024 17:27
Operator : YP/AJ
Sample : P2616-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-206


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 01:07:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO052424.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 15:39:50 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

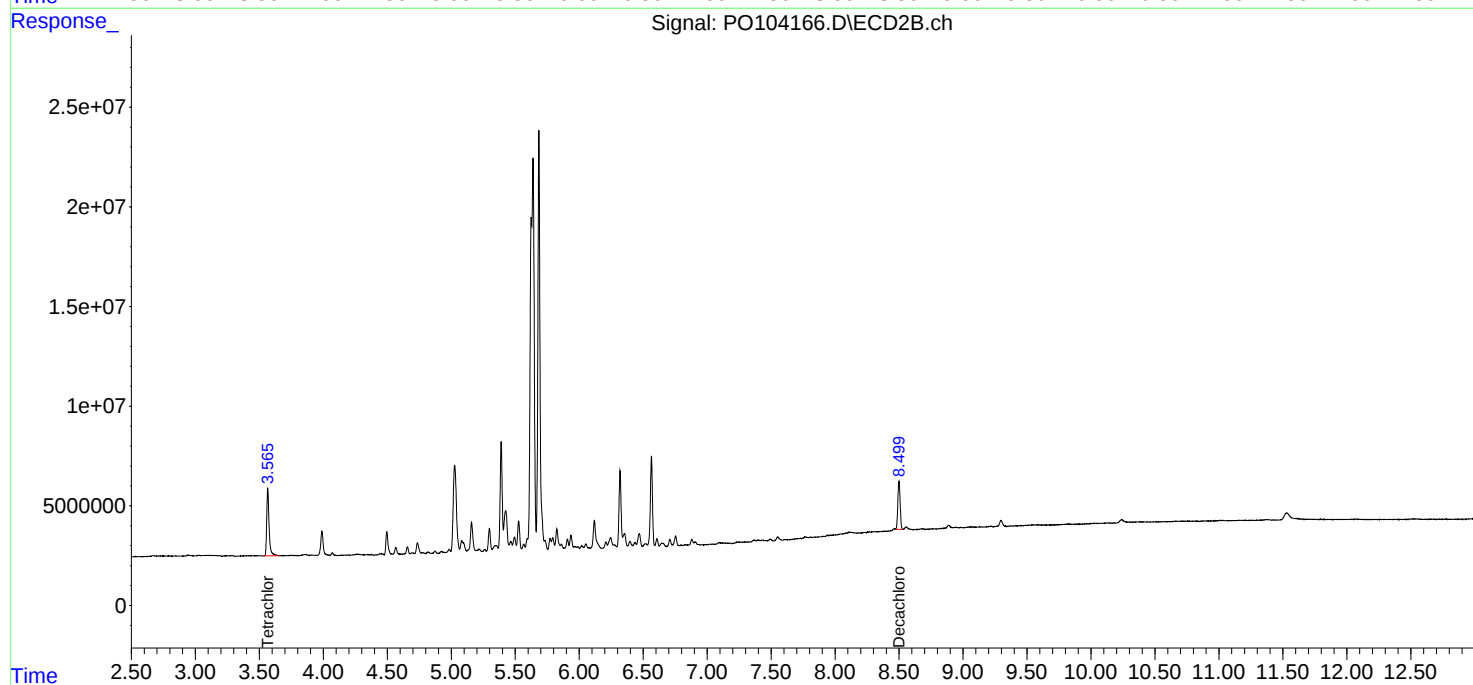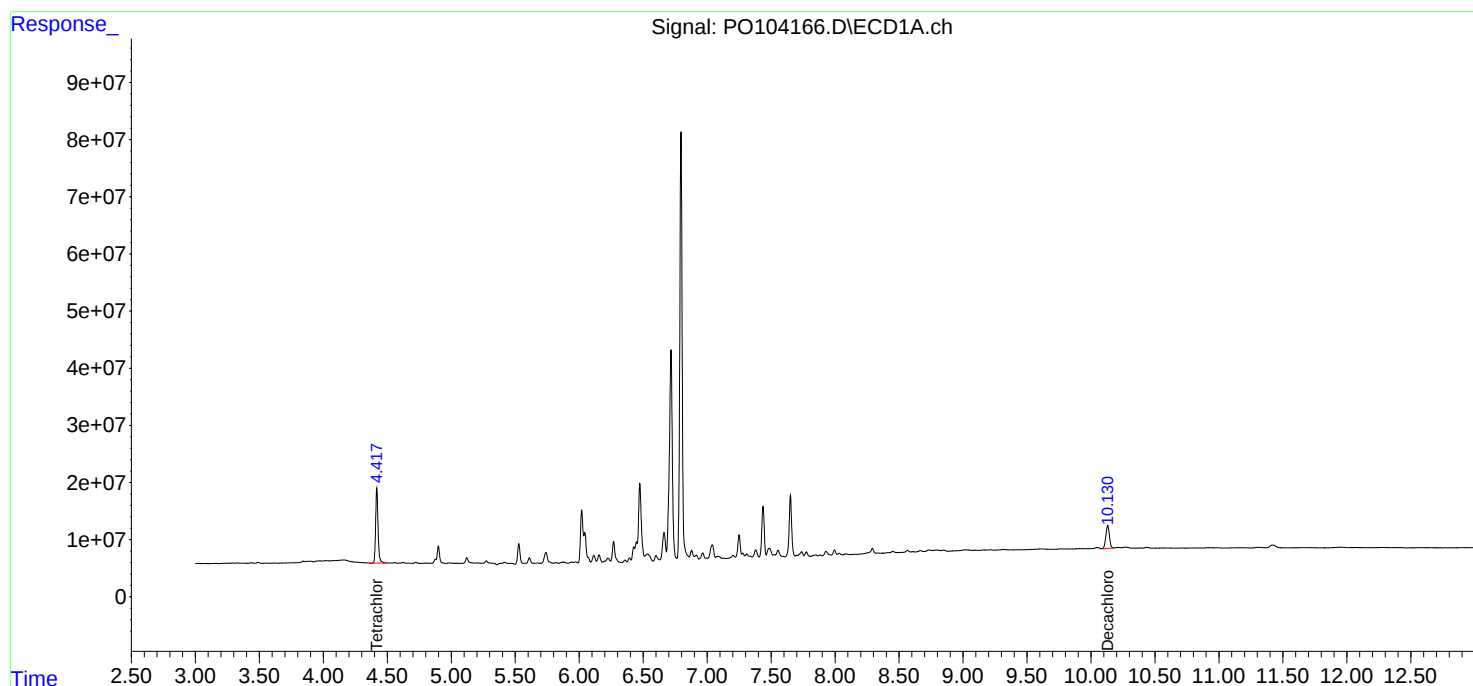

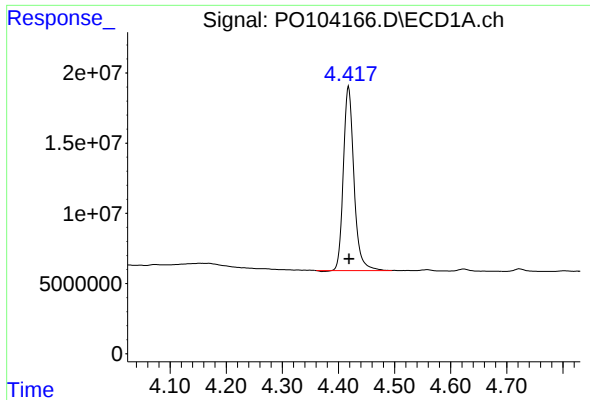


#1 Tetrachloro-m-xylene

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 172498616
Conc: 20.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-206


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2024
Supervised By :Ankita Jodhani 05/28/2024

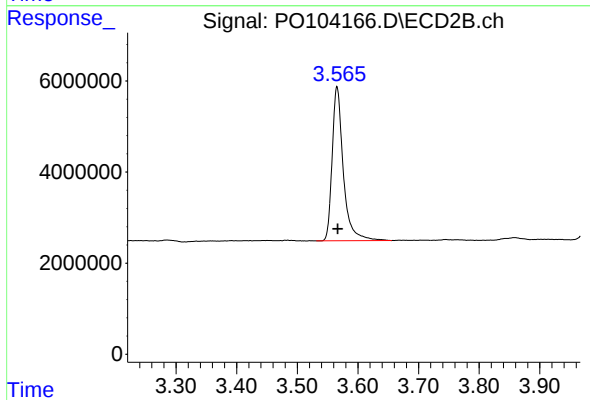


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: -0.001 min
Response: 43310882
Conc: 19.43 ng/ml

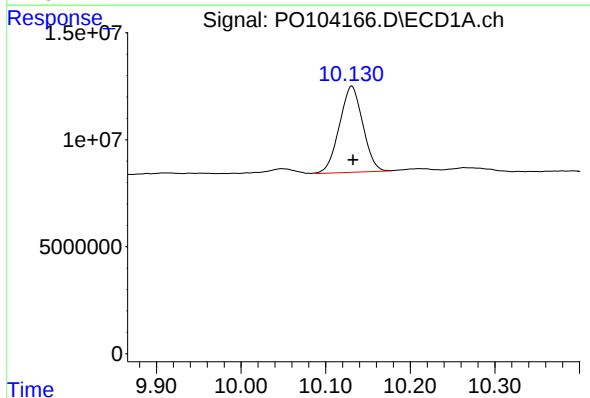

#2 Decachlorobiphenyl

R.T.: 10.130 min
Delta R.T.: -0.002 min
Response: 77390661
Conc: 16.52 ng/ml m

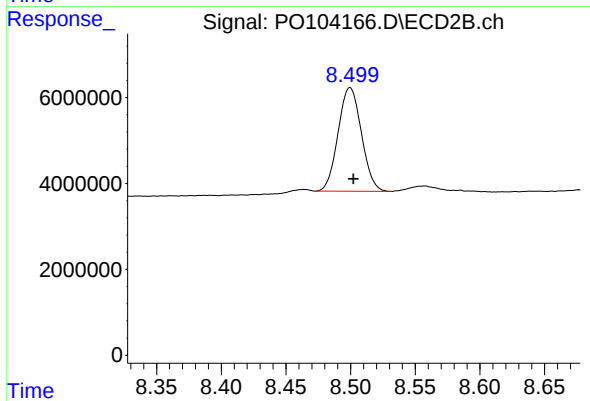

#2 Decachlorobiphenyl

R.T.: 8.499 min
Delta R.T.: -0.003 min
Response: 30284923
Conc: 15.24 ng/ml m