

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0052721\  
 Data File : P0078213.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 May 2021 15:00  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_0  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 27 16:54:54 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0051821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed May 19 06:28:32 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
-----						
System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.621	1346202	605022	18.215	20.023
2) SA Decachlor...	9.958	8.810	859512	512334	17.385	17.620

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_0\Data\P0052721\  
 Data File : P0078213.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 27 May 2021 15:00  
 Operator : DD\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampled :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: May 27 16:54:54 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_0\methods\P0051821.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed May 19 06:28:32 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

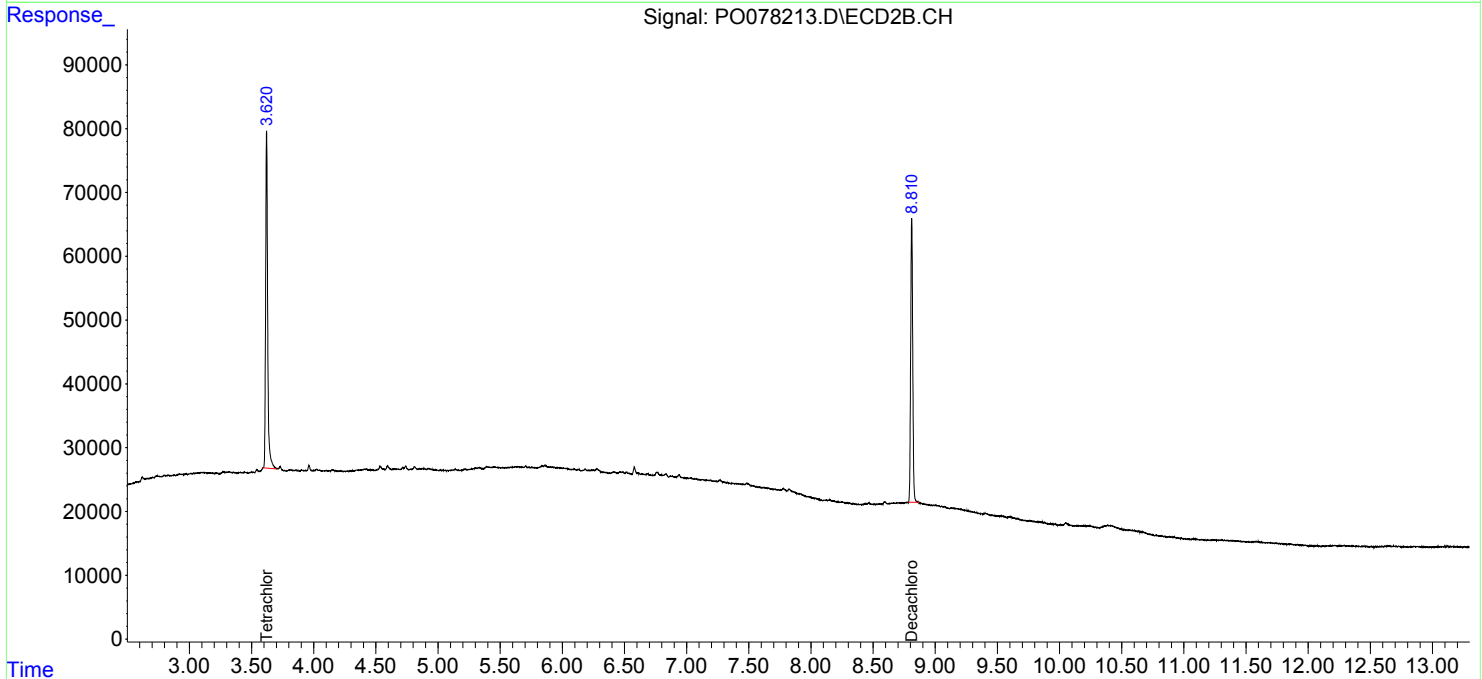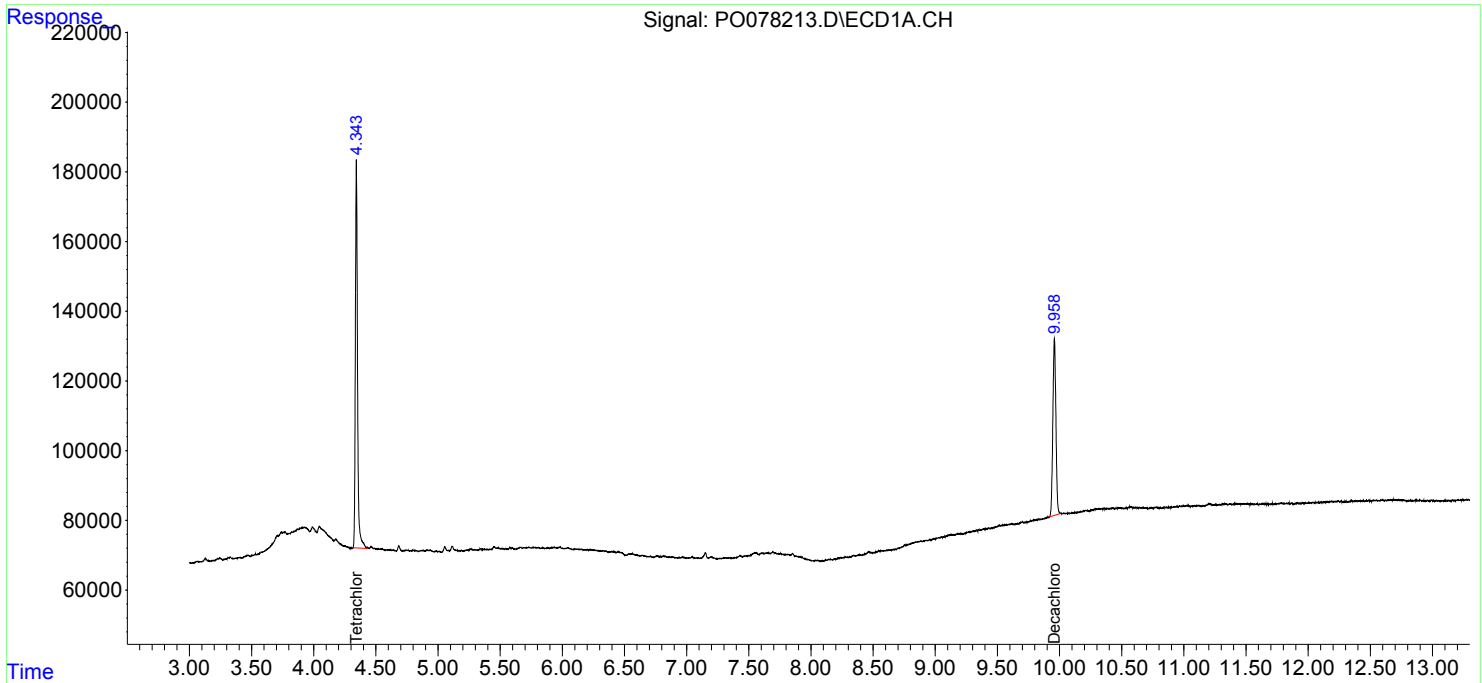

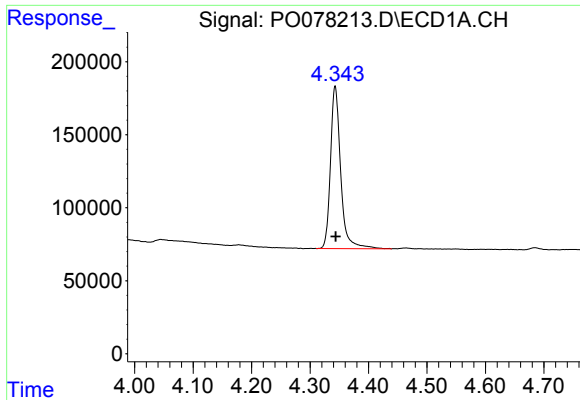


#1 Tetrachloro-m-xylene  
 R.T.: 4.343 min  
 Delta R.T.: 0.000 min  
 Response: 1346202  
 Conc: 18.21 ng/ml


Instrument :  
 ECD\_O  
 ClientSampleId :  
 I.BLK

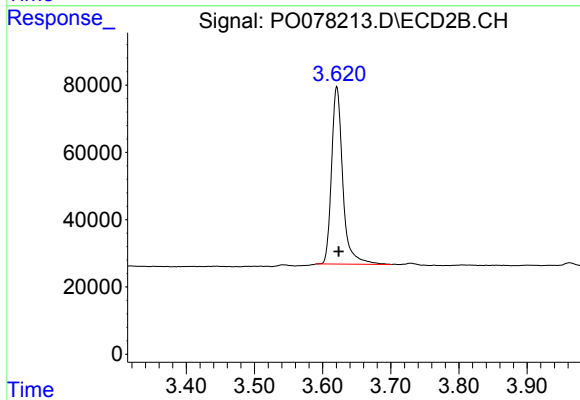

#1 Tetrachloro-m-xylene  
 R.T.: 3.621 min  
 Delta R.T.: -0.003 min  
 Response: 605022  
 Conc: 20.02 ng/ml

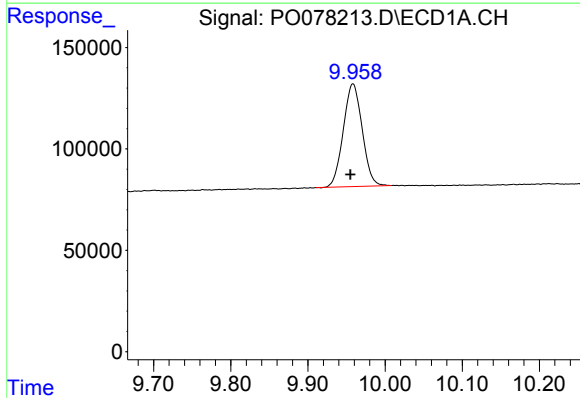

#2 Decachlorobiphenyl  
 R.T.: 9.958 min  
 Delta R.T.: 0.003 min  
 Response: 859512  
 Conc: 17.38 ng/ml

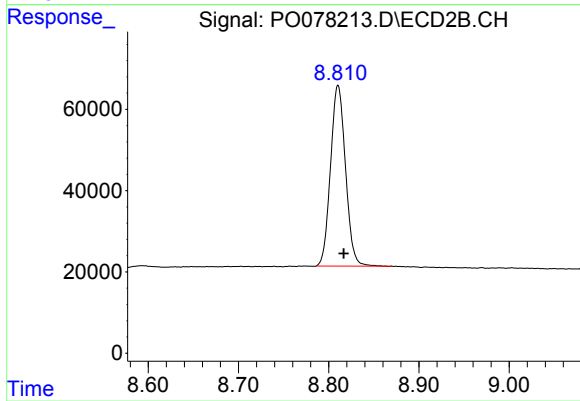

#2 Decachlorobiphenyl  
 R.T.: 8.810 min  
 Delta R.T.: -0.006 min  
 Response: 512334  
 Conc: 17.62 ng/ml