

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
 Data File : P0078215.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 15:35
 Operator : DD\AJ
 Sample : M2536-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-BPM-01-C7-C7A-D7-D7A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 16:55:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.621	1672597	782100	22.631	25.883
2) SA Decachlor...	9.958	8.811	1112820	660027	22.508	22.699

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
Data File : P0078215.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 15:35
Operator : DD\AJ
Sample : M2536-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-C7-C7A-D7-D7A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 16:55:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

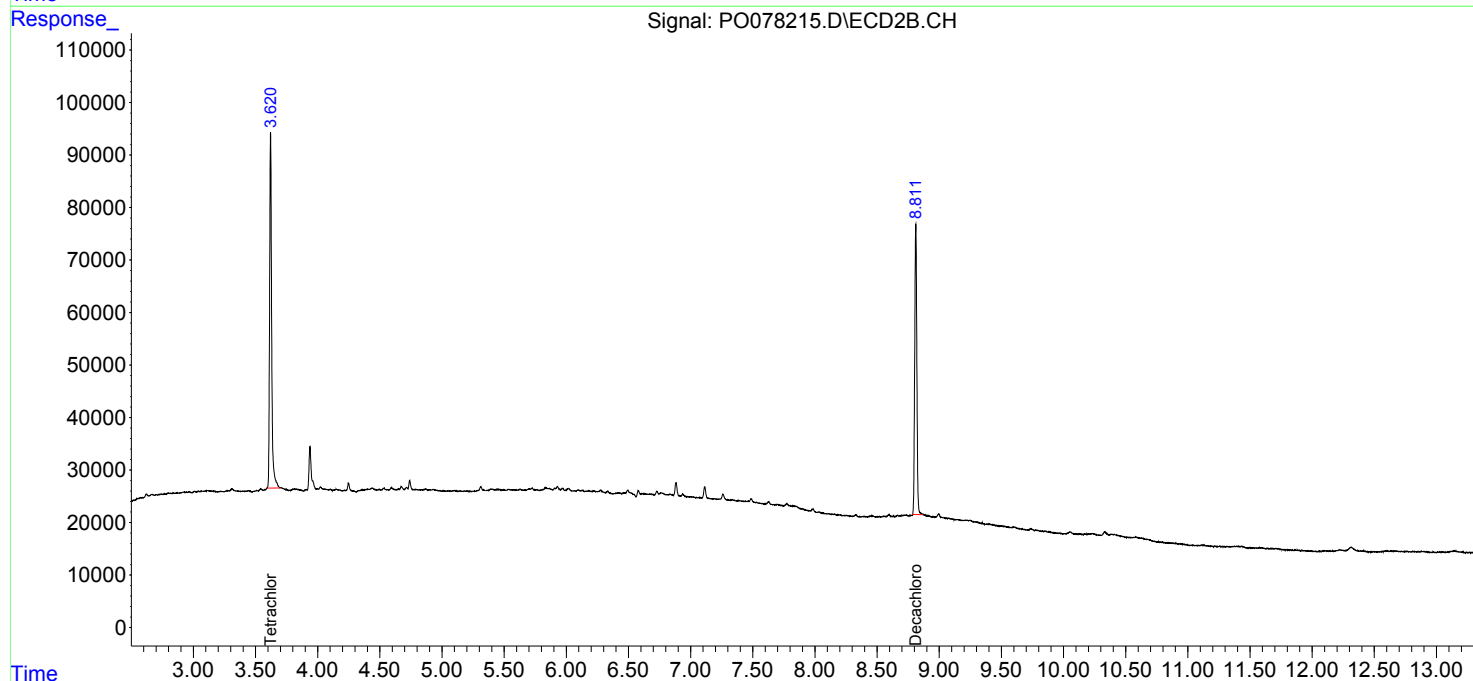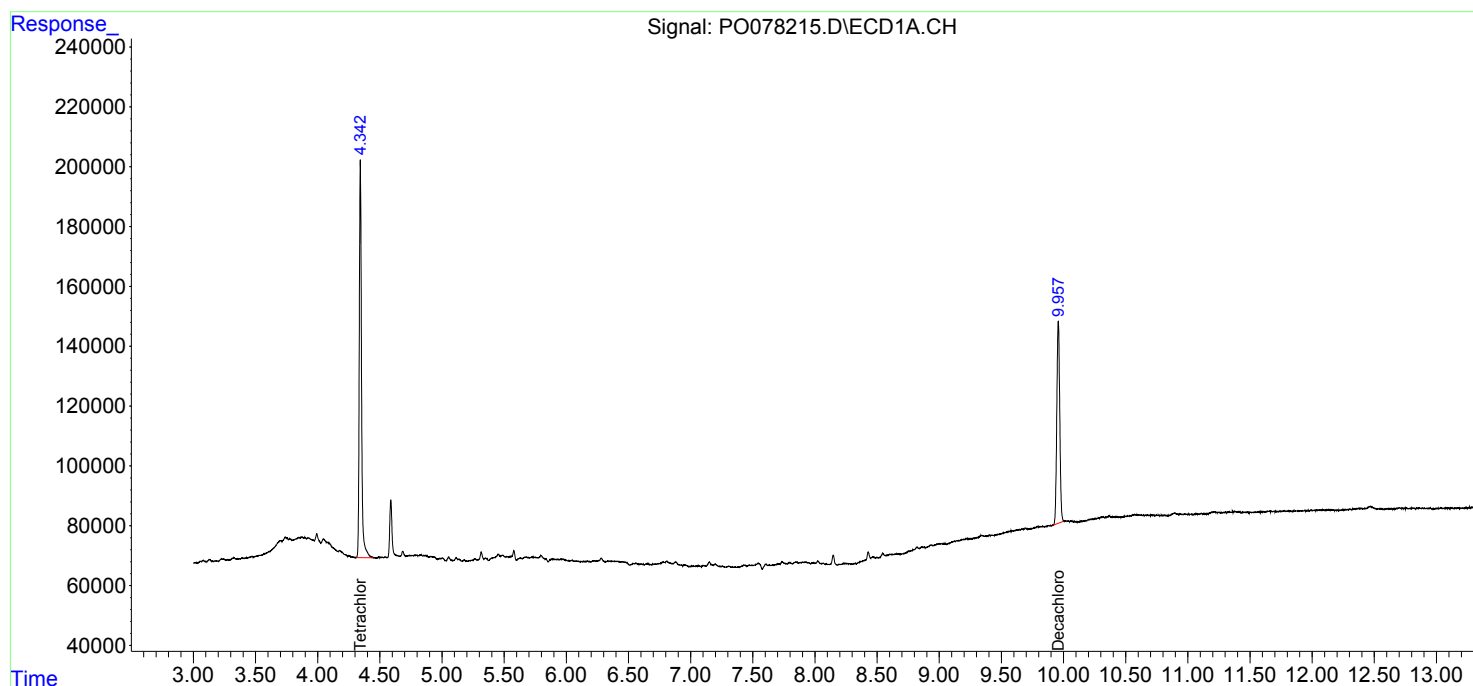


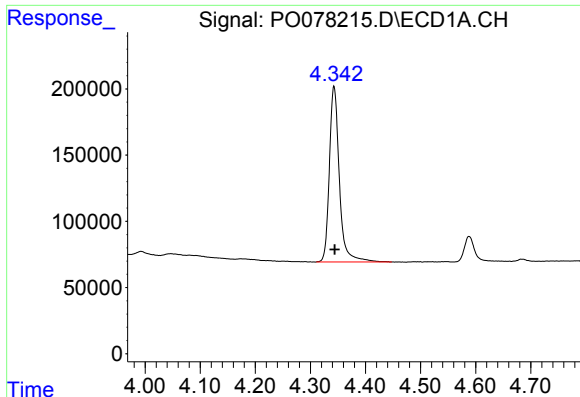

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.001 min
Response: 1672597
Conc: 22.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-BPM-01-C7-C7A-D7-D7A

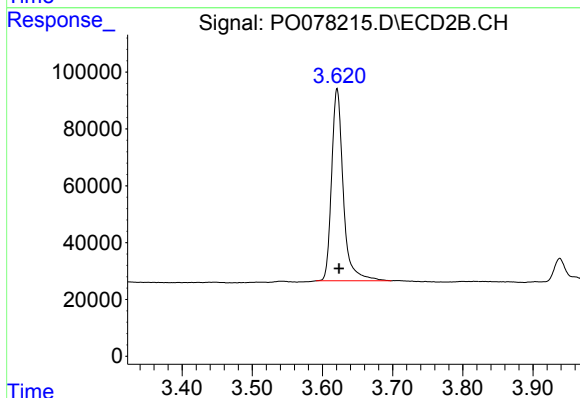


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.003 min
Response: 782100
Conc: 25.88 ng/ml

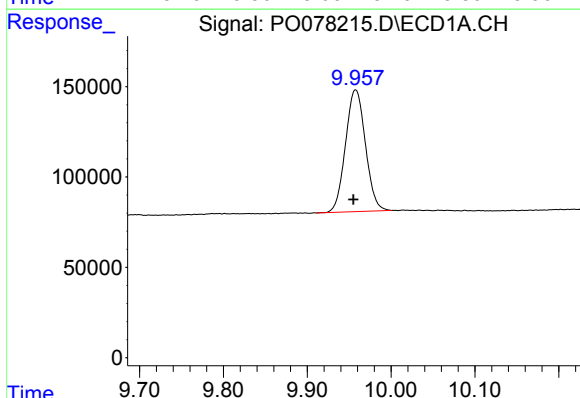

#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.002 min
Response: 1112820
Conc: 22.51 ng/ml

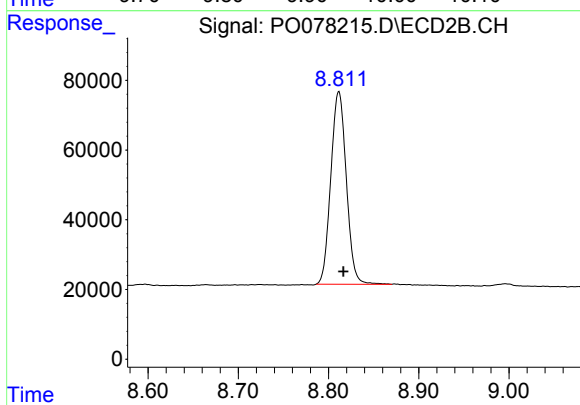

#2 Decachlorobiphenyl

R.T.: 8.811 min
Delta R.T.: -0.005 min
Response: 660027
Conc: 22.70 ng/ml