

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
 Data File : P0078220.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 17:01
 Operator : DD\AJ
 Sample : M2539-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-073

Manual Integrations
 APPROVED

Ankita
 5/28/2021 9:01:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 18:04:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.342	3.619	1462317	735000	19.786m	24.325m
2) SA Decachlor...	9.956	8.810	827561	476985	16.738	16.404

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
Data File : P0078220.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 17:01
Operator : DD\AJ
Sample : M2539-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
FK-PS-01-073


Manual Integrations
APPROVED

Ankita
5/28/2021 9:01:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 18:04:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

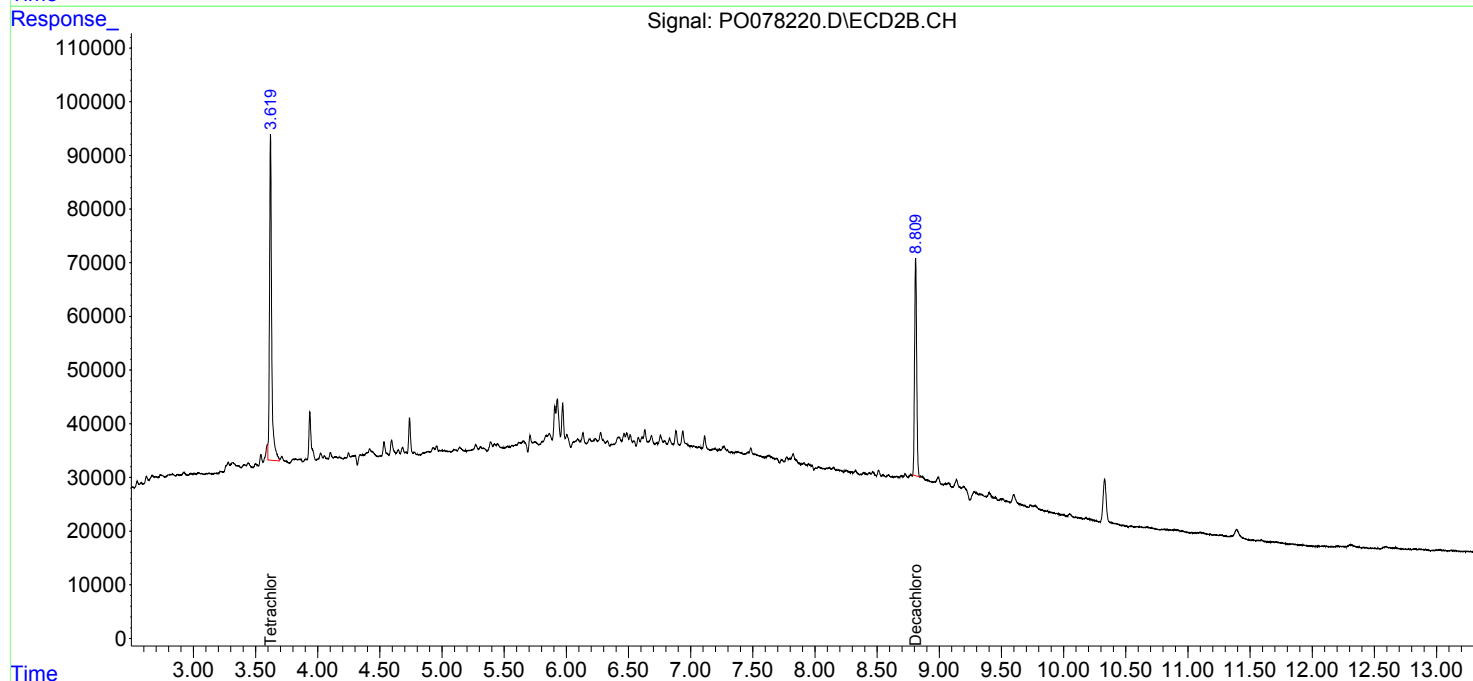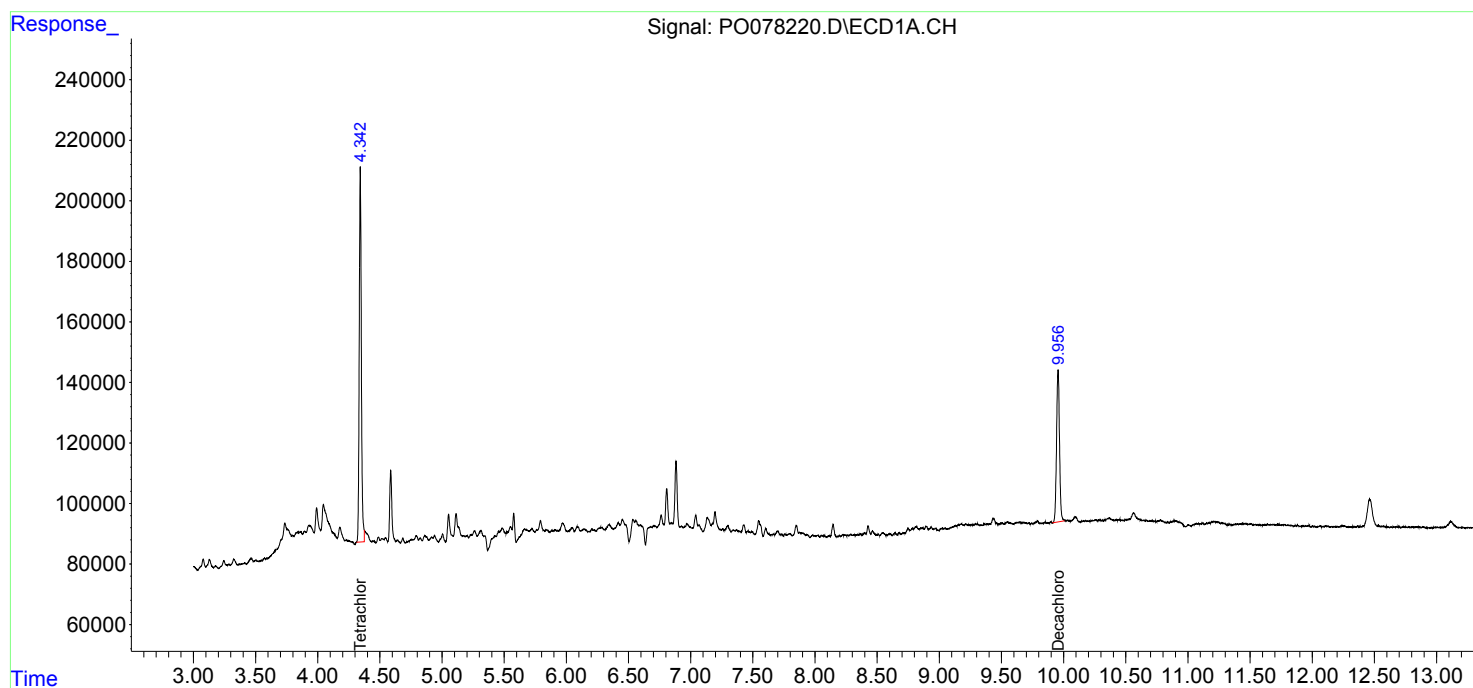

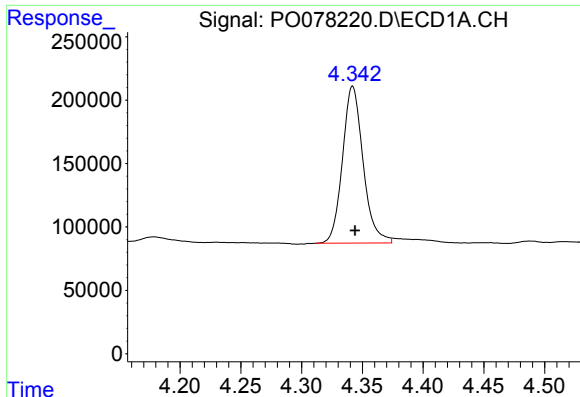


#1 Tetrachloro-m-xylene

R.T.: 4.342 min
Delta R.T.: -0.002 min
Response: 1462317
Conc: 19.79 ng/ml m

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-073


Manual Integrations
APPROVED

Ankita
5/28/2021 9:01:27 AM

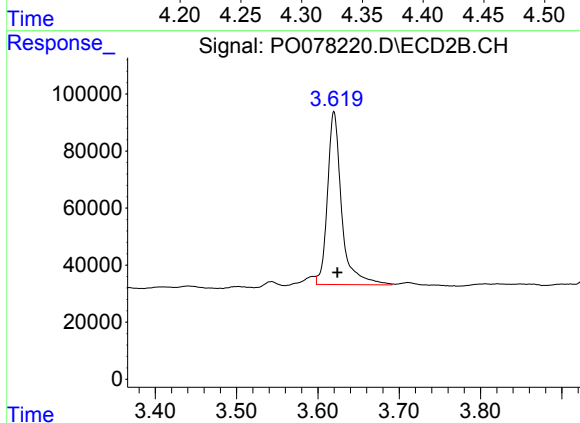


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.004 min
Response: 735000
Conc: 24.32 ng/ml m

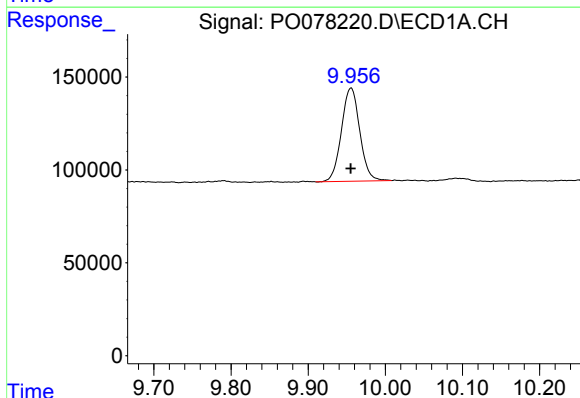

#2 Decachlorobiphenyl

R.T.: 9.956 min
Delta R.T.: 0.000 min
Response: 827561
Conc: 16.74 ng/ml

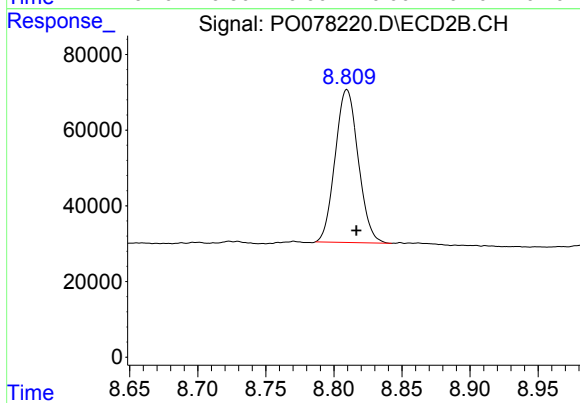

#2 Decachlorobiphenyl

R.T.: 8.810 min
Delta R.T.: -0.007 min
Response: 476985
Conc: 16.40 ng/ml