

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
 Data File : P0078237.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2021 22:29
 Operator : DD\AJ
 Sample : M2532-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-N-(MH-10.29)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 05:02:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.619	1717392	755696	23.237	25.010
2) SA Decachlor...	9.953	8.807	1130369	664014	22.863	22.836

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052721\
Data File : PO078237.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2021 22:29
Operator : DD\AJ
Sample : M2532-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-N-(MH-10.29)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 05:02:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

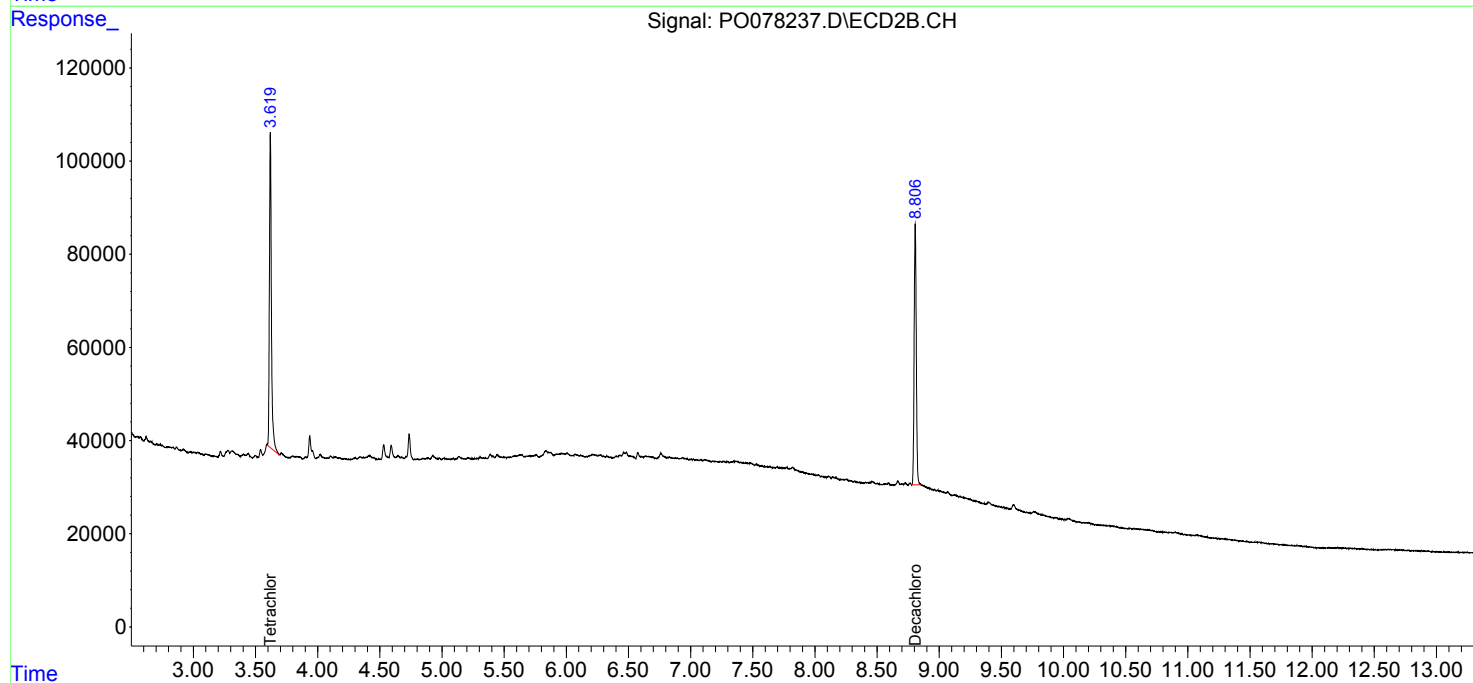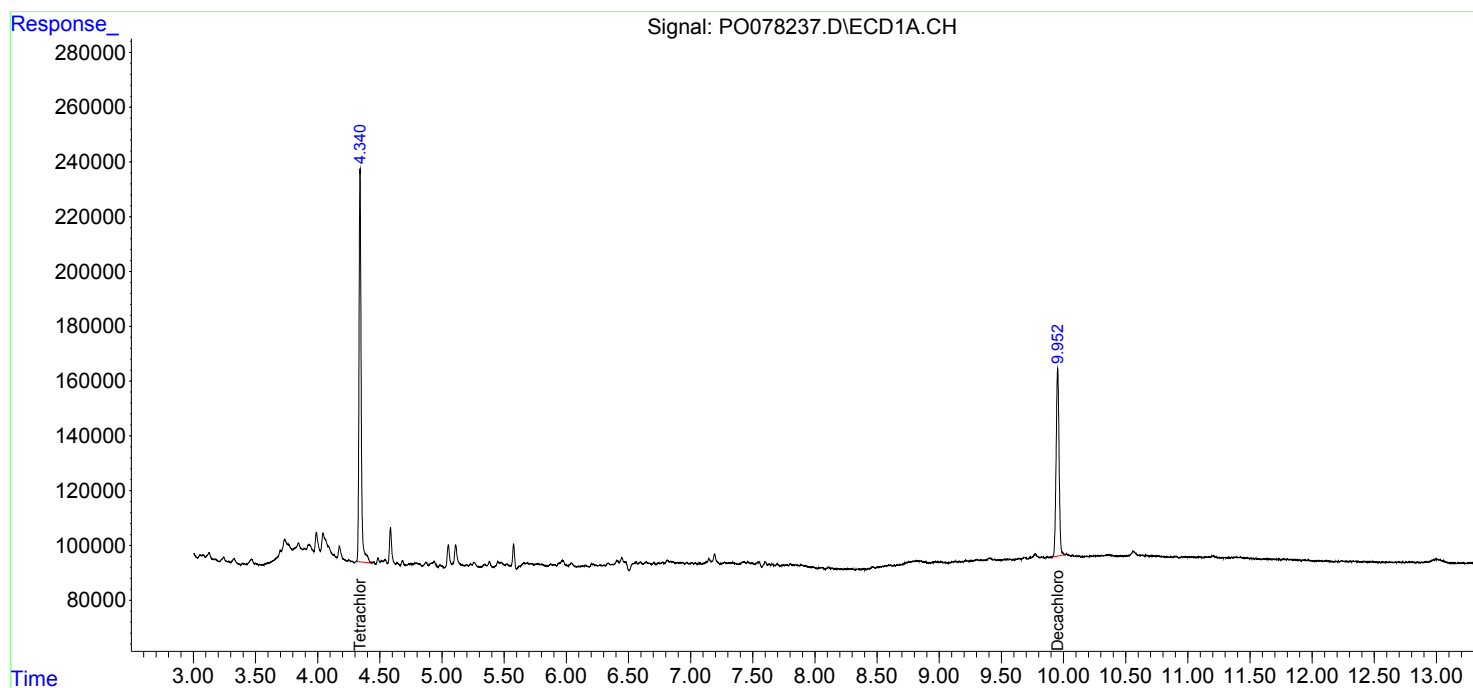


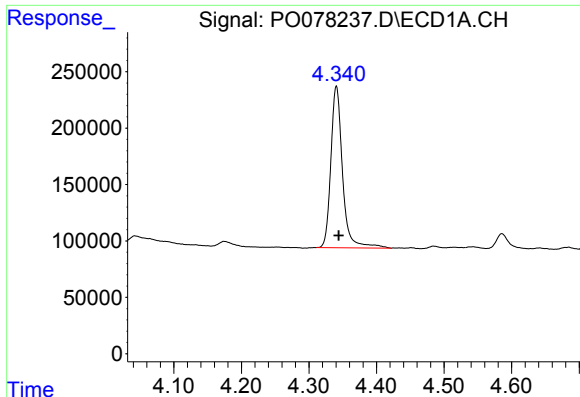

#1 Tetrachloro-m-xylene


R.T.: 4.341 min
Delta R.T.: -0.003 min
Response: 1717392
Conc: 23.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-N-(MH-10.29)

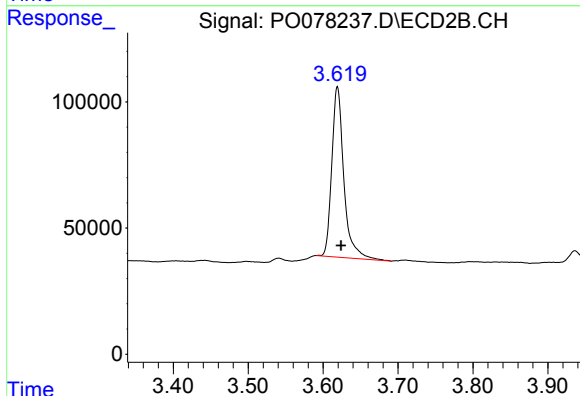


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: -0.005 min
Response: 755696
Conc: 25.01 ng/ml

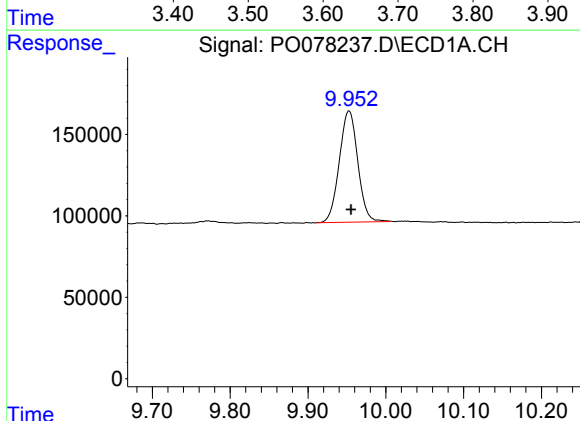

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: -0.002 min
Response: 1130369
Conc: 22.86 ng/ml

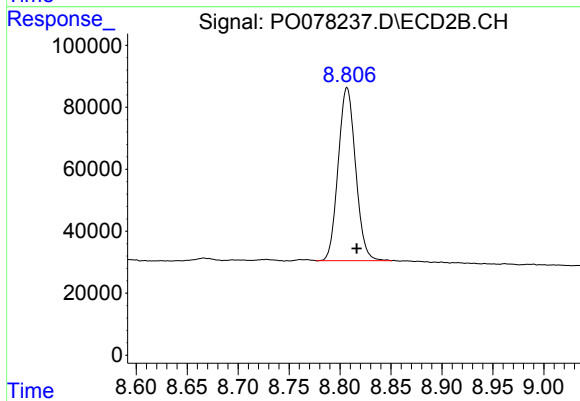

#2 Decachlorobiphenyl

R.T.: 8.807 min
Delta R.T.: -0.010 min
Response: 664014
Conc: 22.84 ng/ml