

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
 Data File : P0078242.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 May 2021 00:31
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 5/28/2021 9:01:43 AM

5/28/2021 9:01:43 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 28 04:39:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.617	1384682	607607	18.735	20.109
2) SA Decachlor...	9.951	8.805	944600	586725	19.106	20.178m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052721\
Data File : P0078242.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 May 2021 00:31
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK



Manual Integrations
APPROVED


Ankita
5/28/2021 9:01:43 AM

5/28/2021 9:01:43 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 04:39:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

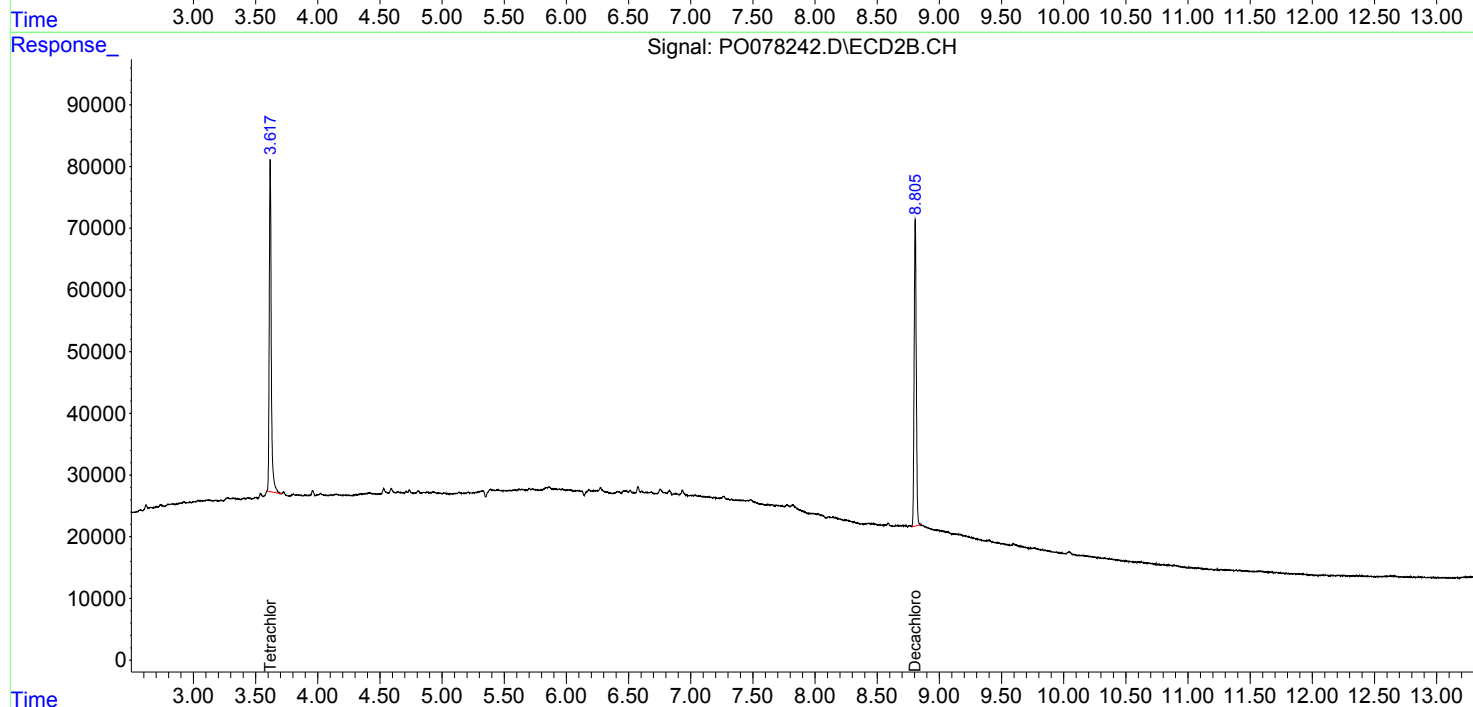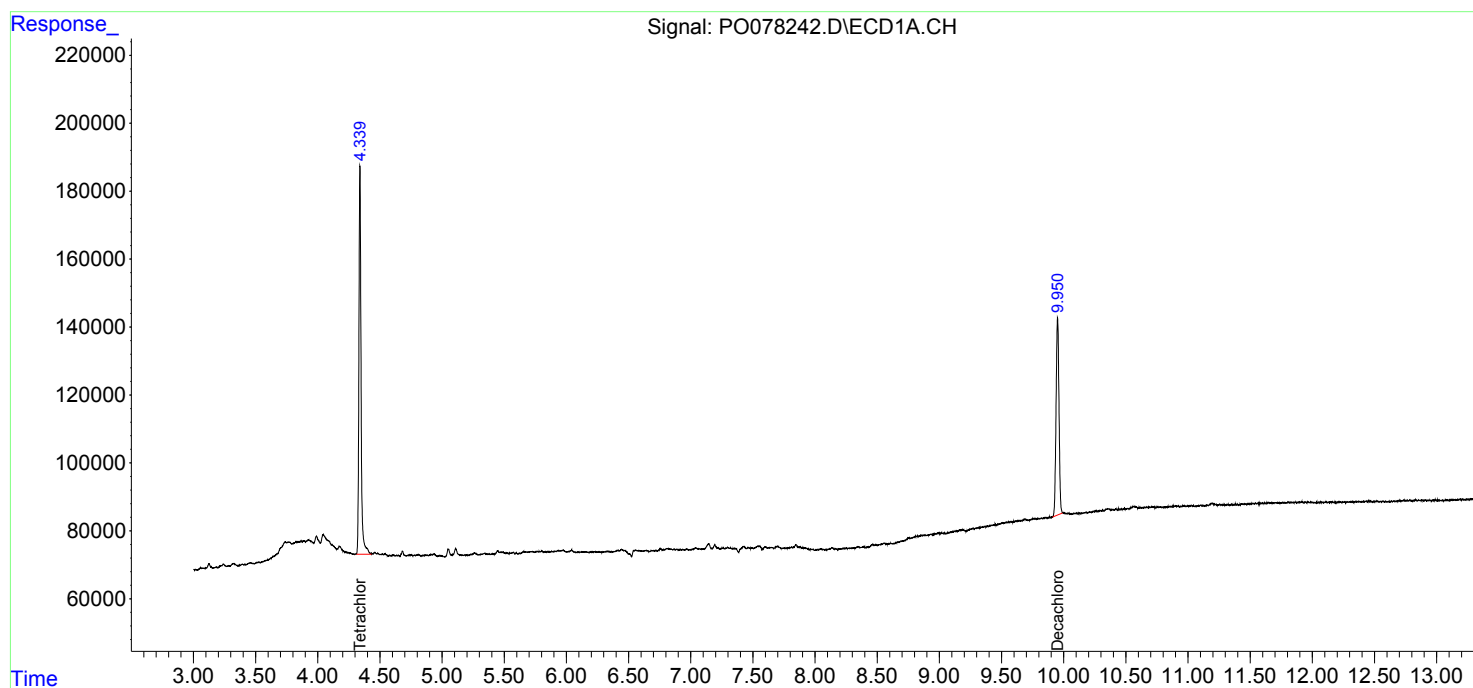

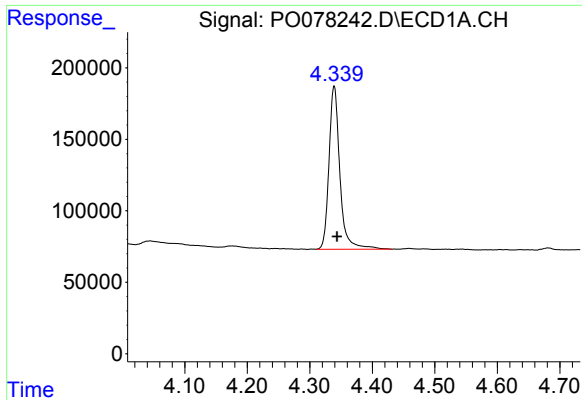

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 1384682
Conc: 18.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED


Ankita
5/28/2021 9:01:43 AM

5/28/2021 9:01:43 AM

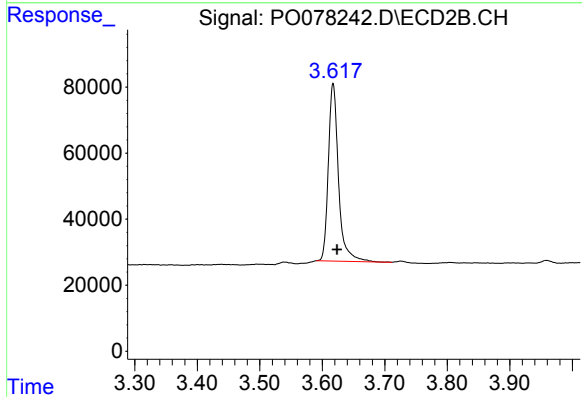


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.006 min
Response: 607607
Conc: 20.11 ng/ml

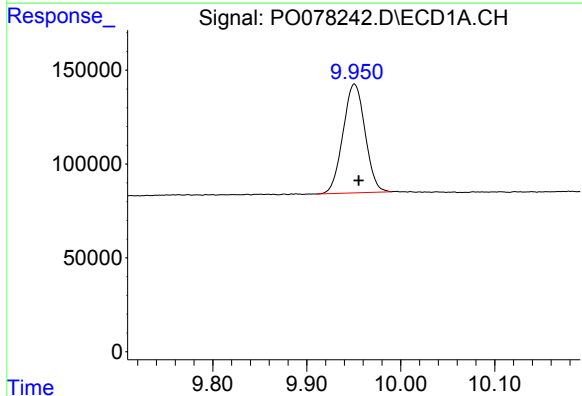

#2 Decachlorobiphenyl

R.T.: 9.951 min
Delta R.T.: -0.005 min
Response: 944600
Conc: 19.11 ng/ml

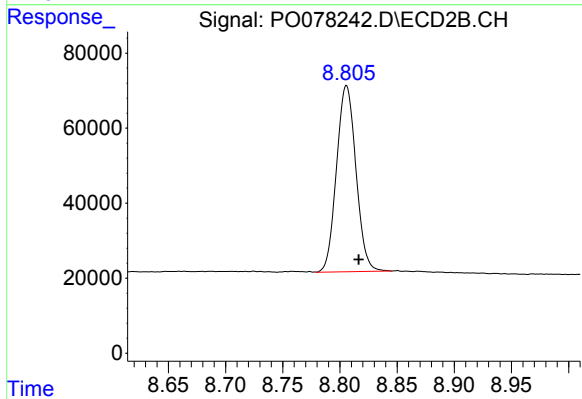

#2 Decachlorobiphenyl

R.T.: 8.805 min
Delta R.T.: -0.011 min
Response: 586725
Conc: 20.18 ng/ml m