

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052722\
 Data File : P0086690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 May 2022 10:31
 Operator : YP\AJ
 Sample : N3052-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEE613R-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/28/2022
 Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 27 23:23:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 19 09:06:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.476	3.670	176317	69961	1.735	1.606m
2) SA Decachlor...	10.332	8.725	98908	53980	1.822	1.551

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052722\
Data File : PO086690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 May 2022 10:31
Operator : YP\AJ
Sample : N3052-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HEE613R-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 27 23:23:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

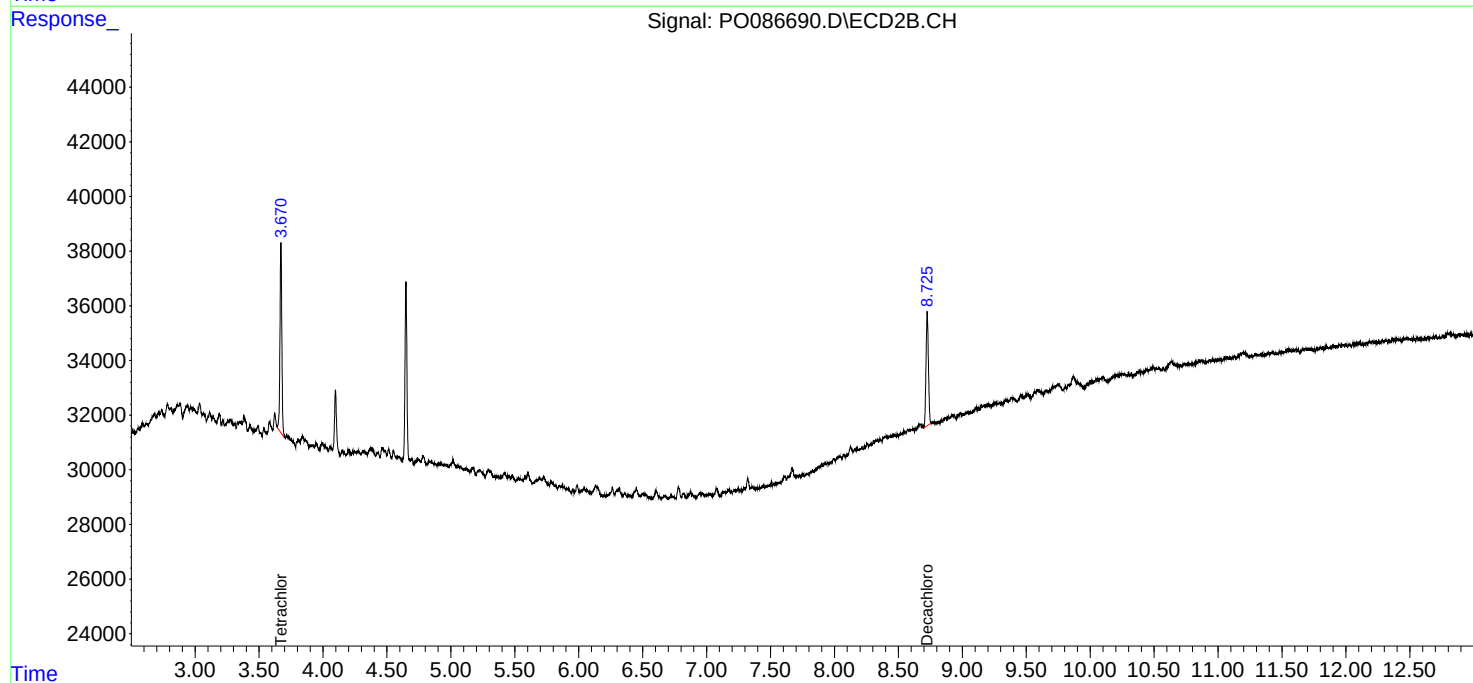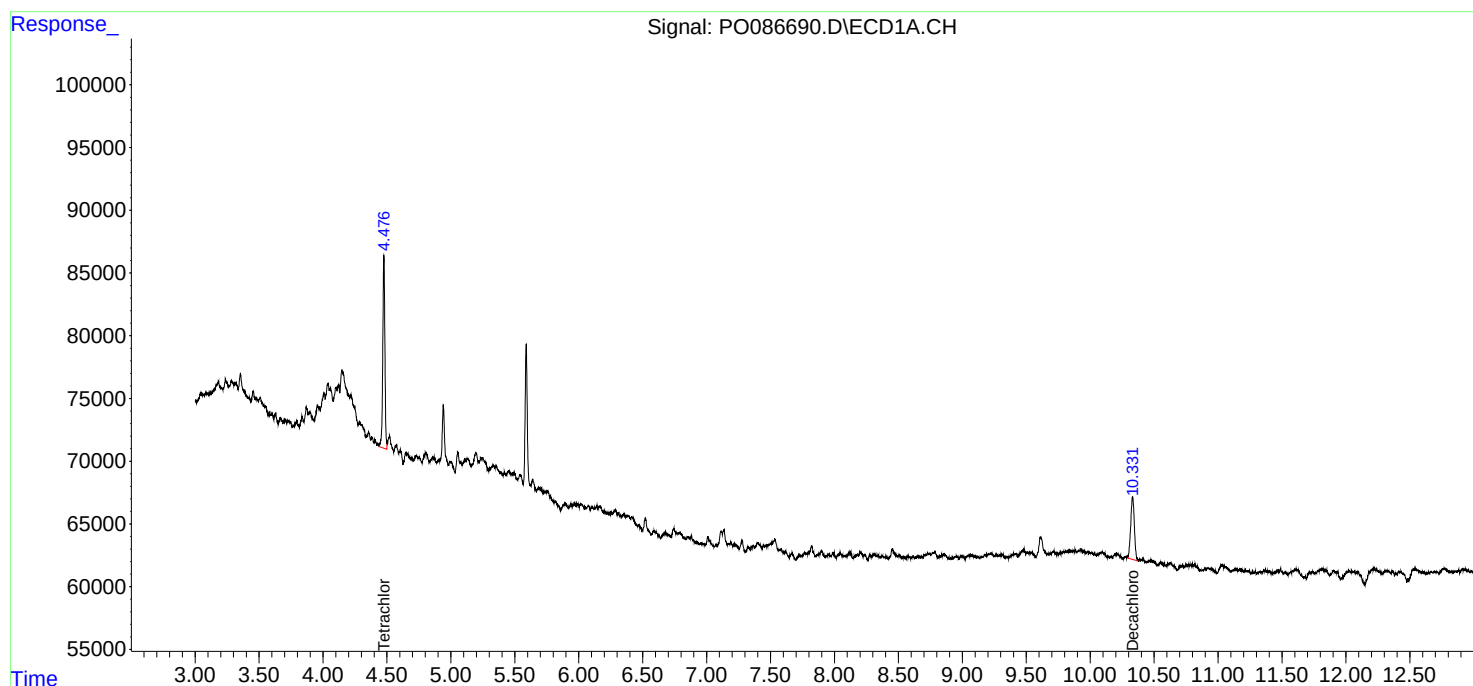

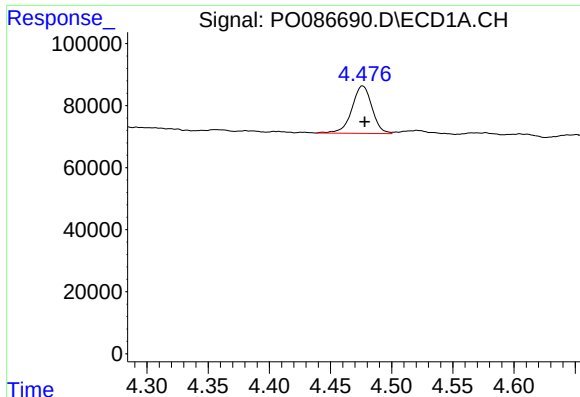


#1 Tetrachloro-m-xylene

R.T.: 4.476 min
Delta R.T.: -0.002 min
Response: 176317
Conc: 1.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEE613R-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/28/2022
Supervised By :Ankita Jodhani 05/28/2022

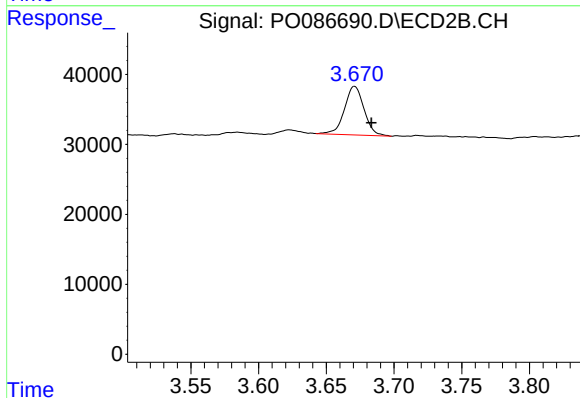


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.013 min
Response: 69961
Conc: 1.61 ng/ml m

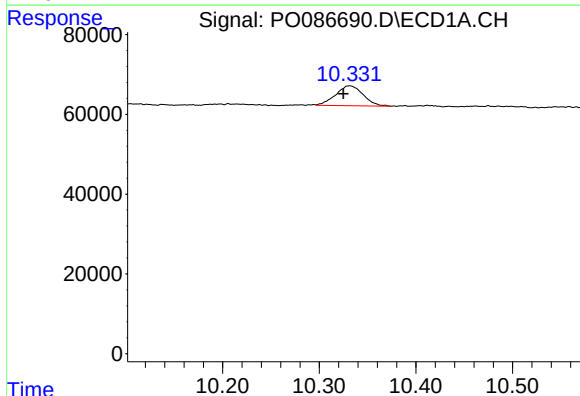

#2 Decachlorobiphenyl

R.T.: 10.332 min
Delta R.T.: 0.007 min
Response: 98908
Conc: 1.82 ng/ml

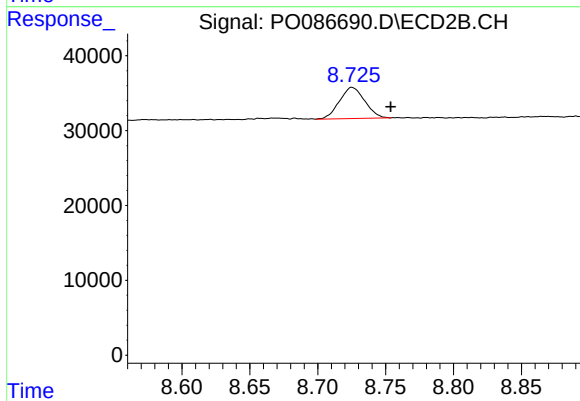

#2 Decachlorobiphenyl

R.T.: 8.725 min
Delta R.T.: -0.029 min
Response: 53980
Conc: 1.55 ng/ml