

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052722\
Data File : P0086738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 May 2022 00:58
Operator : YP\AJ
Sample : N3042-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
303

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:01:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.479	3.673	1053231	458614	10.366	10.529
2) SA Decachlor...	10.334	8.723	336980	201114	6.206	5.779

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052722\
Data File : P0086738.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 May 2022 00:58
Operator : YP\AJ
Sample : N3042-05
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
303

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 28 02:01:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 19 09:06:34 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

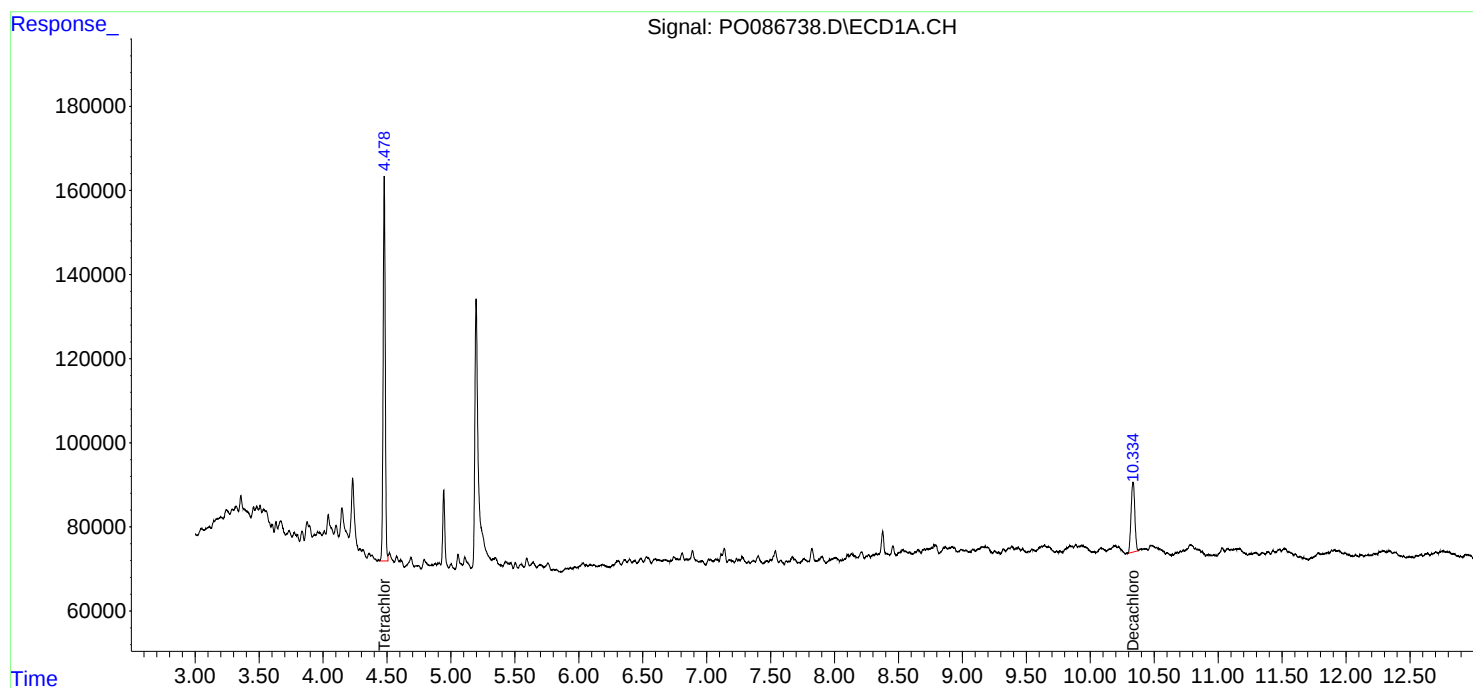


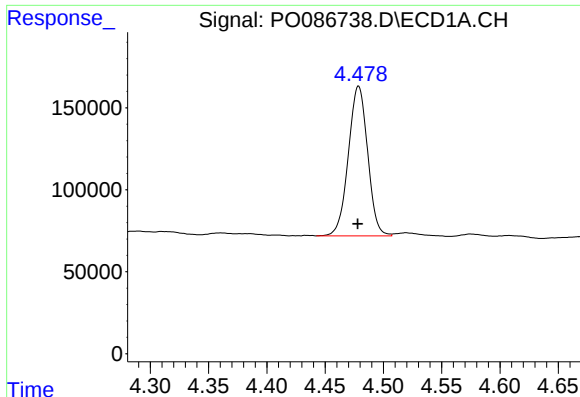

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 1053231
Conc: 10.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
303

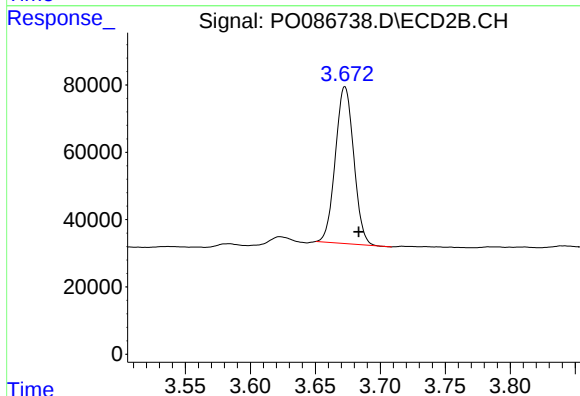


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.010 min
Response: 458614
Conc: 10.53 ng/ml

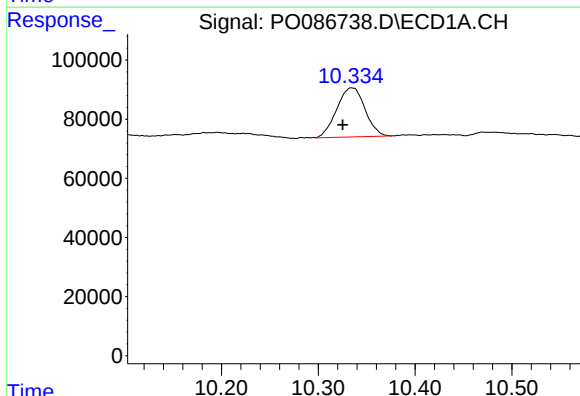

#2 Decachlorobiphenyl

R.T.: 10.334 min
Delta R.T.: 0.009 min
Response: 336980
Conc: 6.21 ng/ml

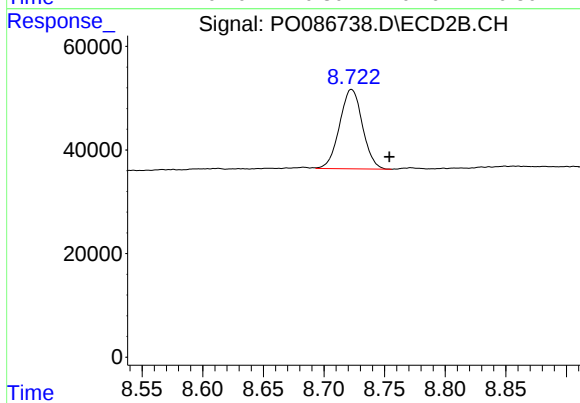

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.031 min
Response: 201114
Conc: 5.78 ng/ml