

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052821\
 Data File : P0078275.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 May 2021 21:25
 Operator : DD\AJ
 Sample : M2566-02 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 02-A-02-B-02-C

Manual Integrations
 APPROVED

Ankita
 6/1/2021 1:44:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 31 03:00:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.617	279296	129076	3.779	4.272
2) SA Decachlor...	9.952	8.805	234147	162744	4.736	5.597m
Target Compounds						
31) L7 AR-1260-1	7.297	6.408	50160	28356	17.874m	17.698
32) L7 AR-1260-2	7.560	6.605	61798	27754	18.370m	14.376
33) L7 AR-1260-3	7.922	6.755	39405	122958	16.150m	67.021 #
34) L7 AR-1260-4	8.146	7.232	43451	29542	16.221m	19.598m
35) L7 AR-1260-5	8.460	7.480	76694	138866	14.933m	39.821 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052821\
Data File : PO078275.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 May 2021 21:25
Operator : DD\AJ
Sample : M2566-02 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
6/1/2021 1:44:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 31 03:00:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

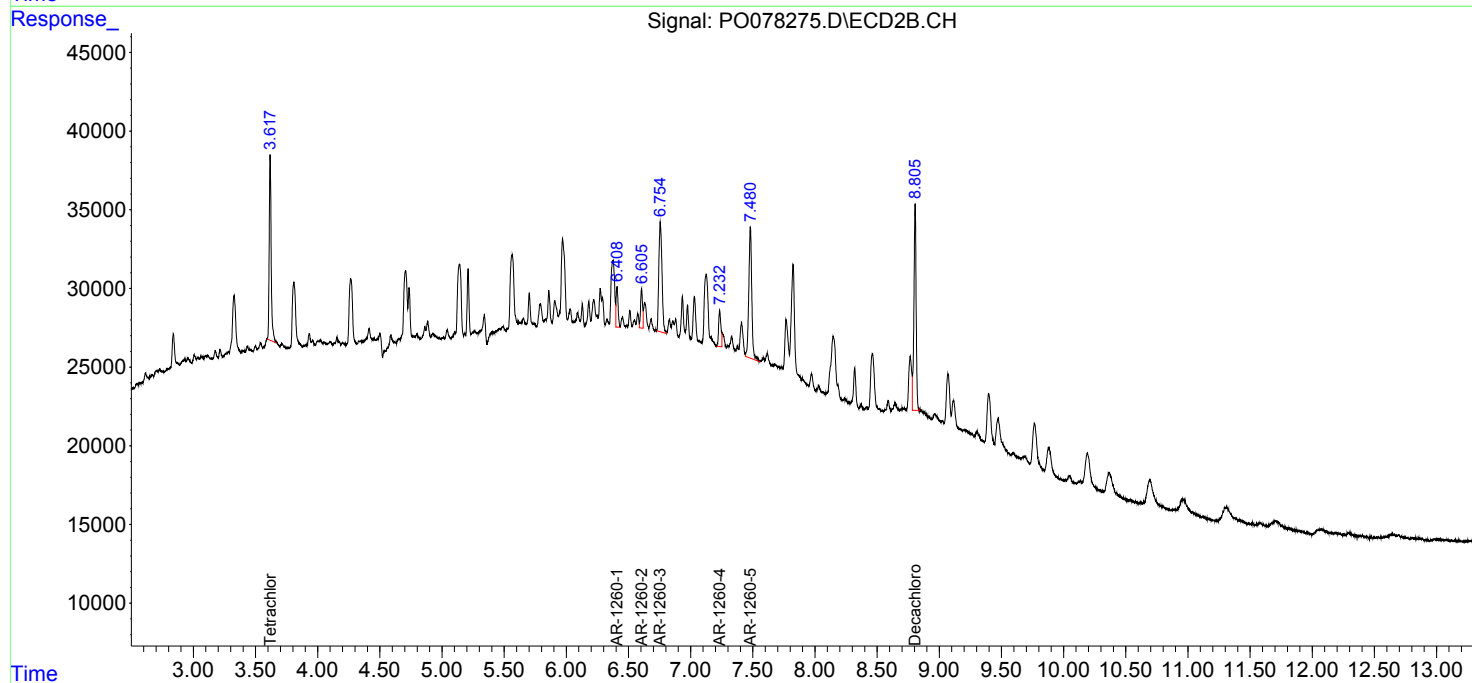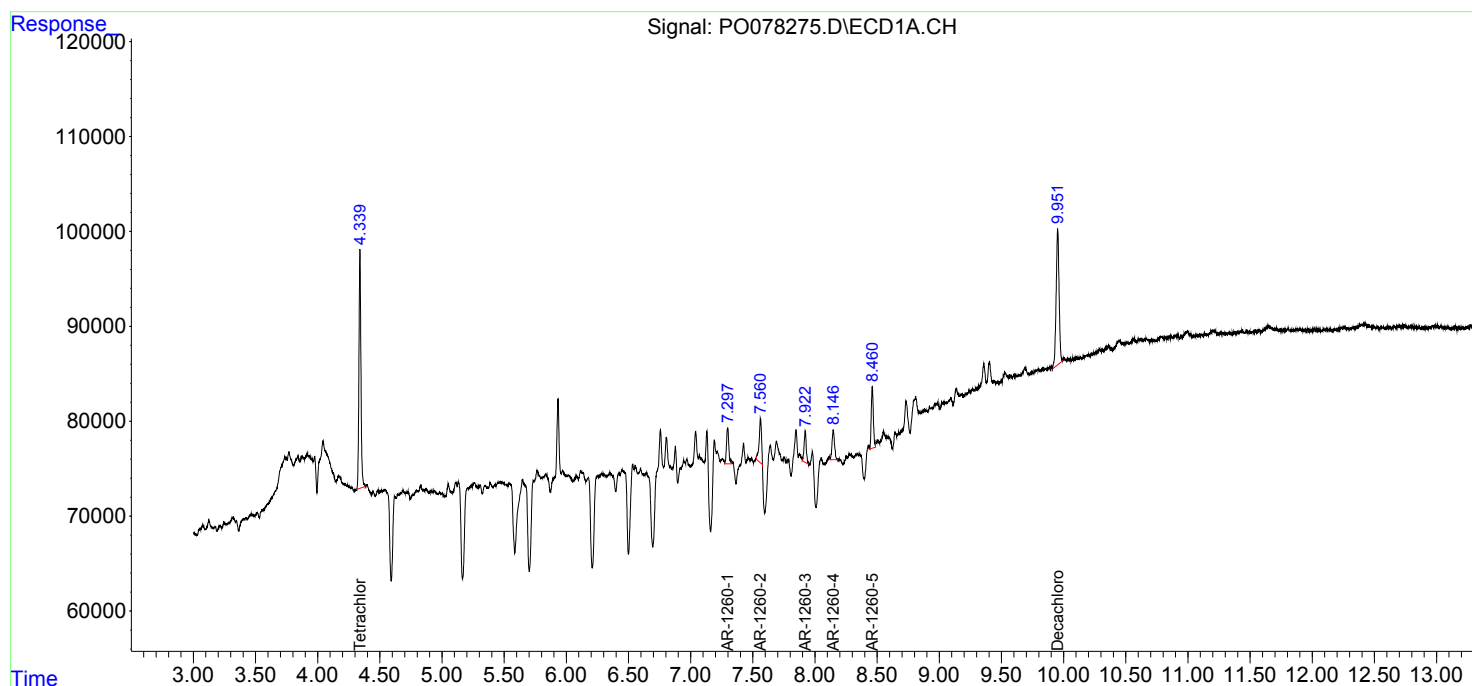

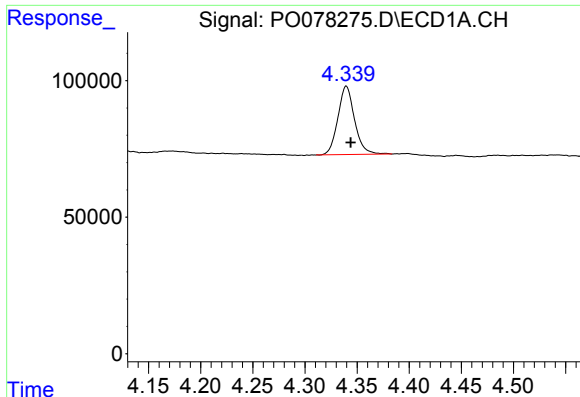


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 279296
Conc: 3.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
6/1/2021 1:44:53 PM

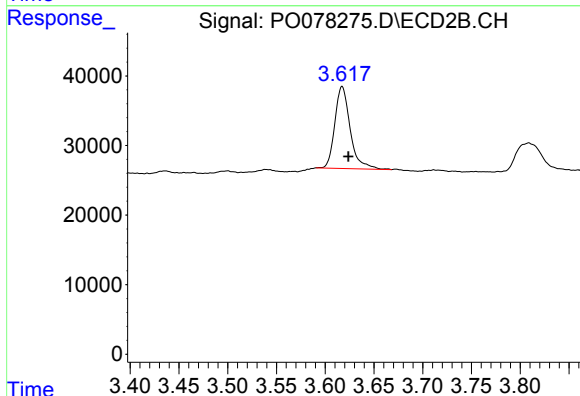


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.006 min
Response: 129076
Conc: 4.27 ng/ml

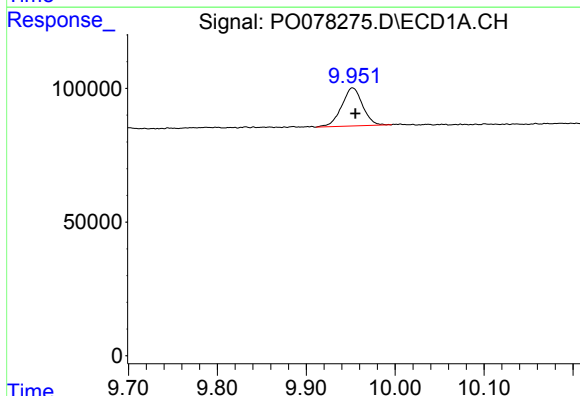


#2 Decachlorobiphenyl

R.T.: 9.952 min
Delta R.T.: -0.003 min
Response: 234147
Conc: 4.74 ng/ml

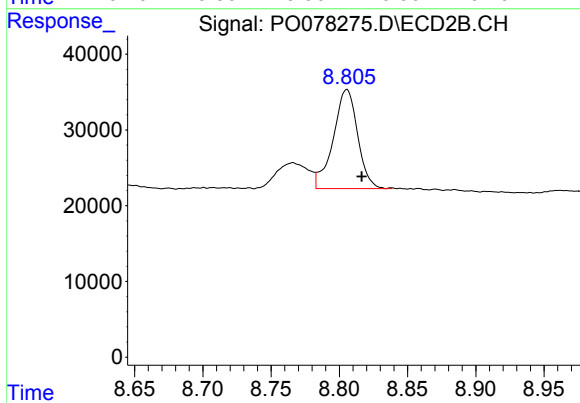

#2 Decachlorobiphenyl

R.T.: 8.805 min
Delta R.T.: -0.011 min
Response: 162744
Conc: 5.60 ng/ml m

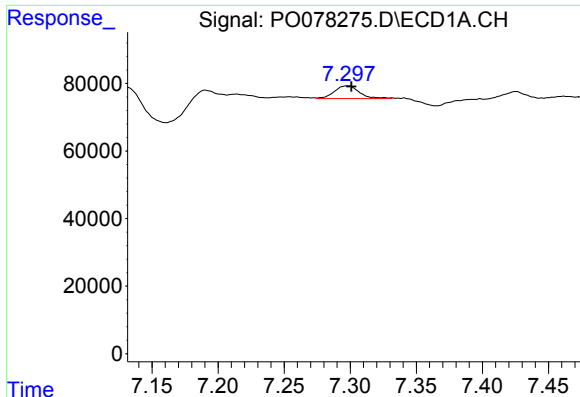


#31 AR-1260-1

R.T.: 7.297 min
Delta R.T.: -0.004 min
Response: 50160
Conc: 17.87 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
6/1/2021 1:44:53 PM

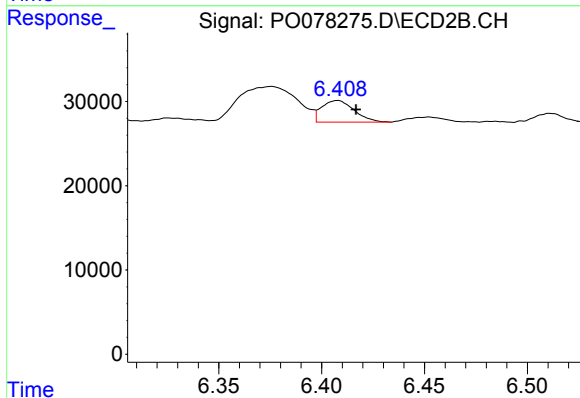


#31 AR-1260-1

R.T.: 6.408 min
Delta R.T.: -0.009 min
Response: 28356
Conc: 17.70 ng/ml

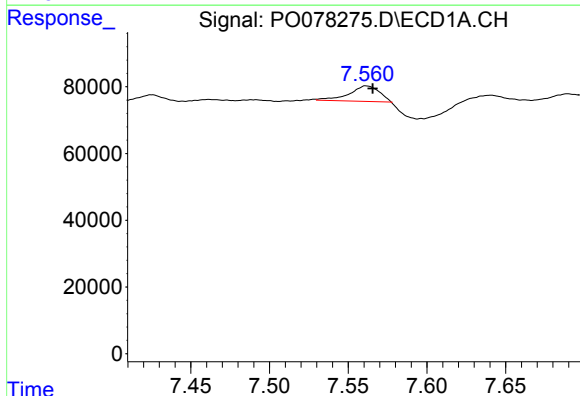


#32 AR-1260-2

R.T.: 7.560 min
Delta R.T.: -0.005 min
Response: 61798
Conc: 18.37 ng/ml m

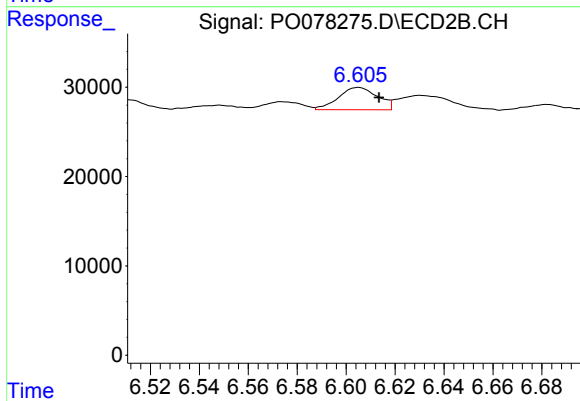

#32 AR-1260-2

R.T.: 6.605 min
Delta R.T.: -0.008 min
Response: 27754
Conc: 14.38 ng/ml

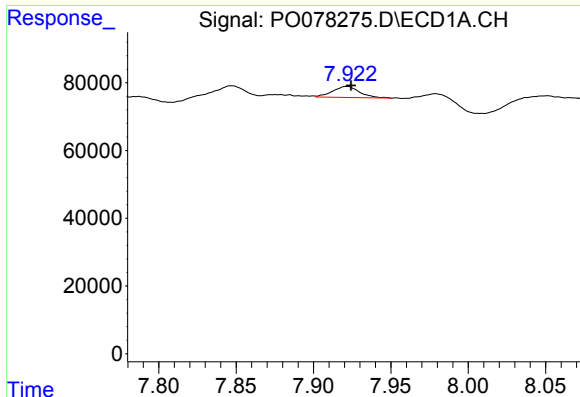


#33 AR-1260-3

R.T.: 7.922 min
Delta R.T.: -0.002 min
Response: 39405
Conc: 16.15 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C


Manual Integrations
APPROVED

Ankita
6/1/2021 1:44:53 PM

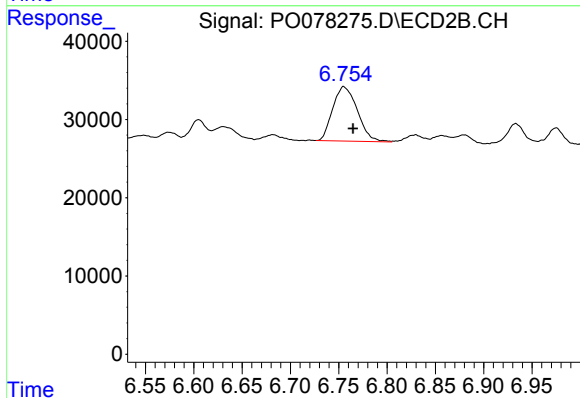


#33 AR-1260-3

R.T.: 6.755 min
Delta R.T.: -0.010 min
Response: 122958
Conc: 67.02 ng/ml

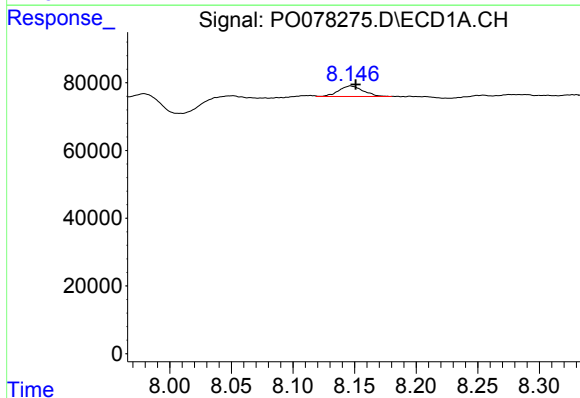


#34 AR-1260-4

R.T.: 8.146 min
Delta R.T.: -0.005 min
Response: 43451
Conc: 16.22 ng/ml m

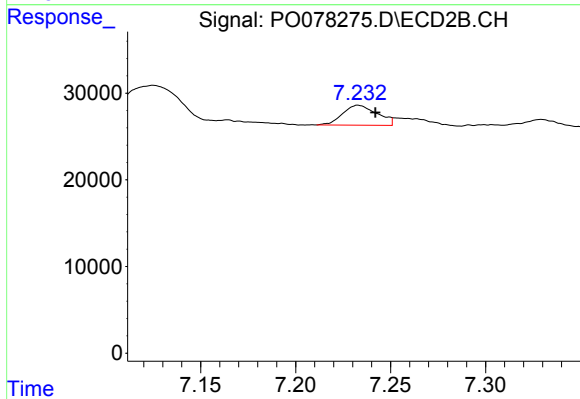

#34 AR-1260-4

R.T.: 7.232 min
Delta R.T.: -0.010 min
Response: 29542
Conc: 19.60 ng/ml m

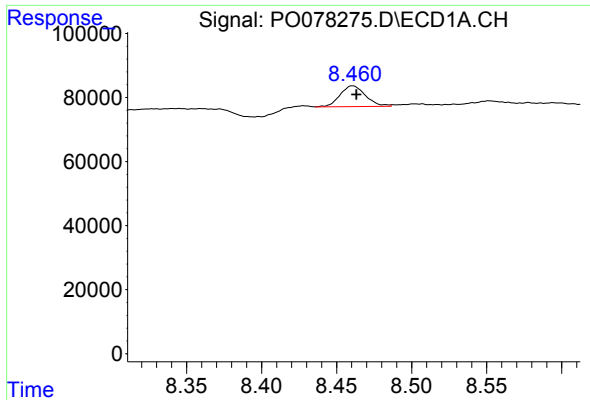


#35 AR-1260-5

R.T.: 8.460 min
Delta R.T.: -0.003 min
Response: 76694
Conc: 14.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
02-A-02-B-02-C

Manual Integrations
APPROVED

Ankita
6/1/2021 1:44:53 PM

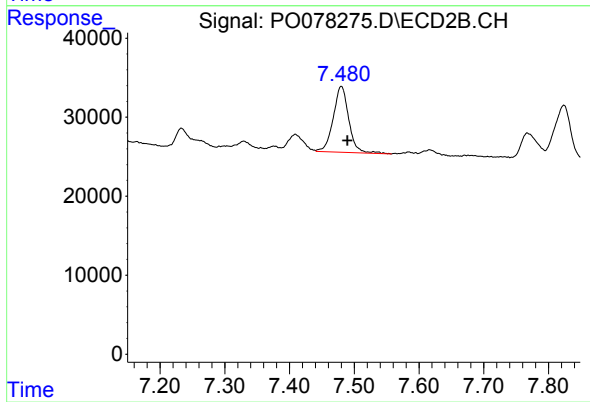

#35 AR-1260-5

R.T.: 7.480 min
Delta R.T.: -0.009 min
Response: 138866
Conc: 39.82 ng/ml