

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0052825\
 Data File : P0111311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 May 2025 13:45
 Operator : YP/AJ
 Sample : Q2130-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/29/2025
 Supervised By :mohammad ahmed 05/30/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 29 02:06:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.680	3.676	115.0E6	97538864	19.546	17.892
2) SA Decachlor...	8.717	8.667	69238603	27439460	13.411	14.831m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO052825\
Data File : PO111311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 May 2025 13:45
Operator : YP/AJ
Sample : Q2130-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2025
Supervised By :mohammad ahmed 05/30/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 29 02:06:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

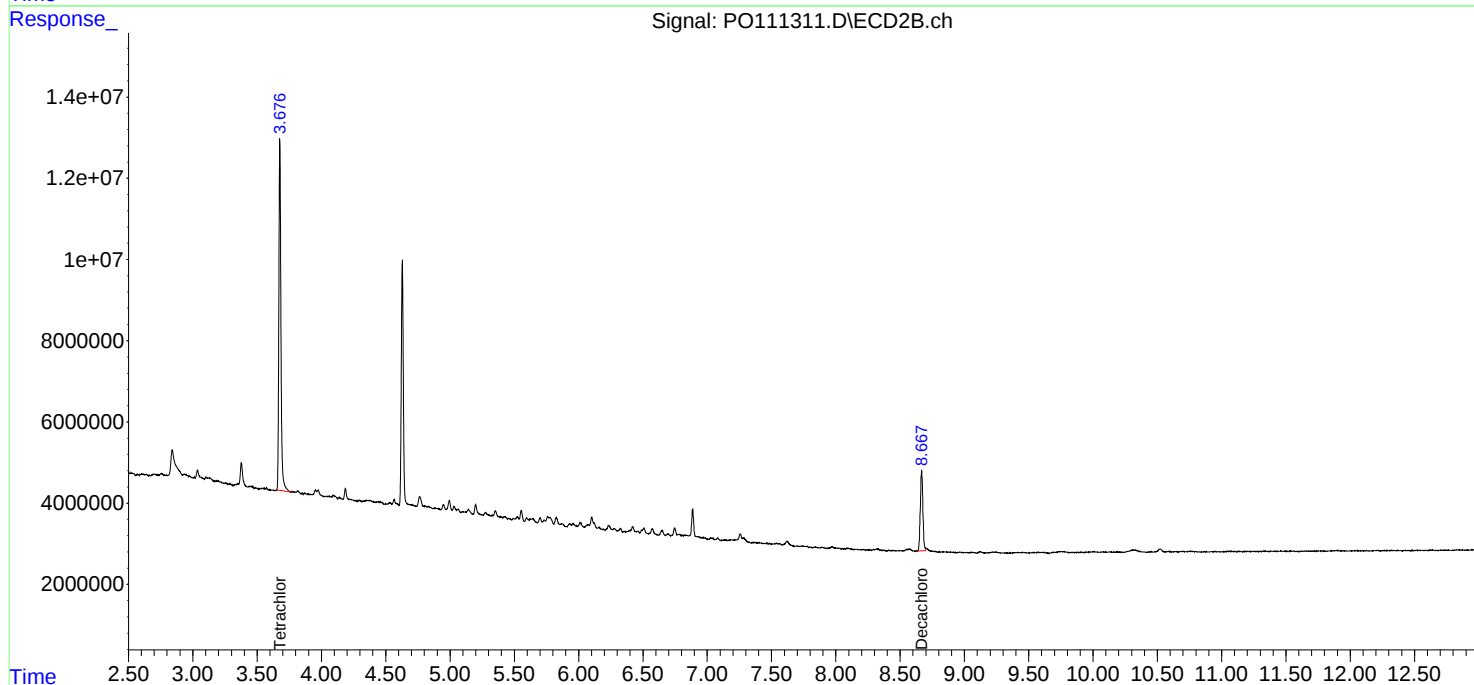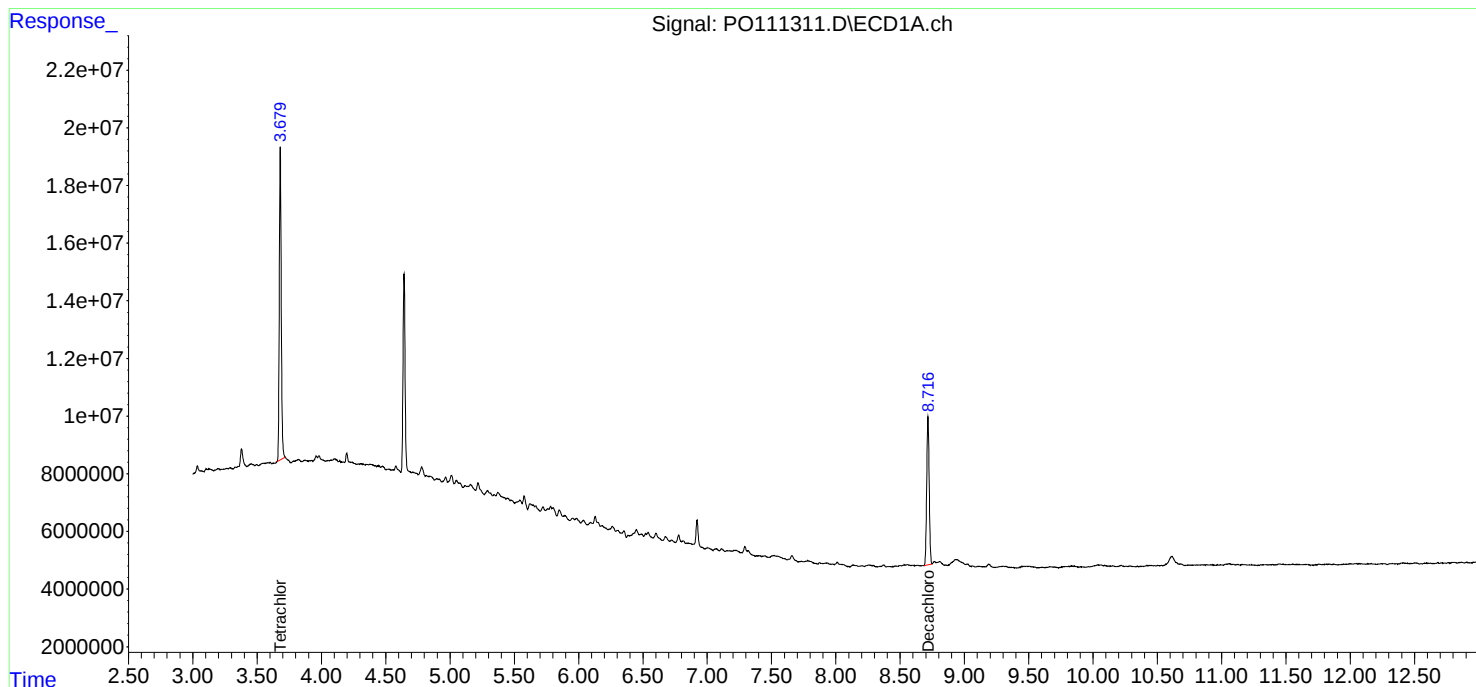

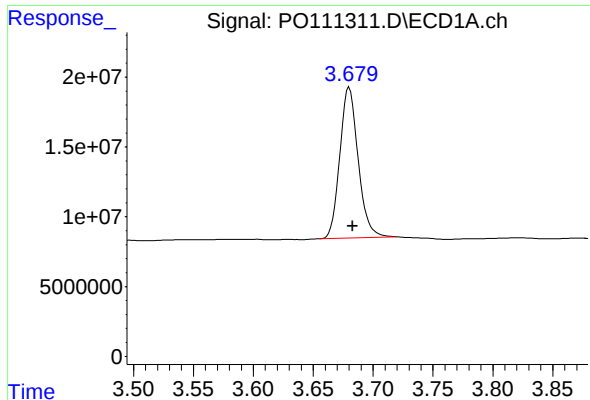


#1 Tetrachloro-m-xylene

R.T.: 3.680 min
Delta R.T.: -0.003 min
Response: 114995203
Conc: 19.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/29/2025
Supervised By :mohammad ahmed 05/30/2025

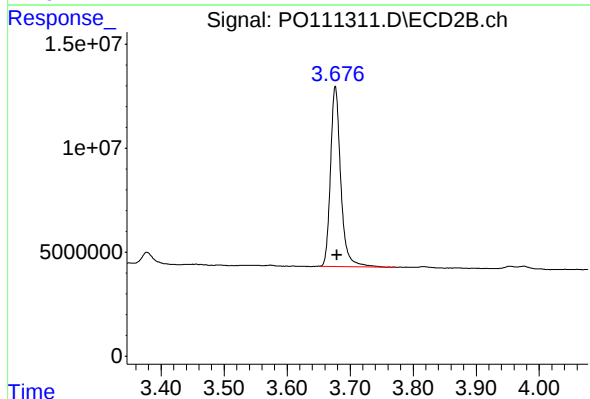


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.002 min
Response: 97538864
Conc: 17.89 ng/ml

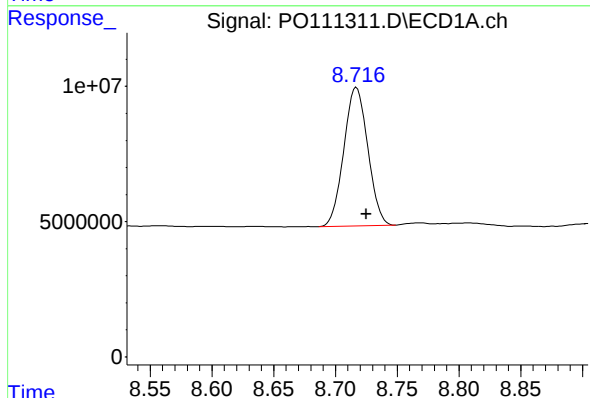

#2 Decachlorobiphenyl

R.T.: 8.717 min
Delta R.T.: -0.008 min
Response: 69238603
Conc: 13.41 ng/ml

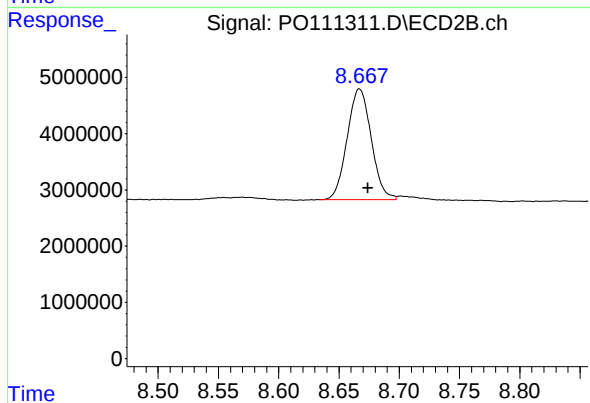

#2 Decachlorobiphenyl

R.T.: 8.667 min
Delta R.T.: -0.008 min
Response: 27439460
Conc: 14.83 ng/ml m