

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060121\
 Data File : P0078304.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2021 16:51
 Operator : DD\AJ
 Sample : M2569-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 C0AA0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:00:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.618	1545007	686116	20.905	22.707
2) SA Decachlor...	9.949	8.804	973862	578609	19.698	19.899
Target Compounds						
8) L2 AR-1221-1	4.584	0.000	379247	0	460.773	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060121\
Data File : P0078304.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2021 16:51
Operator : DD\AJ
Sample : M2569-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
C0AA0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:00:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

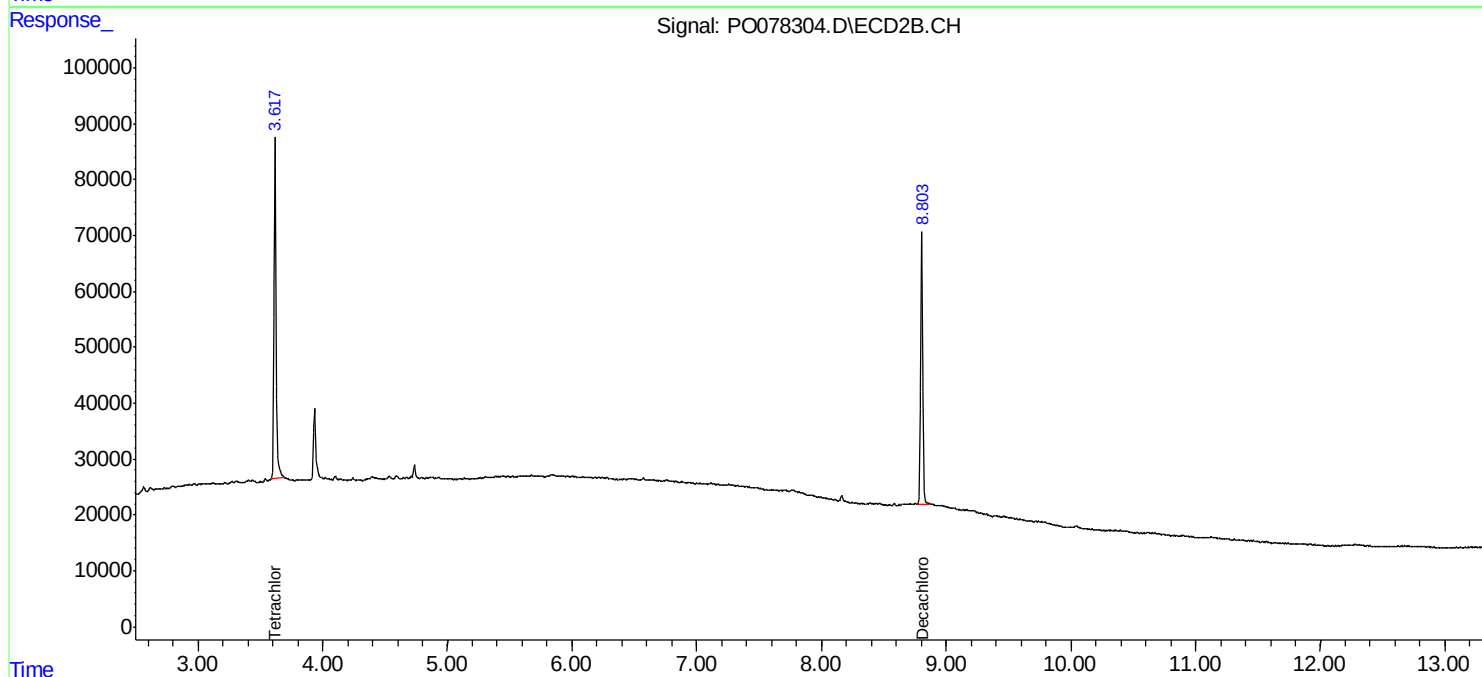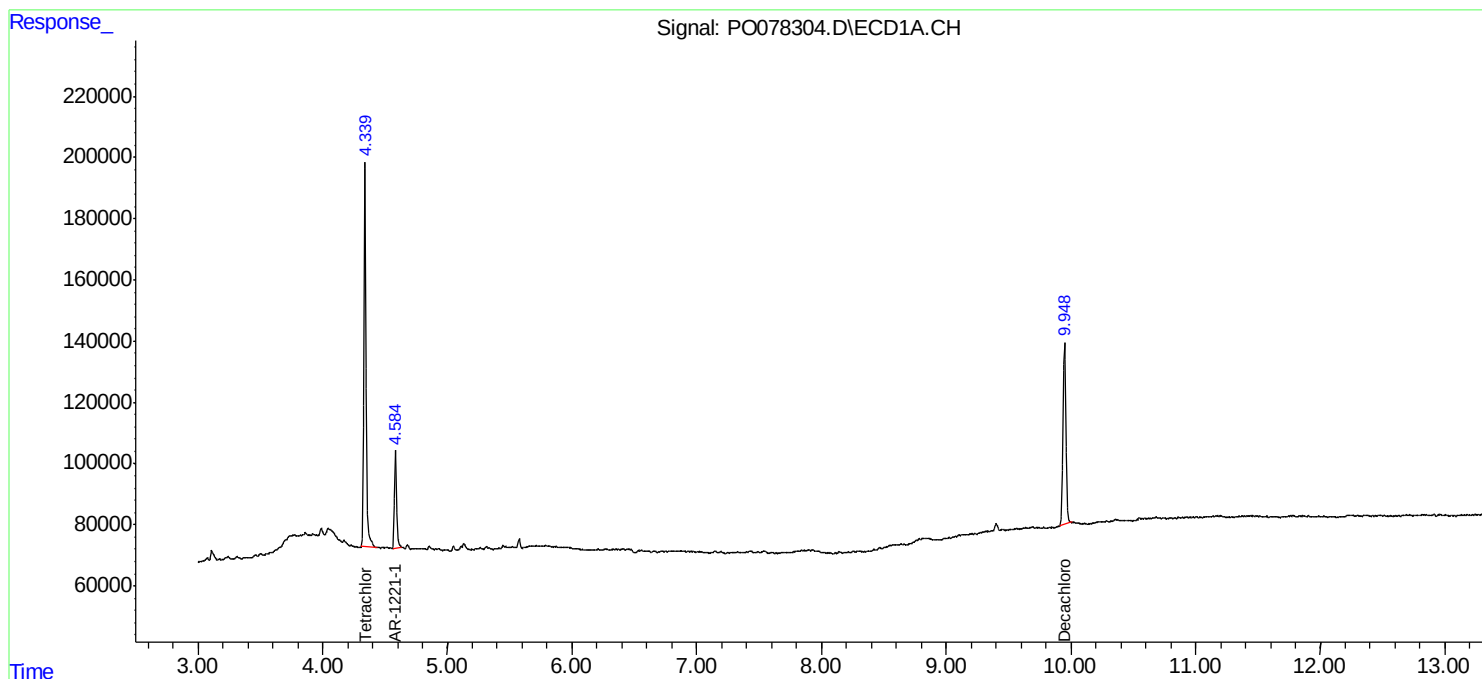


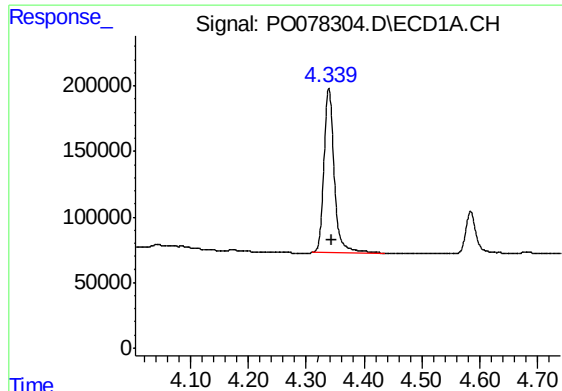

#1 Tetrachloro-m-xylene


R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 1545007
Conc: 20.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AA0

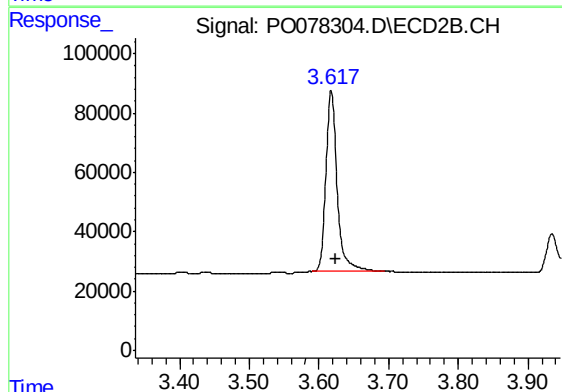


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.006 min
Response: 686116
Conc: 22.71 ng/ml

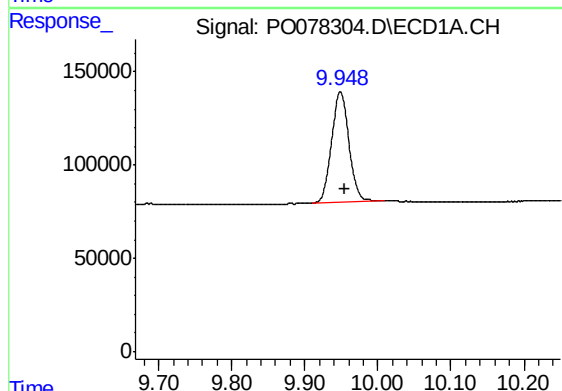


#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.006 min
Response: 973862
Conc: 19.70 ng/ml

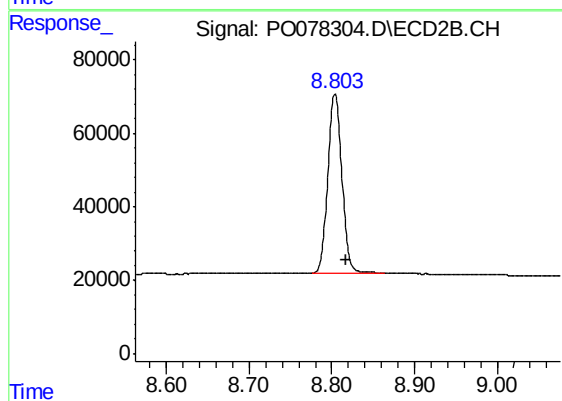

#2 Decachlorobiphenyl


R.T.: 8.804 min
Delta R.T.: -0.013 min
Response: 578609
Conc: 19.90 ng/ml

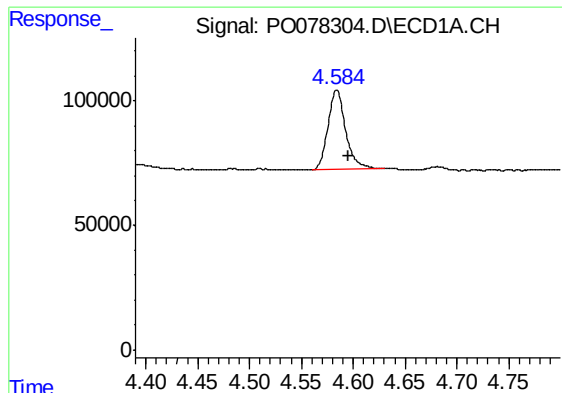

#8 AR-1221-1

R.T.: 4.584 min
Delta R.T.: -0.012 min
Response: 379247
Conc: 460.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
C0AA0

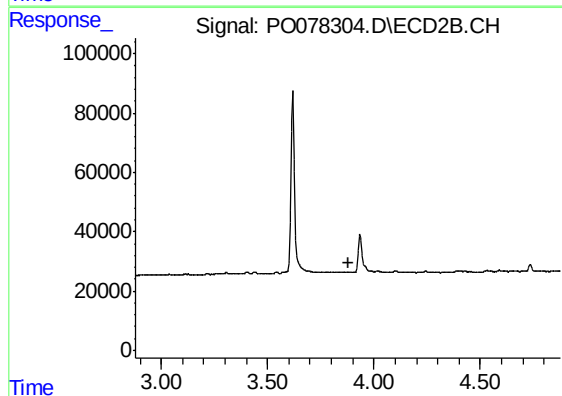

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.878 min
Response: 0
Conc: N.D.