

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060121\
 Data File : P0078291.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2021 13:08
 Operator : DD\AJ
 Sample : M2564-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33190

Manual Integrations
 APPROVED

Ankita
 6/2/2021 10:23:30 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 00:52:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.340	3.618	764180	403748	10.340	13.362 #
2)	SA Decachlor...	9.950	8.804	904221	551274	18.289	18.959
Target Compounds							
26)	L6 AR-1254-1	6.531	5.704	525415	353660	211.691	205.068
27)	L6 AR-1254-2	6.758	5.860	996240	237808	256.727	148.354 #
28)	L6 AR-1254-3	7.129	6.273	974511	489547	248.388	205.111
29)	L6 AR-1254-4	7.423	6.511	474555	287048	174.745	197.711
30)	L6 AR-1254-5	7.847	6.934	831754	763357	284.411	335.846

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060121\
Data File : P0078291.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2021 13:08
Operator : DD\AJ
Sample : M2564-03
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
33190


Manual Integrations
APPROVED

Ankita
6/2/2021 10:23:30 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 00:52:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

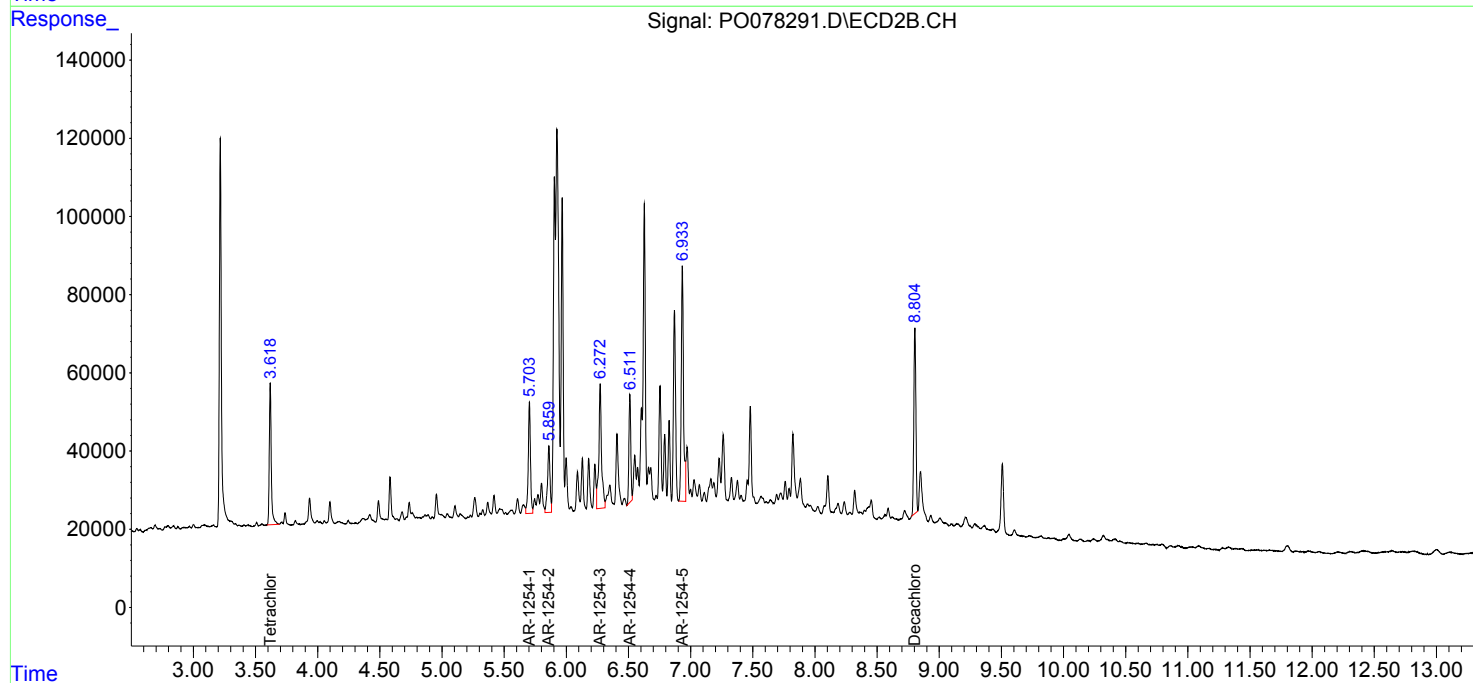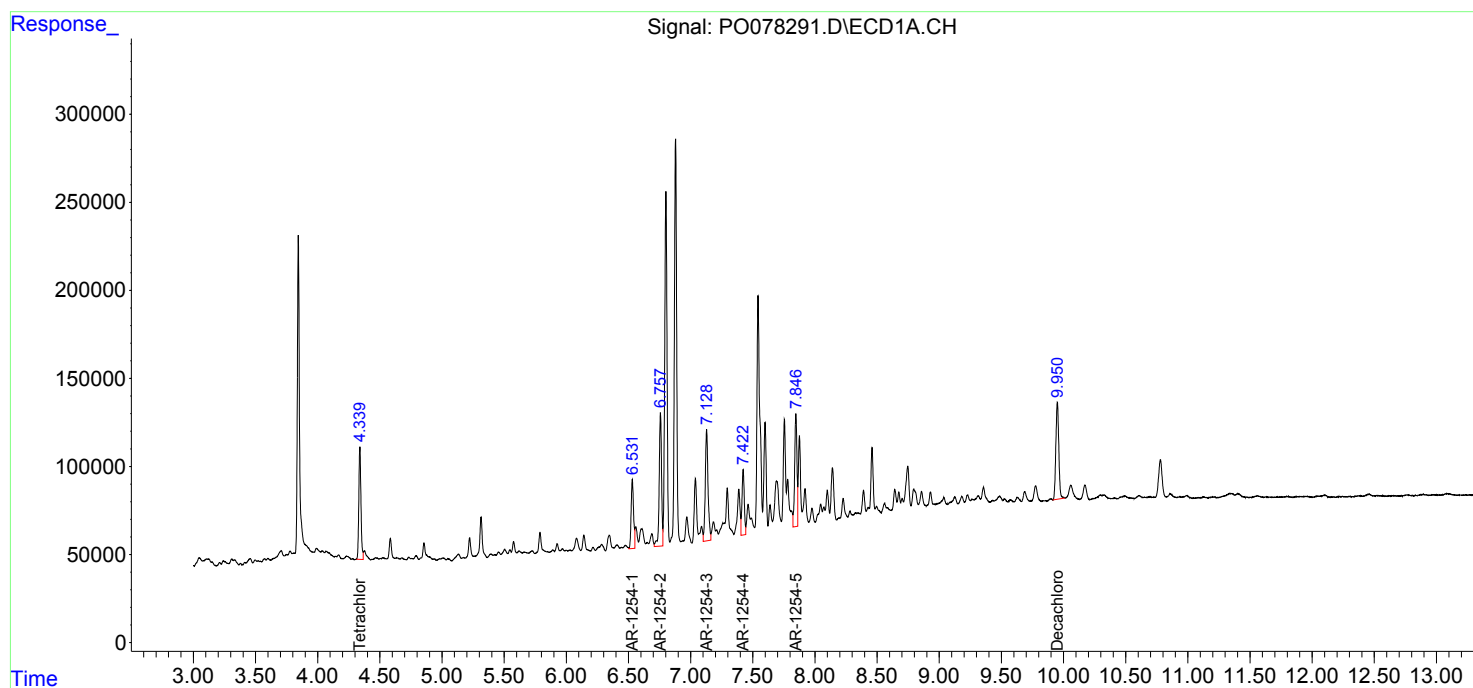

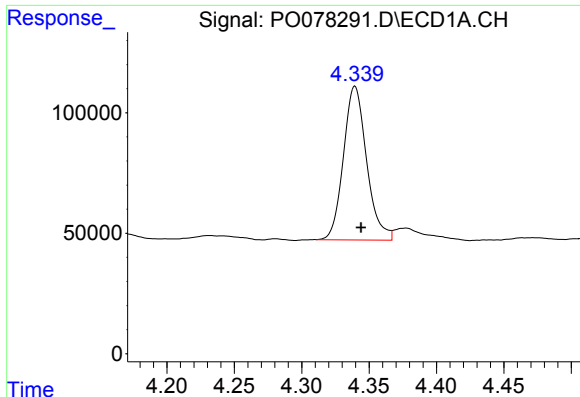


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 764180
Conc: 10.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
33190


Manual Integrations
APPROVED

Ankita
6/2/2021 10:23:30 AM

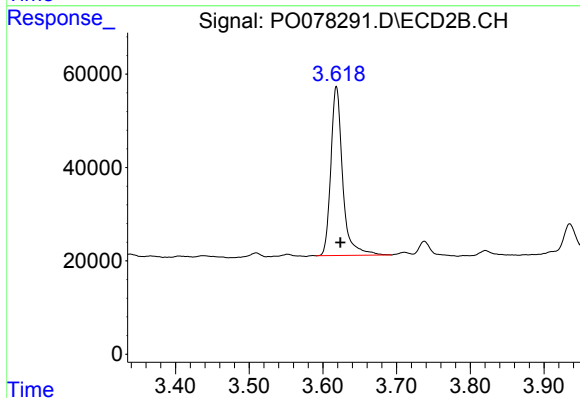


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: -0.005 min
Response: 403748
Conc: 13.36 ng/ml

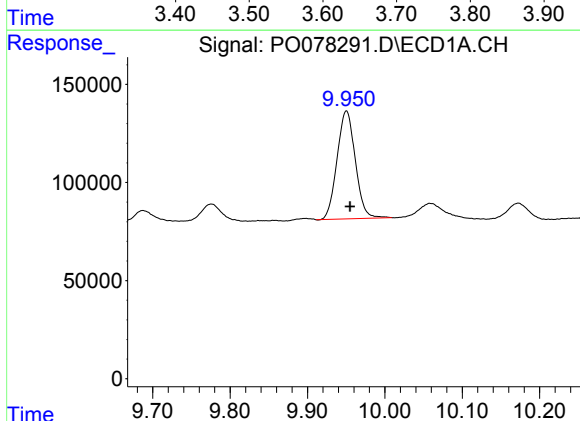


#2 Decachlorobiphenyl

R.T.: 9.950 min
Delta R.T.: -0.005 min
Response: 904221
Conc: 18.29 ng/ml

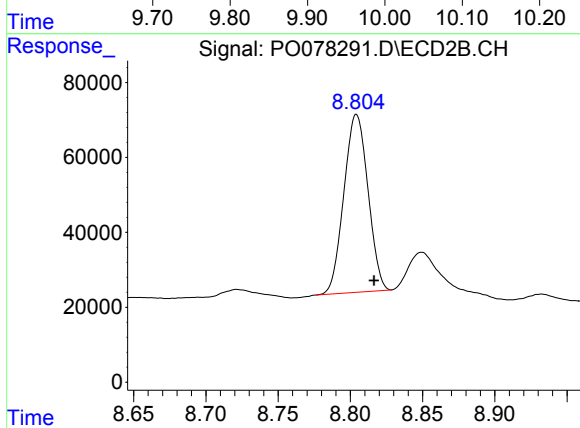

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.012 min
Response: 551274
Conc: 18.96 ng/ml

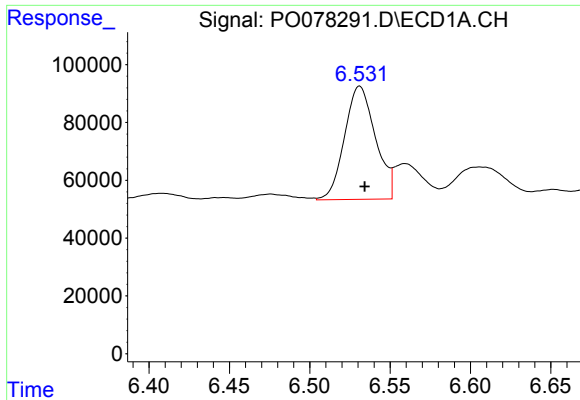


#26 AR-1254-1

R.T.: 6.531 min
Delta R.T.: -0.003 min
Response: 525415
Conc: 211.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
33190


Manual Integrations
APPROVED

Ankita
6/2/2021 10:23:30 AM

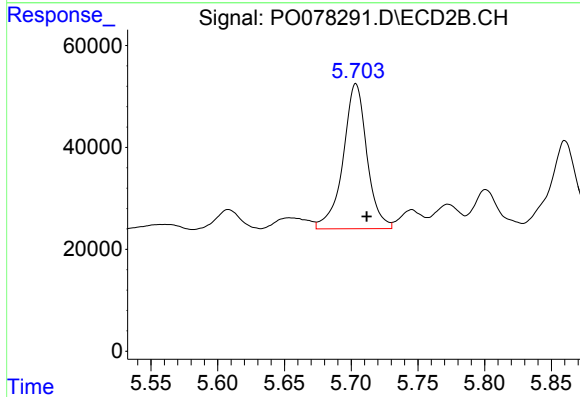


#26 AR-1254-1

R.T.: 5.704 min
Delta R.T.: -0.008 min
Response: 353660
Conc: 205.07 ng/ml

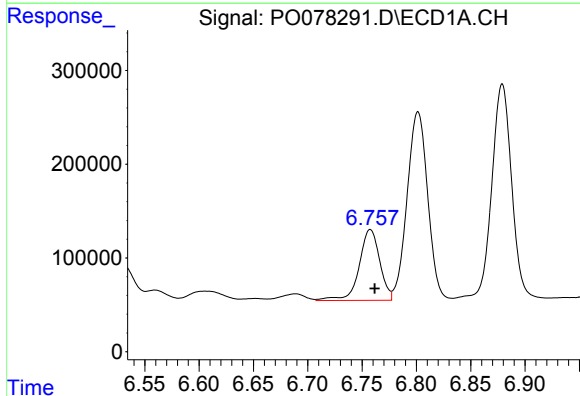


#27 AR-1254-2

R.T.: 6.758 min
Delta R.T.: -0.004 min
Response: 996240
Conc: 256.73 ng/ml

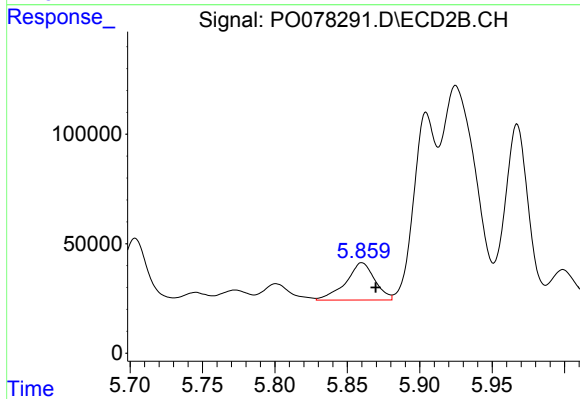

#27 AR-1254-2

R.T.: 5.860 min
Delta R.T.: -0.010 min
Response: 237808
Conc: 148.35 ng/ml

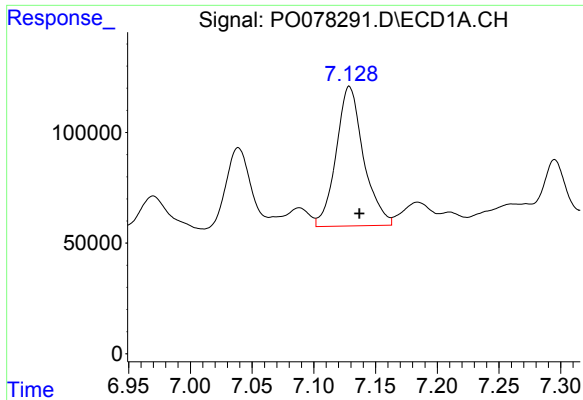


#28 AR-1254-3

R.T.: 7.129 min
Delta R.T.: -0.008 min
Response: 974511
Conc: 248.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
33190


Manual Integrations
APPROVED

Ankita
6/2/2021 10:23:30 AM

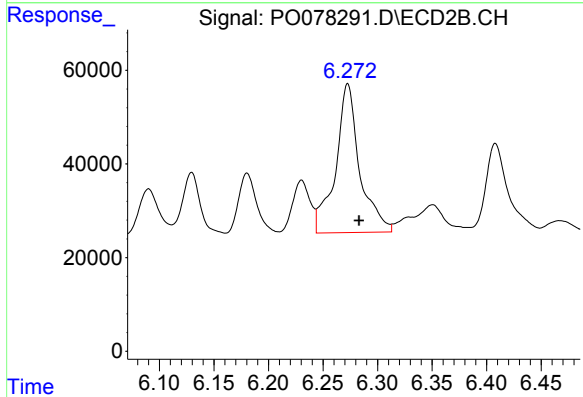


#28 AR-1254-3

R.T.: 6.273 min
Delta R.T.: -0.010 min
Response: 489547
Conc: 205.11 ng/ml

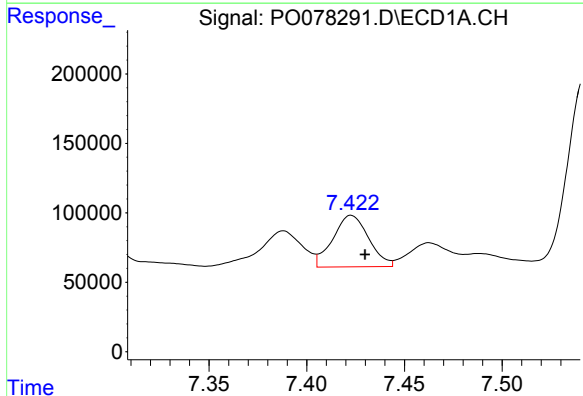


#29 AR-1254-4

R.T.: 7.423 min
Delta R.T.: -0.007 min
Response: 474555
Conc: 174.75 ng/ml

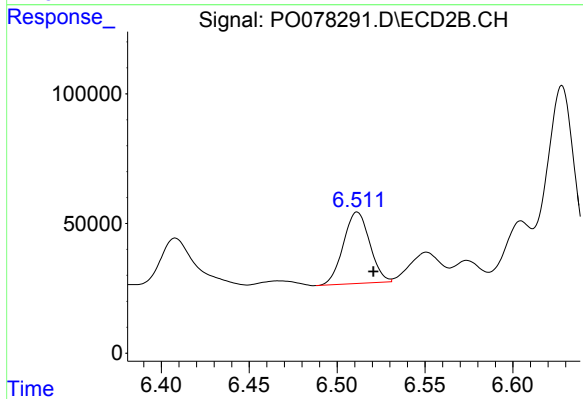

#29 AR-1254-4

R.T.: 6.511 min
Delta R.T.: -0.009 min
Response: 287048
Conc: 197.71 ng/ml

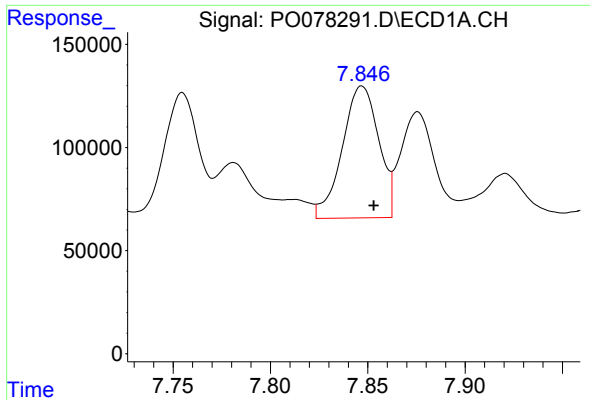


#30 AR-1254-5

R.T.: 7.847 min
Delta R.T.: -0.006 min
Response: 831754
Conc: 284.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
33190

Manual Integrations
APPROVED

Ankita
6/2/2021 10:23:30 AM

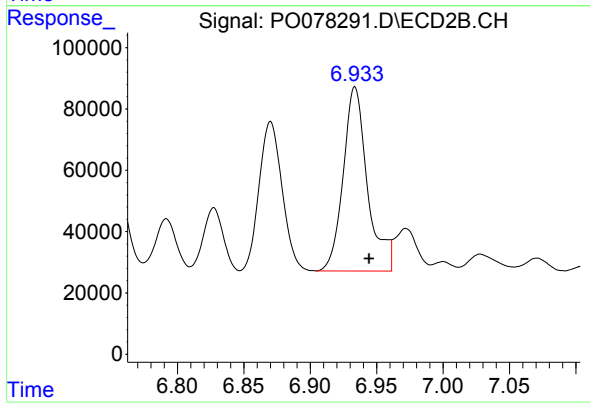

#30 AR-1254-5

R.T.: 6.934 min
Delta R.T.: -0.011 min
Response: 763357
Conc: 335.85 ng/ml