

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060121\
 Data File : P0078317.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2021 20:52
 Operator : DD\AJ
 Sample : M2563-12
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PLA-120

Manual Integrations
 APPROVED

Ankita
 6/2/2021 10:24:14 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 02 01:08:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.616	1345131	602484	18.200	19.939
2) SA Decachlor...	9.946	8.803	1035374	595823	20.942	20.491
Target Compounds						
16) L4 AR-1242-1	5.633	4.843	230080	96580	125.239m	112.445m
17) L4 AR-1242-2	5.655	4.863	431079	136931	159.578m	113.173 #
18) L4 AR-1242-3	5.719	5.051	220916	77443	126.925m	120.205
19) L4 AR-1242-4	5.824	5.146	225408	78757	161.234m	116.496 #
20) L4 AR-1242-5	6.595	5.701	229332	126435	171.383m	154.188

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060121\
Data File : PO078317.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2021 20:52
Operator : DD\AJ
Sample : M2563-12
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PLA-120


Manual Integrations
APPROVED

Ankita
6/2/2021 10:24:14 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 02 01:08:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

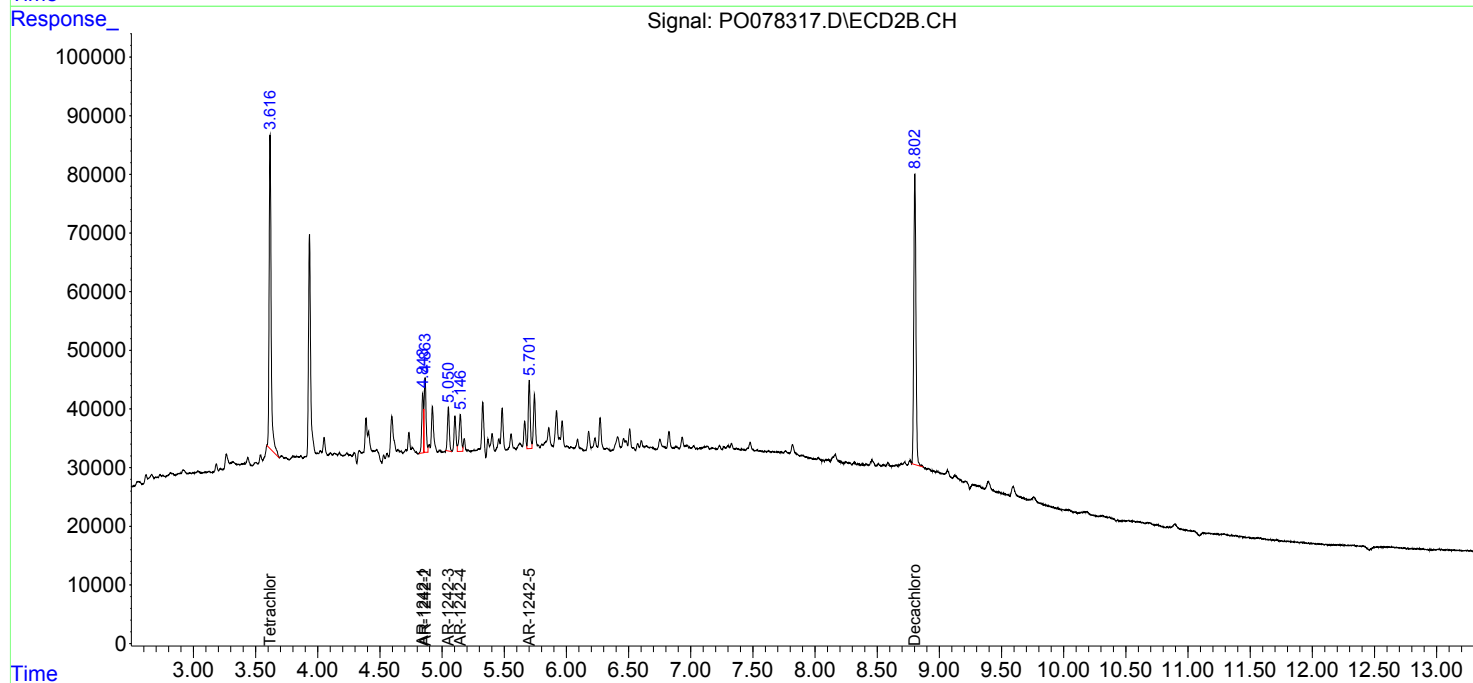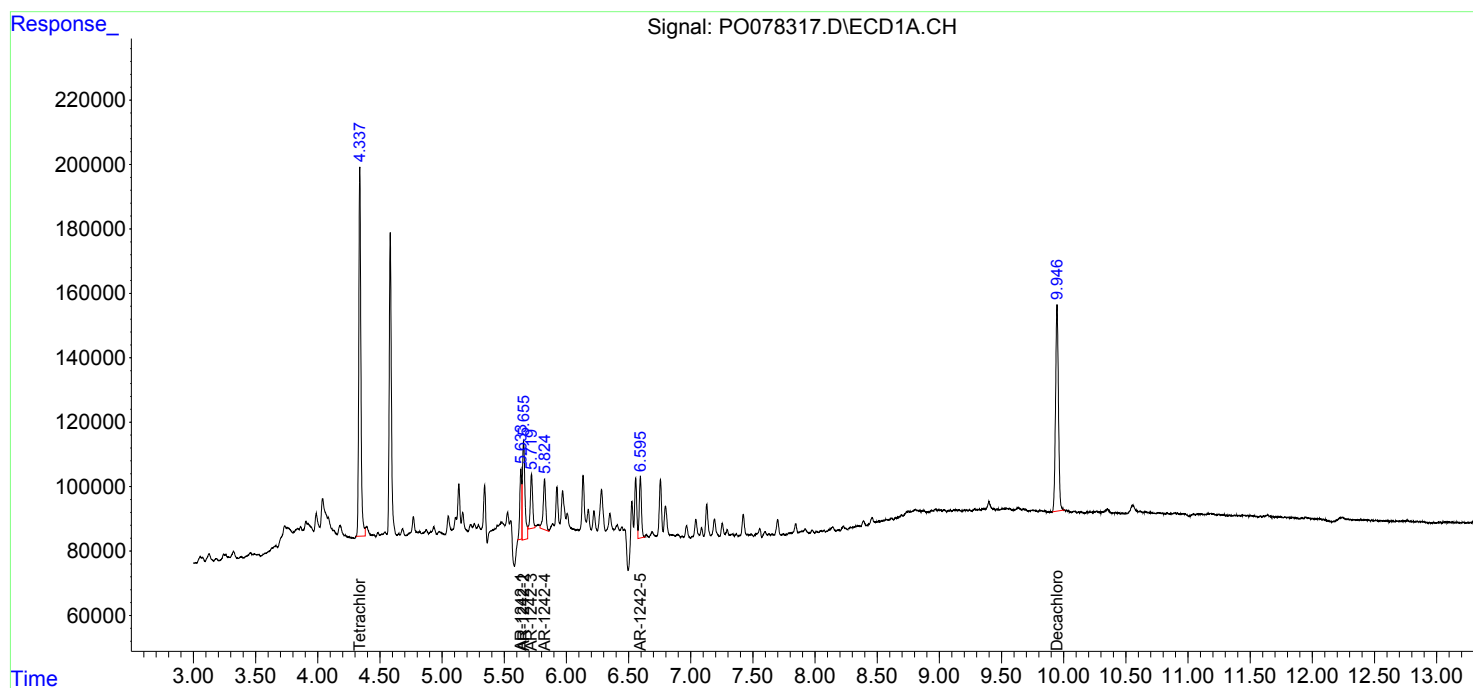

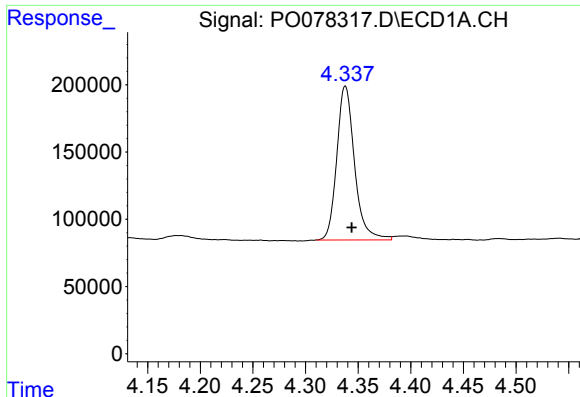


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 1345131
Conc: 18.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-120


Manual Integrations
APPROVED

Ankita
6/2/2021 10:24:14 AM

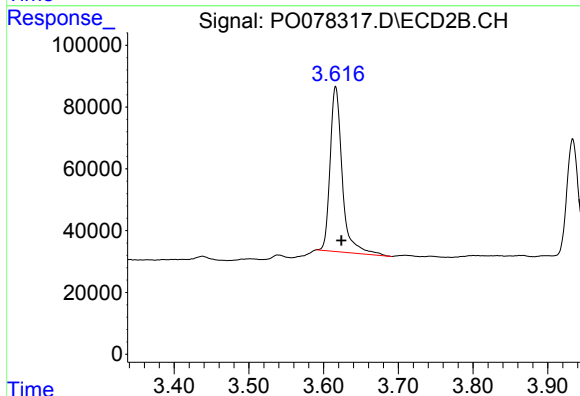


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.008 min
Response: 602484
Conc: 19.94 ng/ml

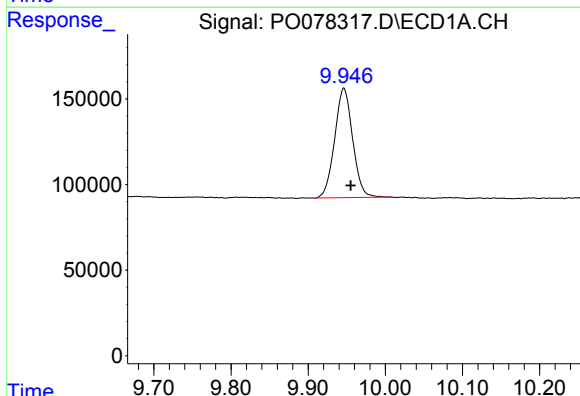


#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: -0.009 min
Response: 1035374
Conc: 20.94 ng/ml

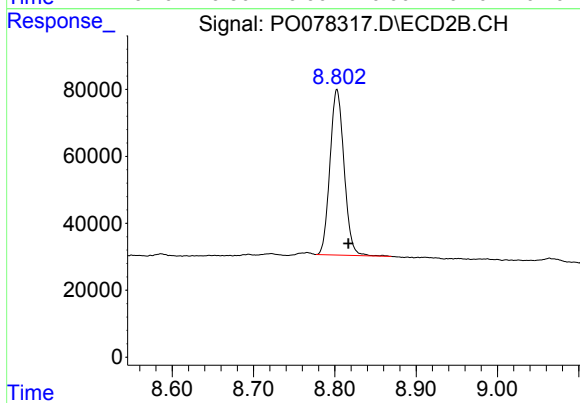

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.014 min
Response: 595823
Conc: 20.49 ng/ml

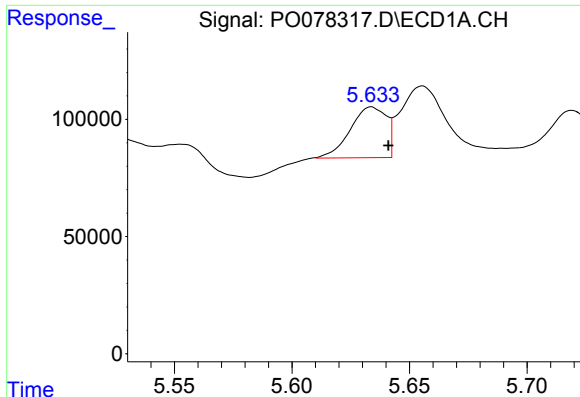


#16 AR-1242-1

R.T.: 5.633 min
Delta R.T.: -0.008 min
Response: 230080
Conc: 125.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PLA-120


Manual Integrations
APPROVED

Ankita
6/2/2021 10:24:14 AM

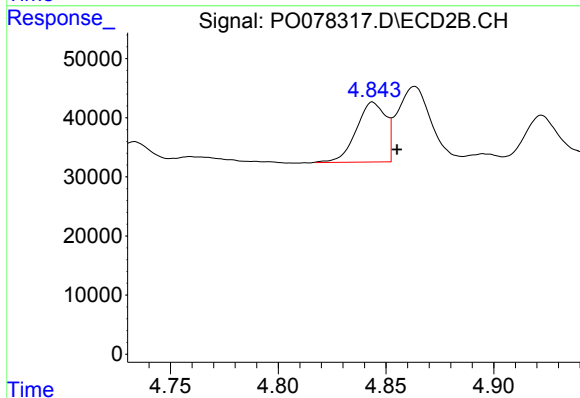


#16 AR-1242-1

R.T.: 4.843 min
Delta R.T.: -0.012 min
Response: 96580
Conc: 112.44 ng/ml m

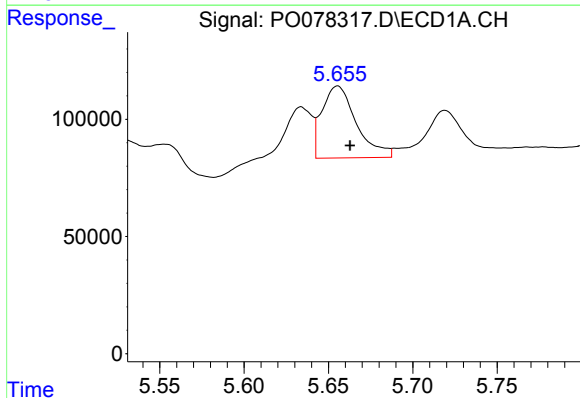


#17 AR-1242-2

R.T.: 5.655 min
Delta R.T.: -0.008 min
Response: 431079
Conc: 159.58 ng/ml m

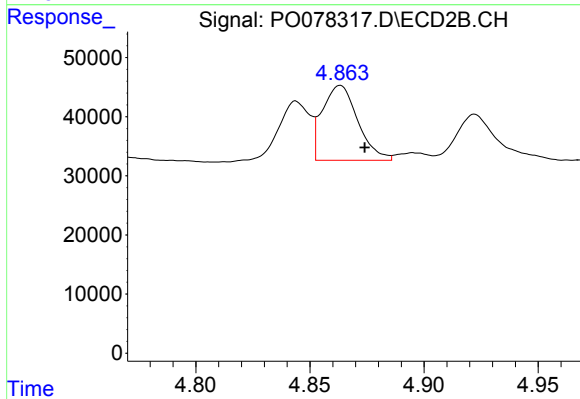

#17 AR-1242-2

R.T.: 4.863 min
Delta R.T.: -0.011 min
Response: 136931
Conc: 113.17 ng/ml

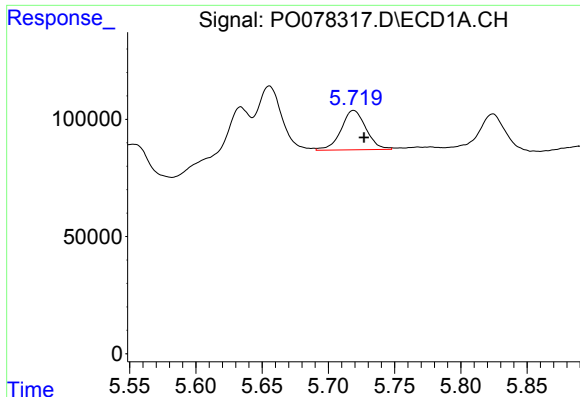


#18 AR-1242-3

R.T.: 5.719 min
Delta R.T.: -0.008 min
Response: 220916
Conc: 126.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PLA-120


Manual Integrations
APPROVED

Ankita
6/2/2021 10:24:14 AM

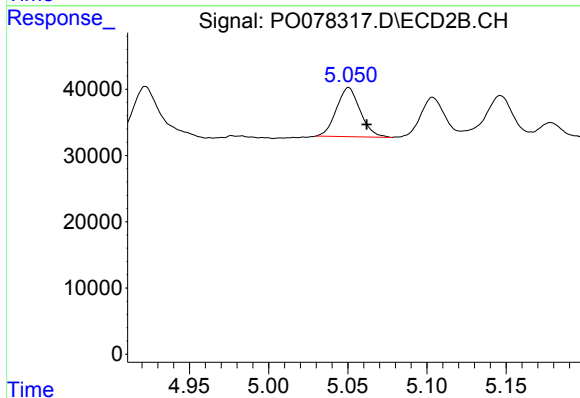


#18 AR-1242-3

R.T.: 5.051 min
Delta R.T.: -0.011 min
Response: 77443
Conc: 120.20 ng/ml

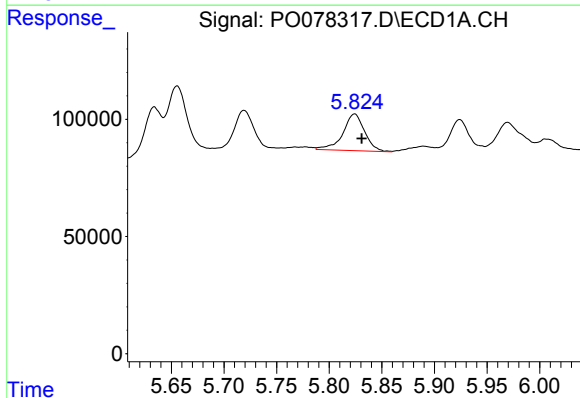


#19 AR-1242-4

R.T.: 5.824 min
Delta R.T.: -0.007 min
Response: 225408
Conc: 161.23 ng/ml m

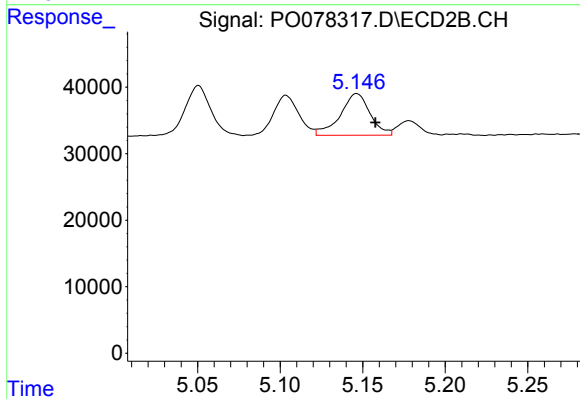

#19 AR-1242-4

R.T.: 5.146 min
Delta R.T.: -0.011 min
Response: 78757
Conc: 116.50 ng/ml

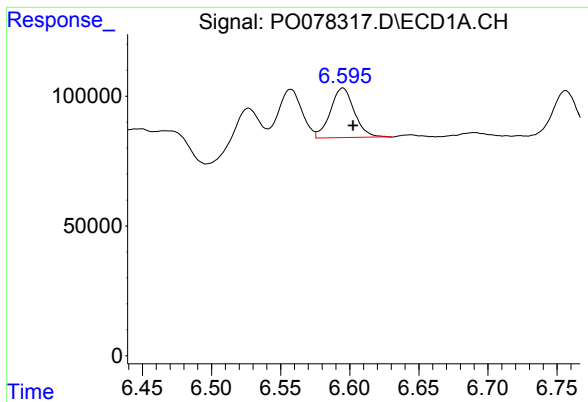


#20 AR-1242-5

R.T.: 6.595 min
Delta R.T.: -0.008 min
Response: 229332
Conc: 171.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PLA-120

Manual Integrations
APPROVED

Ankita
6/2/2021 10:24:14 AM

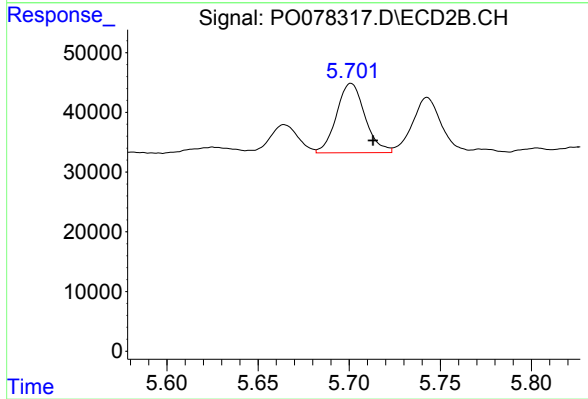

#20 AR-1242-5

R.T.: 5.701 min
Delta R.T.: -0.012 min
Response: 126435
Conc: 154.19 ng/ml