

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060122\
 Data File : P0086831.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jun 2022 13:46
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/06/2022
 Supervised By :Ankita Jodhani 06/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 01 14:15:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 14:13:22 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.515	3.666	261840	168915	4.144	4.708m
2)	SA Decachlor...	10.388	8.701	227411	116483	4.593	4.725
Target Compounds							
16)	L4 AR-1242-1	5.699	4.761	76530	39990	46.010	49.504
17)	L4 AR-1242-2	5.722	4.781	105554	53555	44.258	47.765
18)	L4 AR-1242-3	5.786	4.956	68292	30147	45.972	49.797
19)	L4 AR-1242-4	5.885	5.041	55151	29943	46.724	51.286
20)	L4 AR-1242-5	6.627	5.564	54086	32179	43.684	45.898

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060122\
Data File : P0086831.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jun 2022 13:46
Operator : YP\AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2022
Supervised By :Ankita Jodhani 06/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 01 14:15:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 14:13:22 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

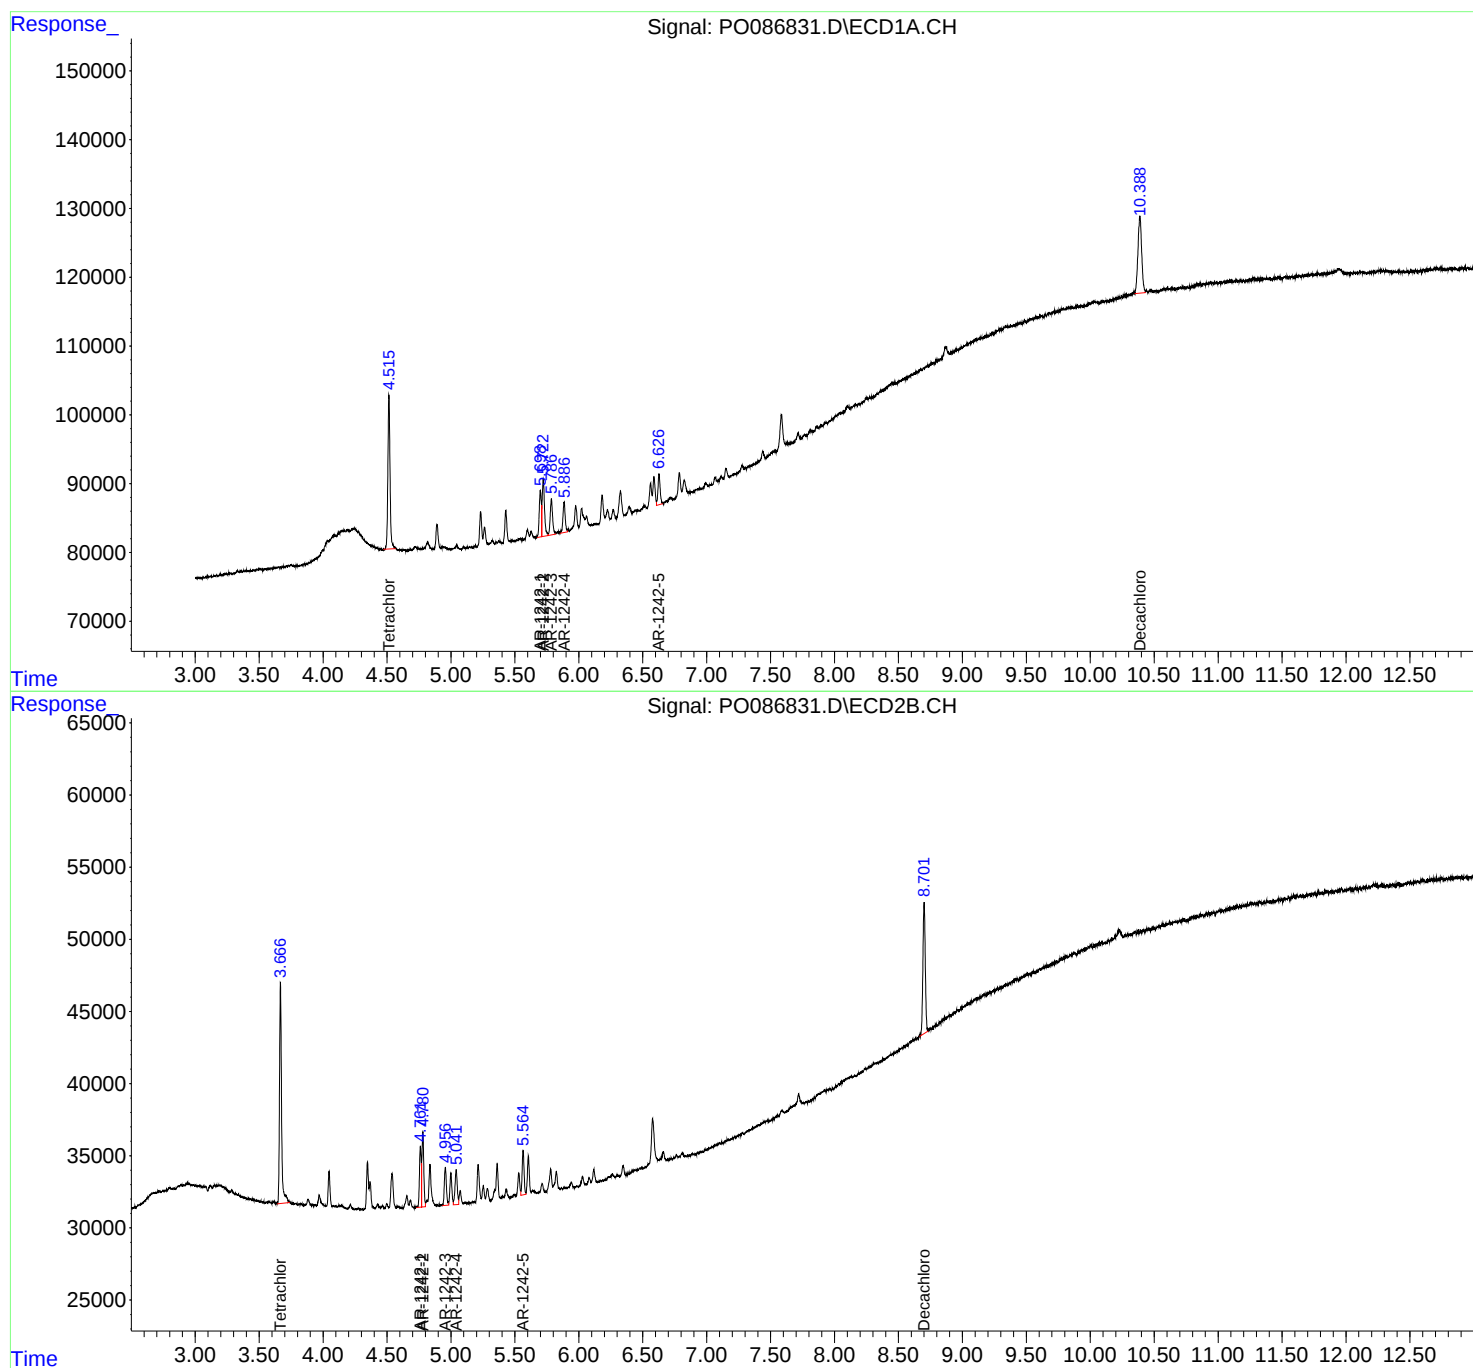

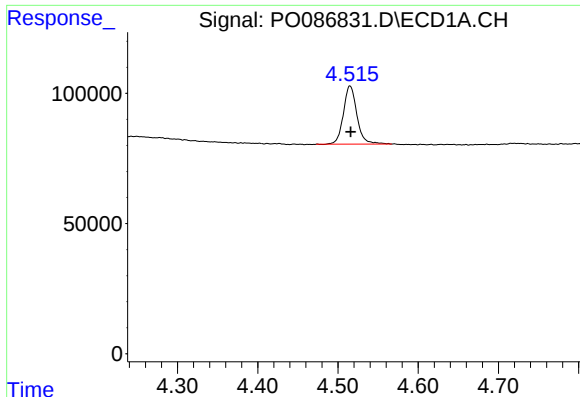


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: -0.001 min
Response: 261840
Conc: 4.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2022
Supervised By :Ankita Jodhani 06/06/2022

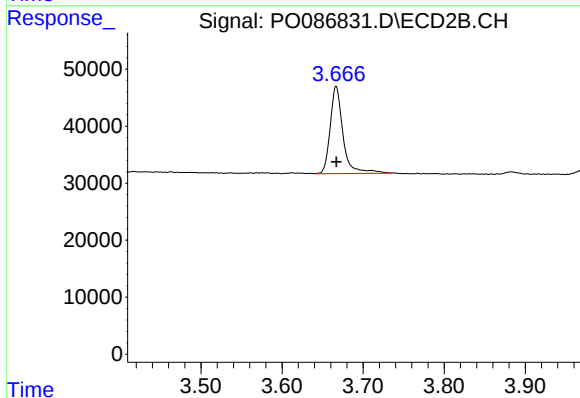


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: 0.000 min
Response: 168915
Conc: 4.71 ng/ml m

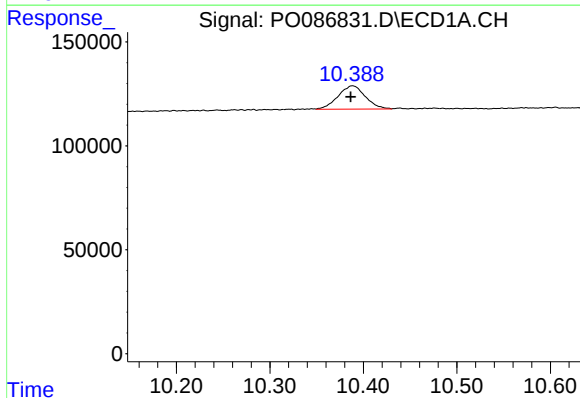


#2 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: 0.002 min
Response: 227411
Conc: 4.59 ng/ml

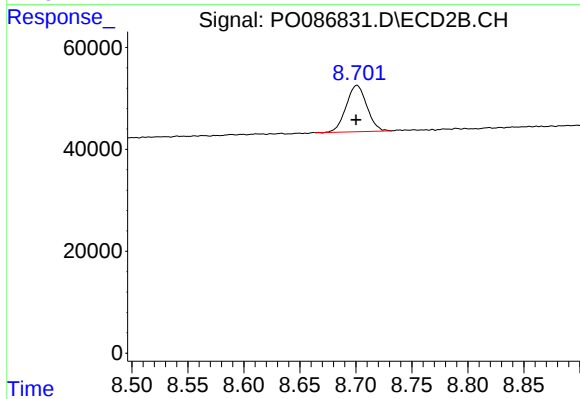

#2 Decachlorobiphenyl

R.T.: 8.701 min
Delta R.T.: 0.000 min
Response: 116483
Conc: 4.73 ng/ml

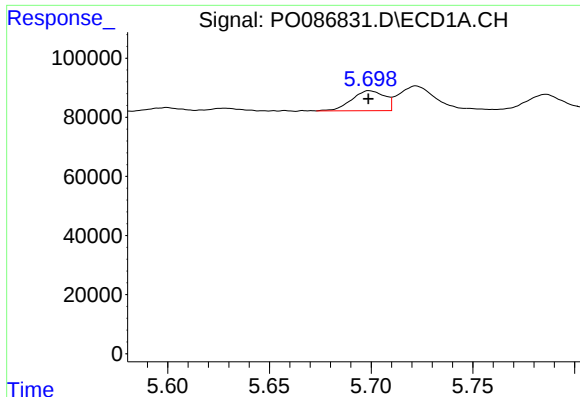


#16 AR-1242-1

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 76530
Conc: 46.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2022
Supervised By :Ankita Jodhani 06/06/2022

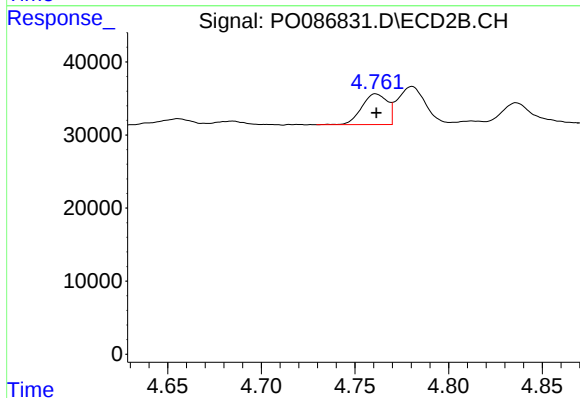


#16 AR-1242-1

R.T.: 4.761 min
Delta R.T.: 0.000 min
Response: 39990
Conc: 49.50 ng/ml

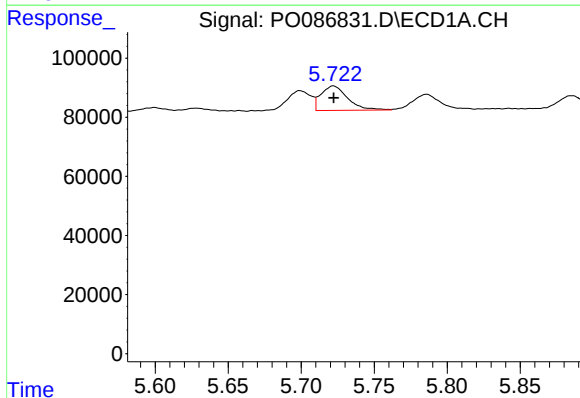


#17 AR-1242-2

R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 105554
Conc: 44.26 ng/ml

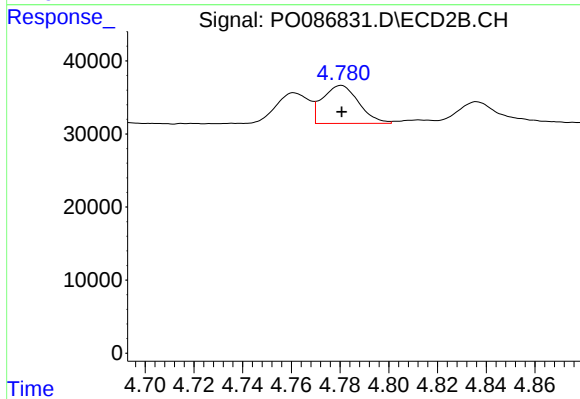

#17 AR-1242-2

R.T.: 4.781 min
Delta R.T.: 0.000 min
Response: 53555
Conc: 47.77 ng/ml

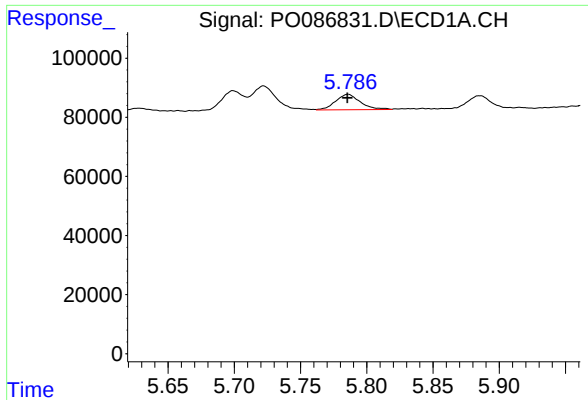


#18 AR-1242-3

R.T.: 5.786 min
Delta R.T.: 0.000 min
Response: 68292
Conc: 45.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2022
Supervised By :Ankita Jodhani 06/06/2022

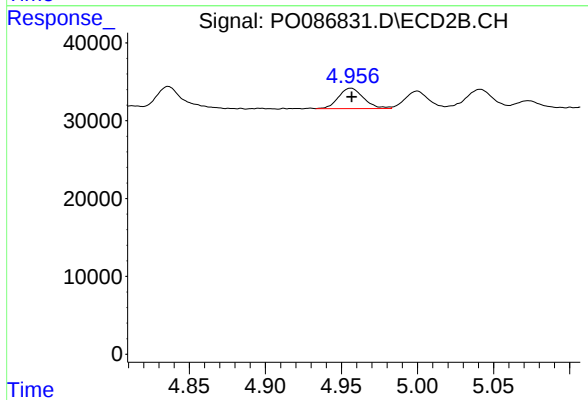


#18 AR-1242-3

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 30147
Conc: 49.80 ng/ml

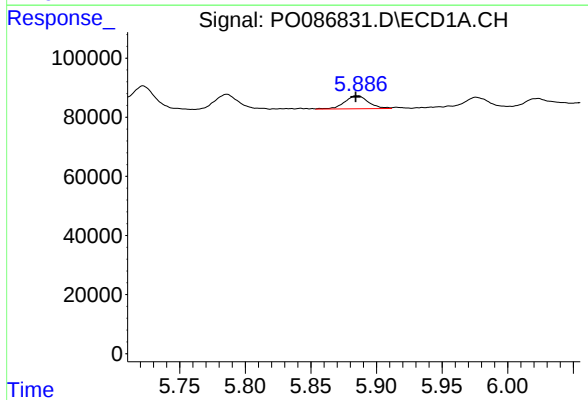


#19 AR-1242-4

R.T.: 5.885 min
Delta R.T.: 0.000 min
Response: 55151
Conc: 46.72 ng/ml

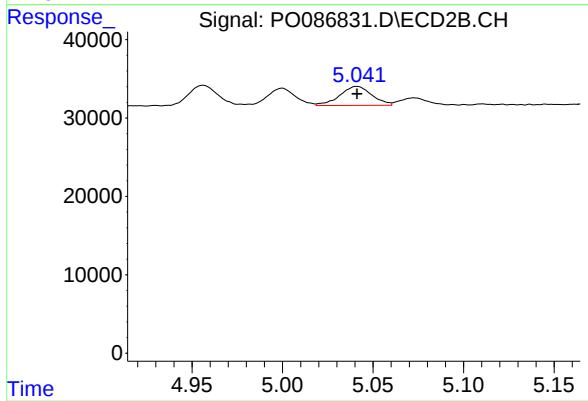

#19 AR-1242-4

R.T.: 5.041 min
Delta R.T.: 0.000 min
Response: 29943
Conc: 51.29 ng/ml

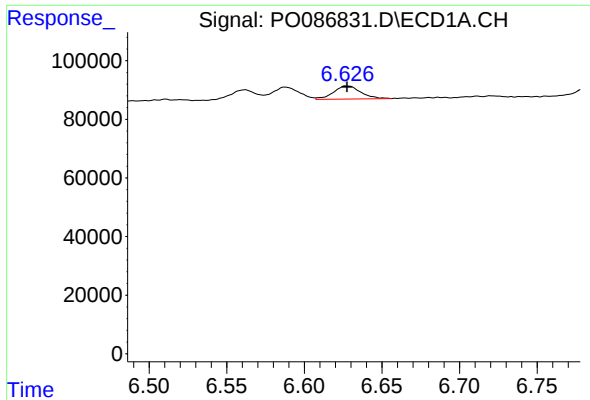


#20 AR-1242-5

R.T.: 6.627 min
Delta R.T.: 0.000 min
Response: 54086
Conc: 43.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2022
Supervised By :Ankita Jodhani 06/06/2022

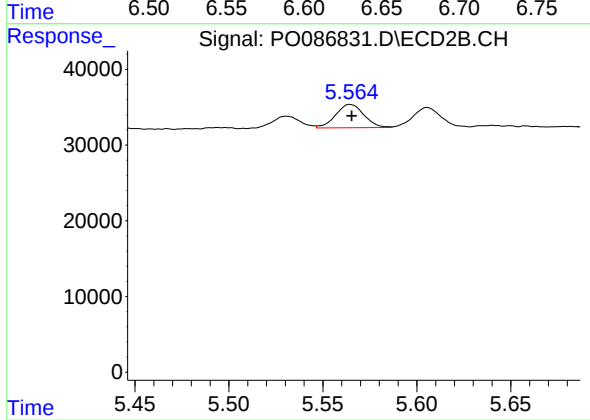

#20 AR-1242-5

R.T.: 5.564 min
Delta R.T.: 0.000 min
Response: 32179
Conc: 45.90 ng/ml