

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078331.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 9:49
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:19:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:48:46 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.340	3.617	3443855	1450317	46.597	47.998
2)	SA Decachlor...	9.948	8.804	2290361	1316204	46.325	45.265
Target Compounds							
21)	L5 AR-1248-1	5.635	4.845	656255	319209	460.561	495.326m
22)	L5 AR-1248-2	5.925	5.105	903536	429434	475.921	449.225
23)	L5 AR-1248-3	6.136	5.147	1050560	435627	473.642	453.195
24)	L5 AR-1248-4	6.559	5.328	1190015	506867	511.254	442.577
25)	L5 AR-1248-5	6.596	5.743	1174038	506474	518.895	483.347

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
Data File : P0078331.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 9:49
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:48:46 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

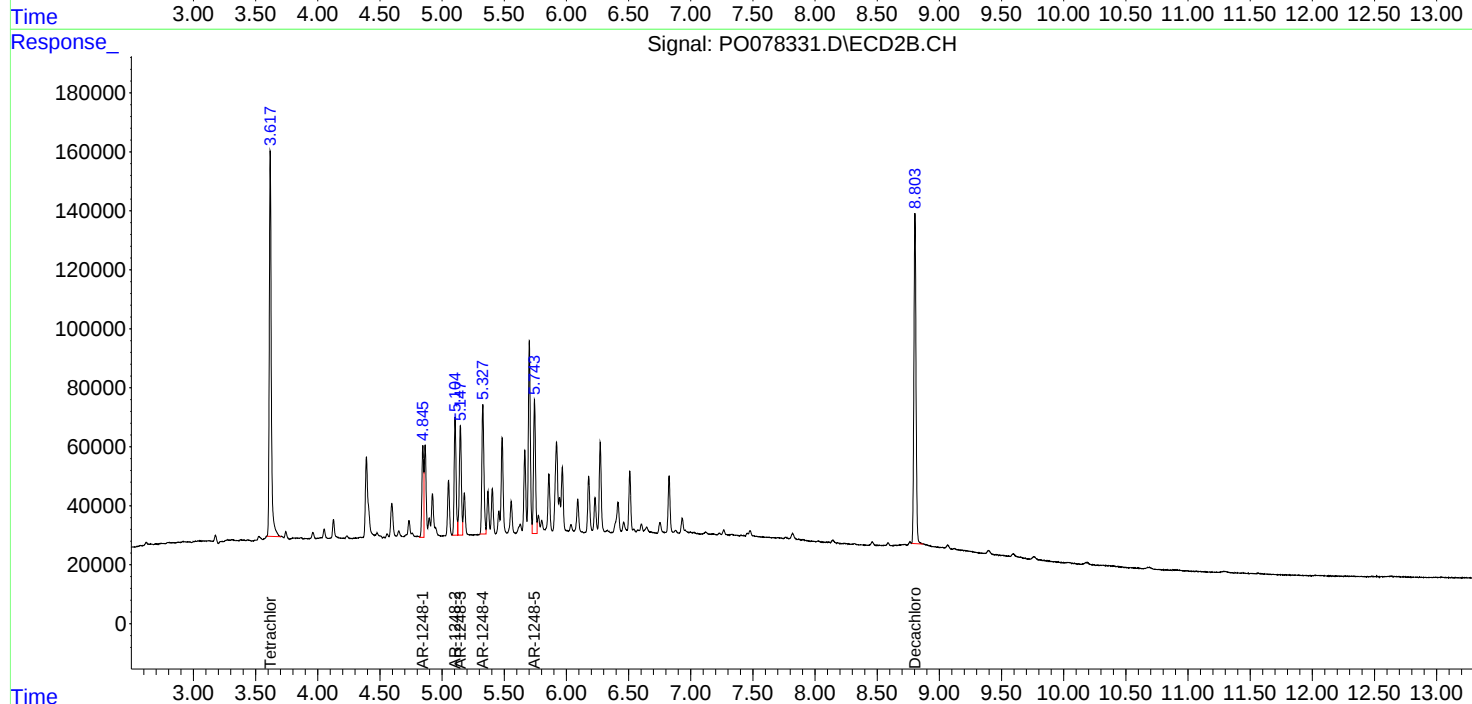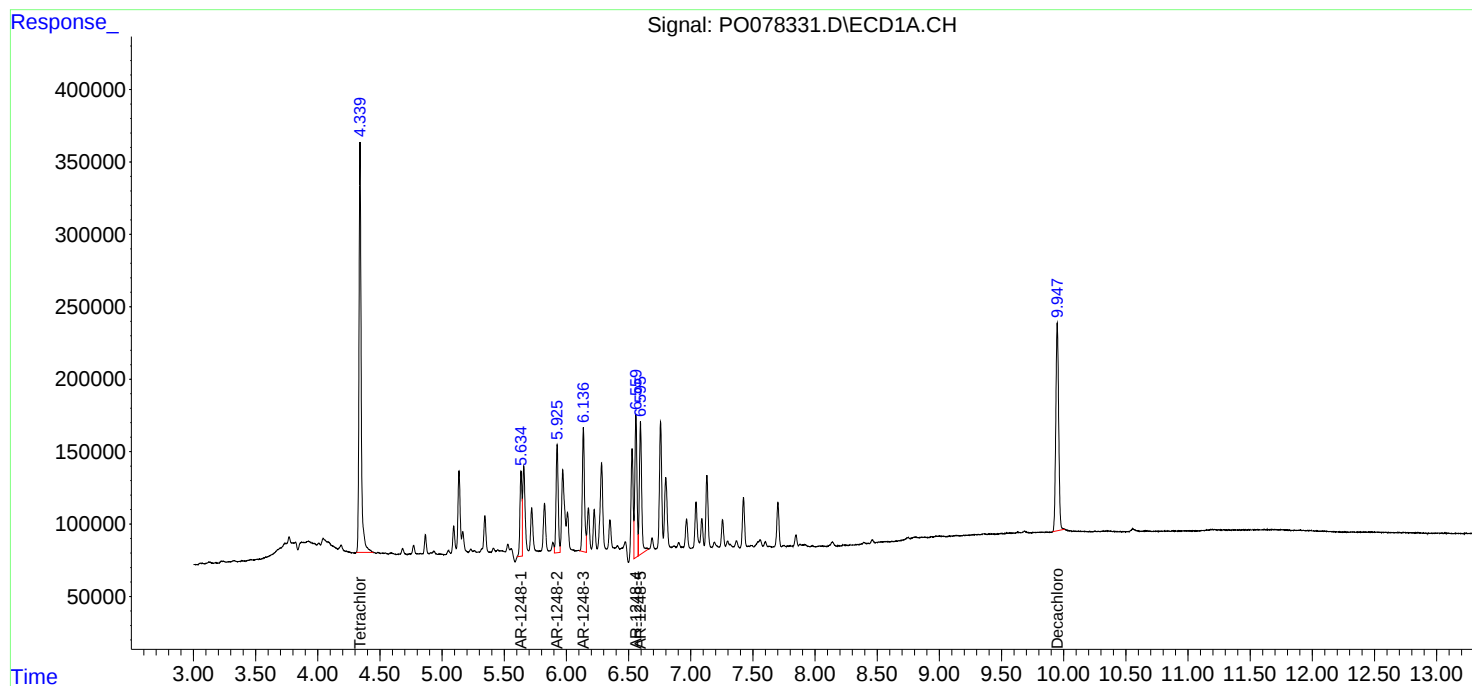

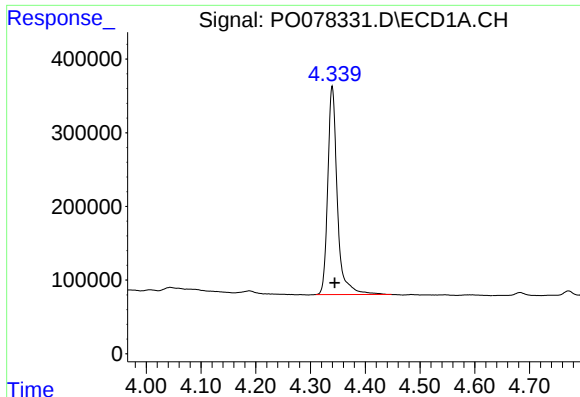


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 3443855
Conc: 46.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:10 PM

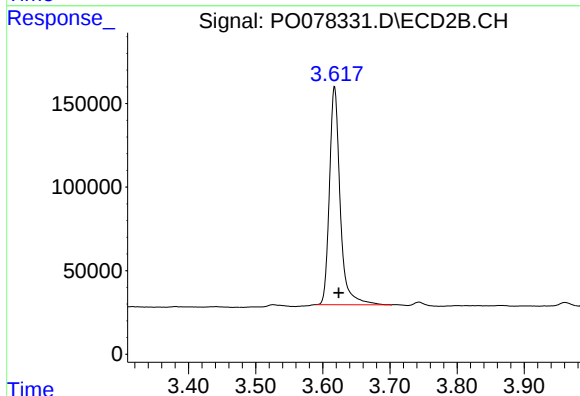


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.006 min
Response: 1450317
Conc: 48.00 ng/ml

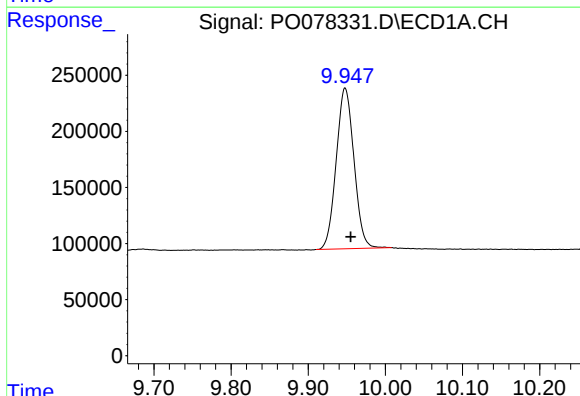


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.007 min
Response: 2290361
Conc: 46.33 ng/ml

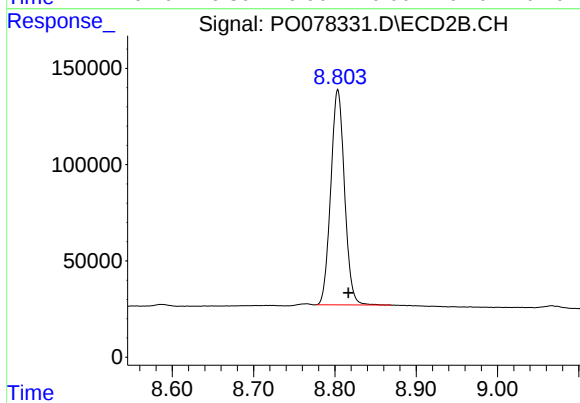

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.013 min
Response: 1316204
Conc: 45.27 ng/ml

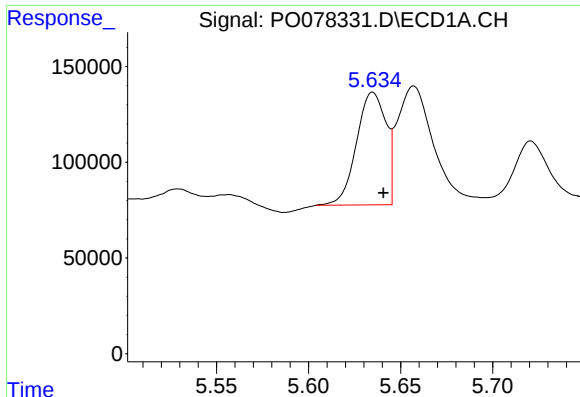


#21 AR-1248-1

R.T.: 5.635 min
Delta R.T.: -0.006 min
Response: 656255
Conc: 460.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:10 PM

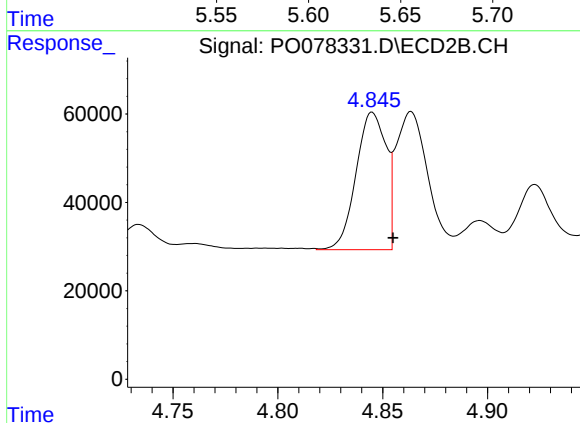


#21 AR-1248-1

R.T.: 4.845 min
Delta R.T.: -0.010 min
Response: 319209
Conc: 495.33 ng/ml m

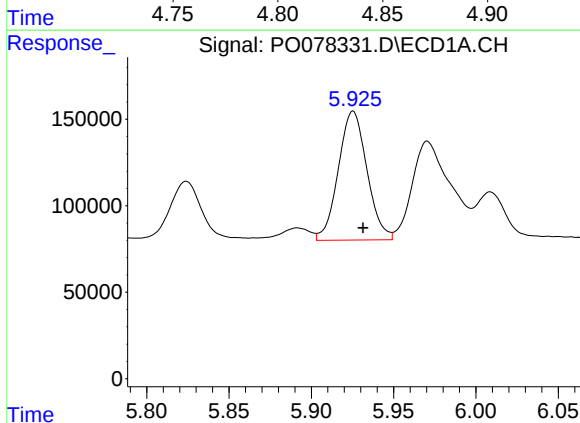


#22 AR-1248-2

R.T.: 5.925 min
Delta R.T.: -0.006 min
Response: 903536
Conc: 475.92 ng/ml

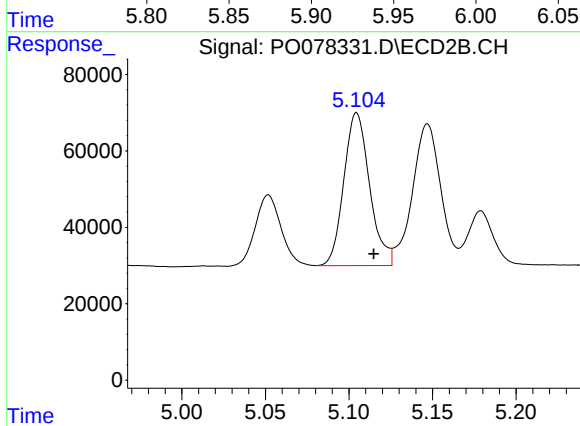

#22 AR-1248-2

R.T.: 5.105 min
Delta R.T.: -0.010 min
Response: 429434
Conc: 449.22 ng/ml

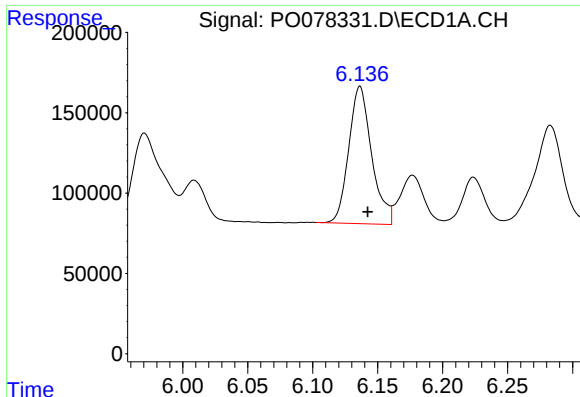


#23 AR-1248-3

R.T.: 6.136 min
Delta R.T.: -0.006 min
Response: 1050560
Conc: 473.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:10 PM

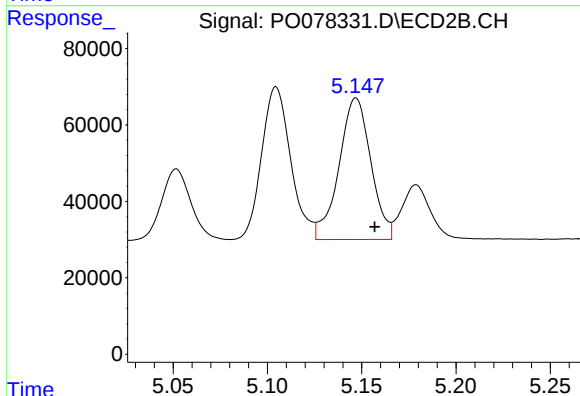


#23 AR-1248-3

R.T.: 5.147 min
Delta R.T.: -0.010 min
Response: 435627
Conc: 453.19 ng/ml

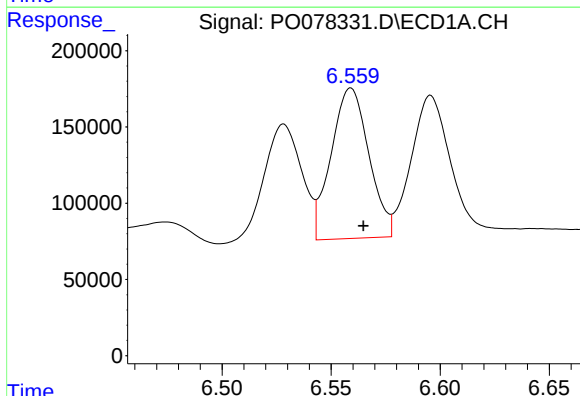


#24 AR-1248-4

R.T.: 6.559 min
Delta R.T.: -0.006 min
Response: 1190015
Conc: 511.25 ng/ml

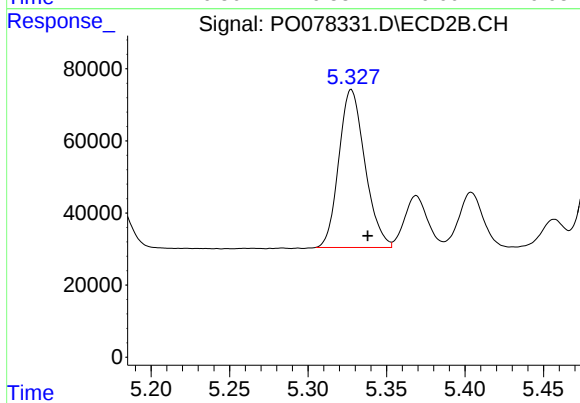

#24 AR-1248-4

R.T.: 5.328 min
Delta R.T.: -0.010 min
Response: 506867
Conc: 442.58 ng/ml

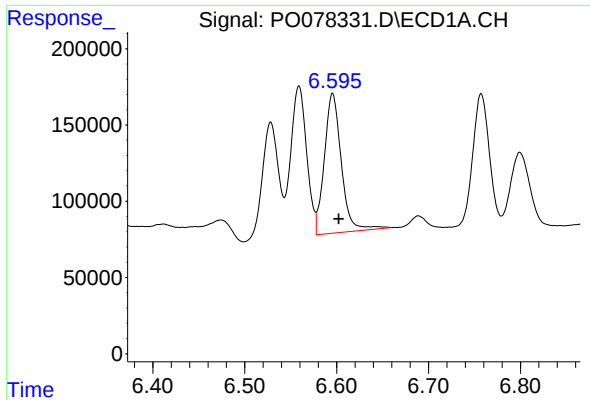


#25 AR-1248-5

R.T.: 6.596 min
Delta R.T.: -0.007 min
Response: 1174038
Conc: 518.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:10 PM

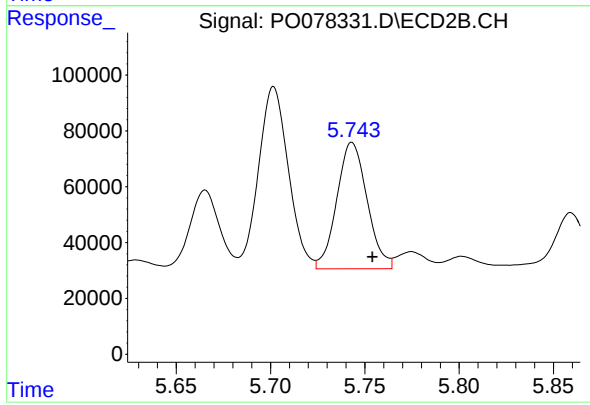

#25 AR-1248-5

R.T.: 5.743 min
Delta R.T.: -0.011 min
Response: 506474
Conc: 483.35 ng/ml