

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078334.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 10:40
 Operator : DD\AJ
 Sample : M2563-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 33213-14

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:19:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 07:19:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.338	3.616	1563815	696238	21.159	23.042
2)	SA Decachlor...	9.948	8.803	1200297	692507	24.277	23.816
Target Compounds							
21)	L5 AR-1248-1	5.634	4.844	433301	197445	304.091	306.380m
22)	L5 AR-1248-2	5.925	5.104	330298	154405	173.978	161.520
23)	L5 AR-1248-3	6.136	5.146	409552	185388	184.645	192.864
24)	L5 AR-1248-4	6.558	5.327	282200	201586	121.238	176.018 #
25)	L5 AR-1248-5	6.596	5.741	266727	93398	117.887	89.134m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
Data File : P0078334.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 10:40
Operator : DD\AJ
Sample : M2563-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
33213-14


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 07:19:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

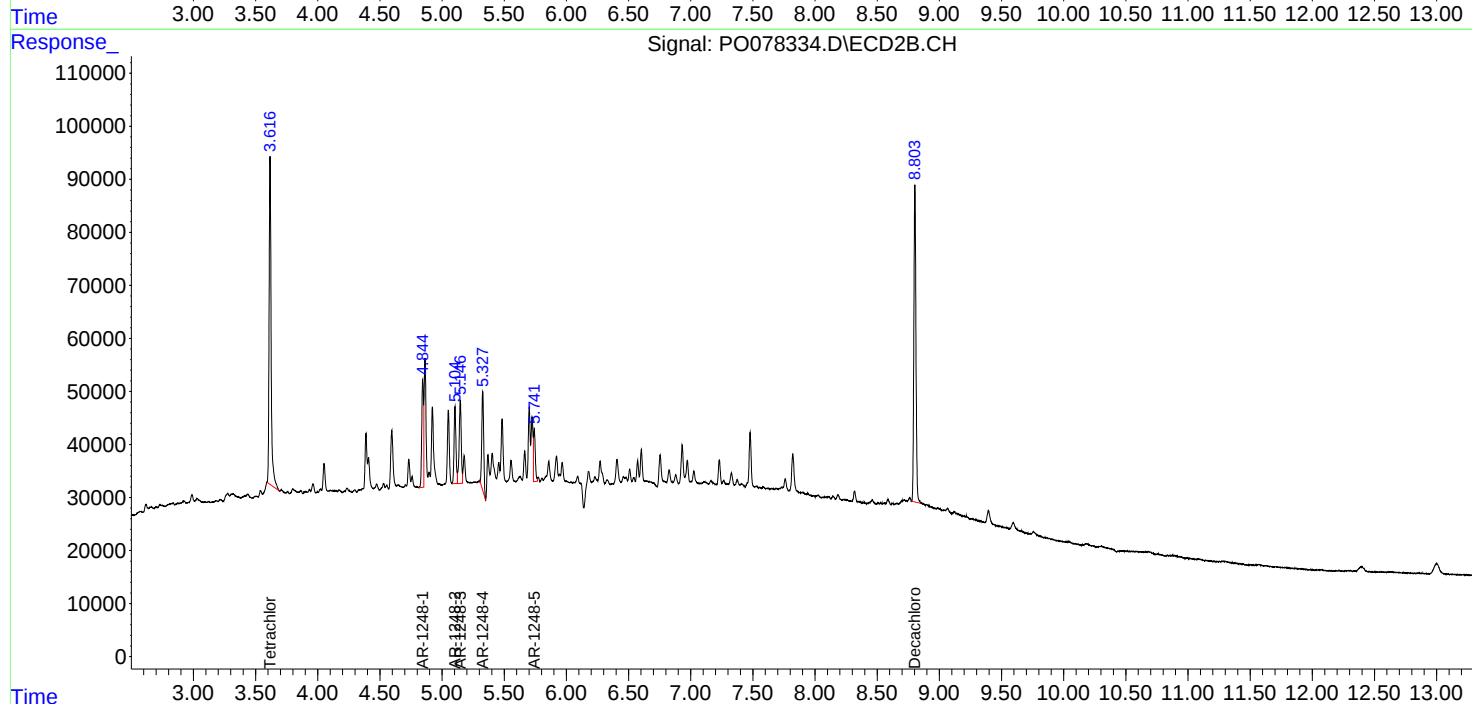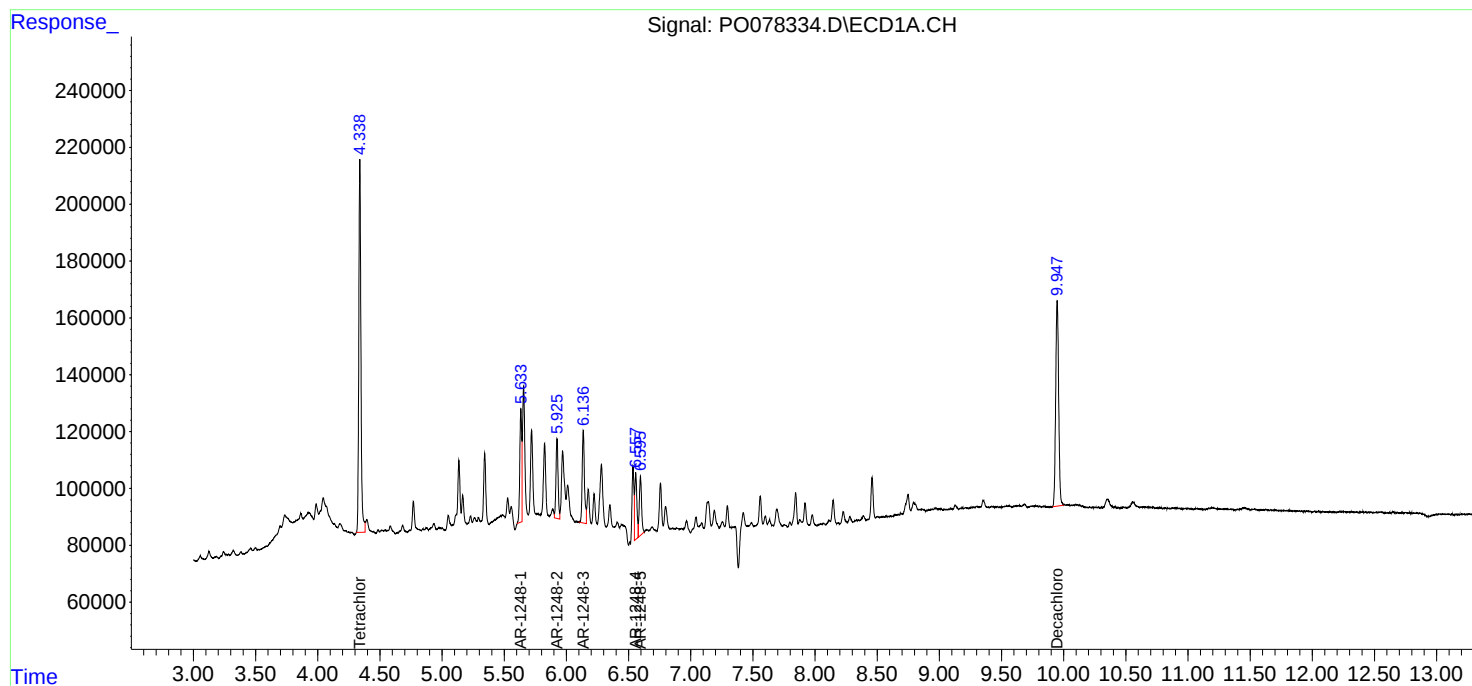

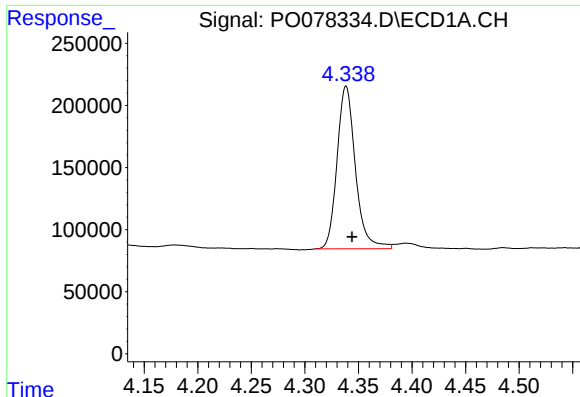


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 1563815
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
33213-14


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:40 PM

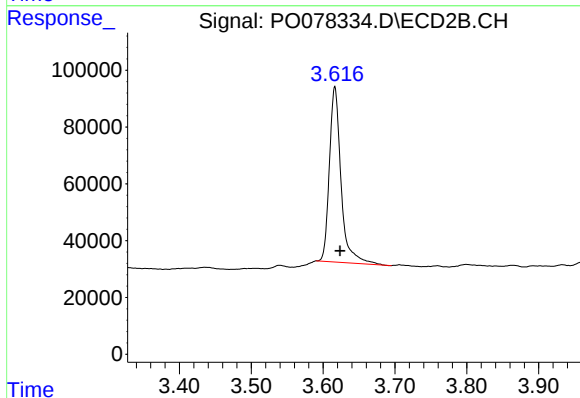


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.007 min
Response: 696238
Conc: 23.04 ng/ml

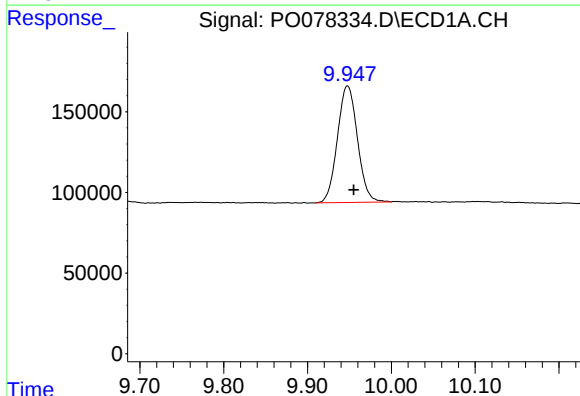


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.007 min
Response: 1200297
Conc: 24.28 ng/ml

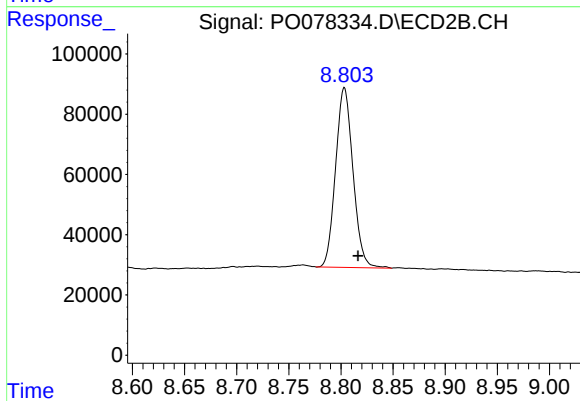

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.013 min
Response: 692507
Conc: 23.82 ng/ml

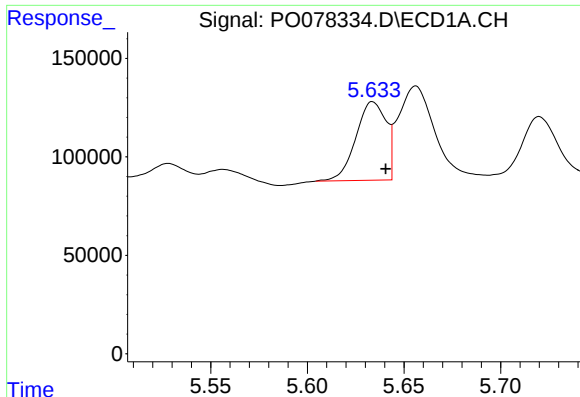


#21 AR-1248-1

R.T.: 5.634 min
Delta R.T.: -0.007 min
Response: 433301
Conc: 304.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
33213-14


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:40 PM

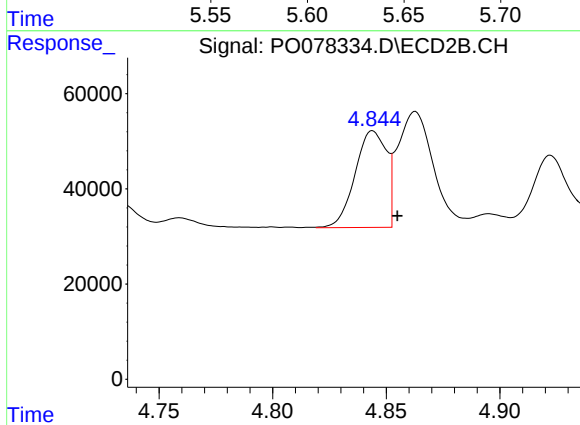


#21 AR-1248-1

R.T.: 4.844 min
Delta R.T.: -0.011 min
Response: 197445
Conc: 306.38 ng/ml m

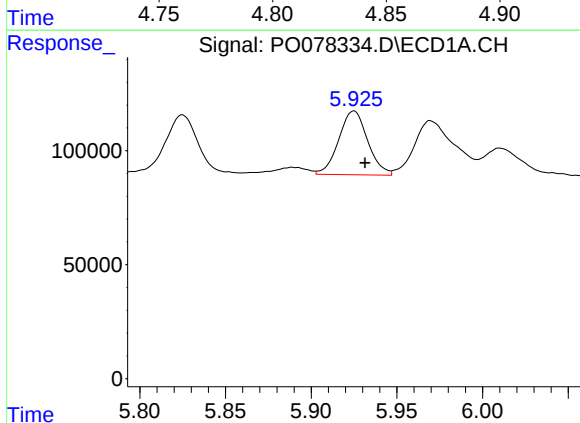


#22 AR-1248-2

R.T.: 5.925 min
Delta R.T.: -0.006 min
Response: 330298
Conc: 173.98 ng/ml

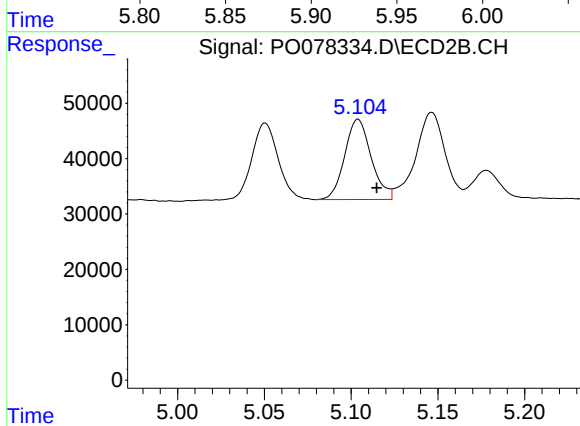

#22 AR-1248-2

R.T.: 5.104 min
Delta R.T.: -0.011 min
Response: 154405
Conc: 161.52 ng/ml

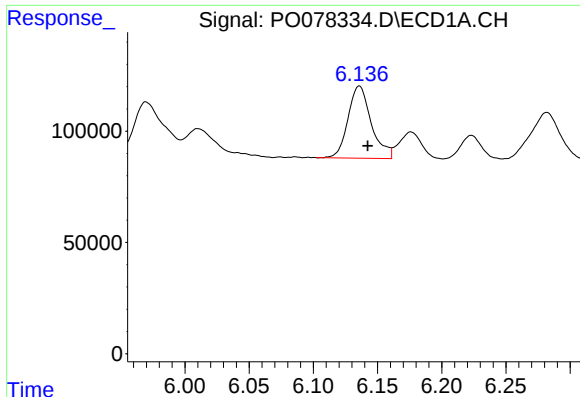


#23 AR-1248-3

R.T.: 6.136 min
Delta R.T.: -0.007 min
Response: 409552
Conc: 184.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
33213-14


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:40 PM

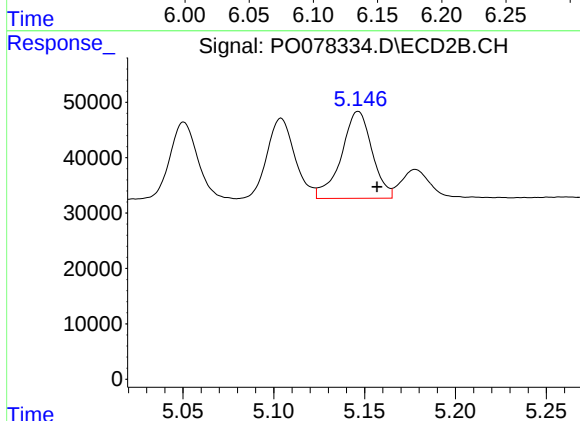


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: -0.010 min
Response: 185388
Conc: 192.86 ng/ml

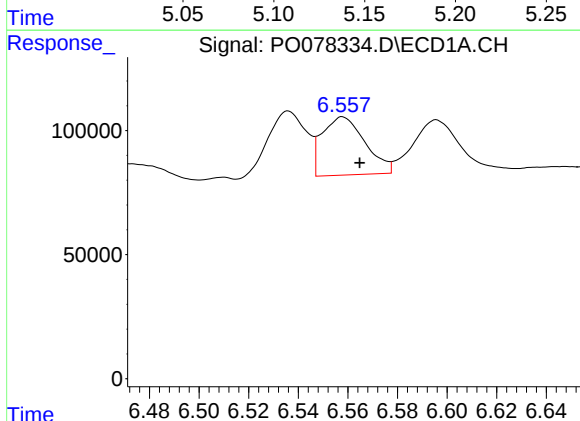


#24 AR-1248-4

R.T.: 6.558 min
Delta R.T.: -0.007 min
Response: 282200
Conc: 121.24 ng/ml

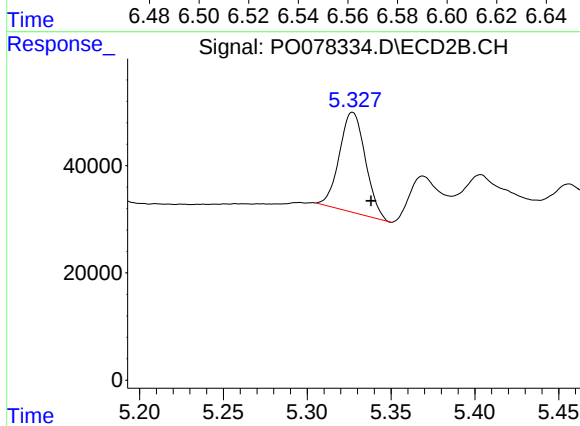

#24 AR-1248-4

R.T.: 5.327 min
Delta R.T.: -0.011 min
Response: 201586
Conc: 176.02 ng/ml

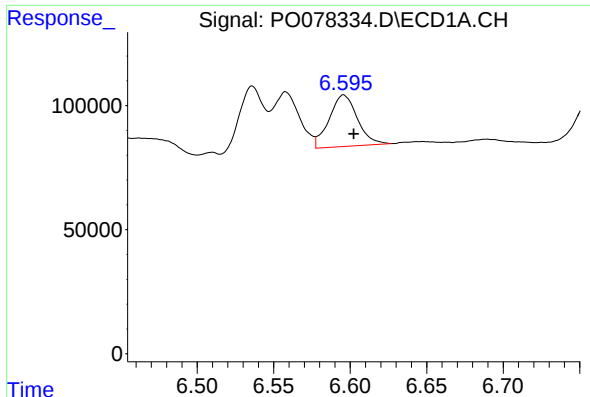


#25 AR-1248-5

R.T.: 6.596 min
Delta R.T.: -0.007 min
Response: 266727
Conc: 117.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
33213-14

Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:40 PM

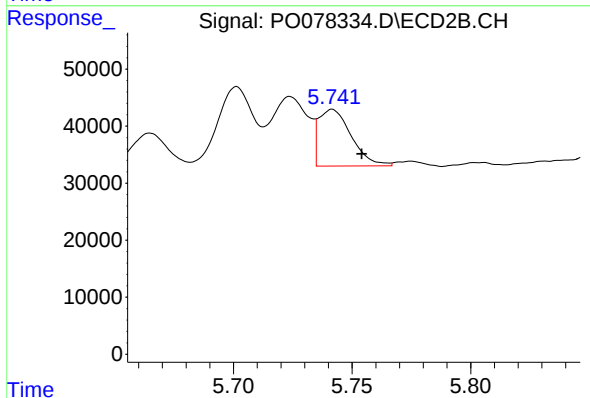

#25 AR-1248-5

R.T.: 5.741 min
Delta R.T.: -0.013 min
Response: 93398
Conc: 89.13 ng/ml m