

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078338.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 11:49
 Operator : DD\AJ
 Sample : M2563-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PLA-118

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:19:17 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:55:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.616	1363682	606296	18.451	20.065
2) SA Decachlor...	9.947	8.803	1071455	624219	21.672	21.467
Target Compounds						
21) L5 AR-1248-1	5.633	4.844	382242	182933	268.258	283.862m
22) L5 AR-1248-2	5.924	5.104	174327	85873	91.823	89.831
23) L5 AR-1248-3	6.135	5.146	151277	100620	68.203	104.677 #
24) L5 AR-1248-4	6.559	5.326	105408	96168	45.285m	83.970 #
25) L5 AR-1248-5	6.596	5.742	109936	19443	48.589m	18.555 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
Data File : P0078338.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 11:49
Operator : DD\AJ
Sample : M2563-10
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PLA-118


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:17 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:55:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

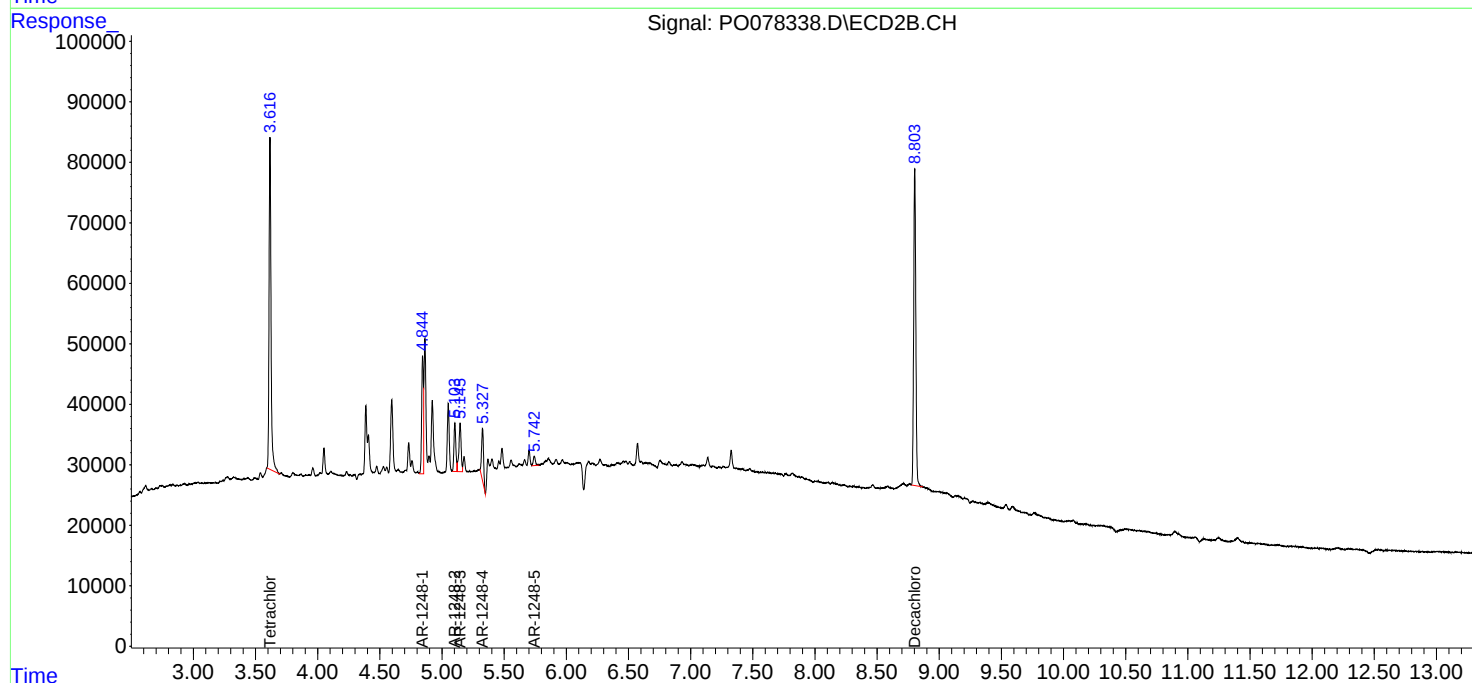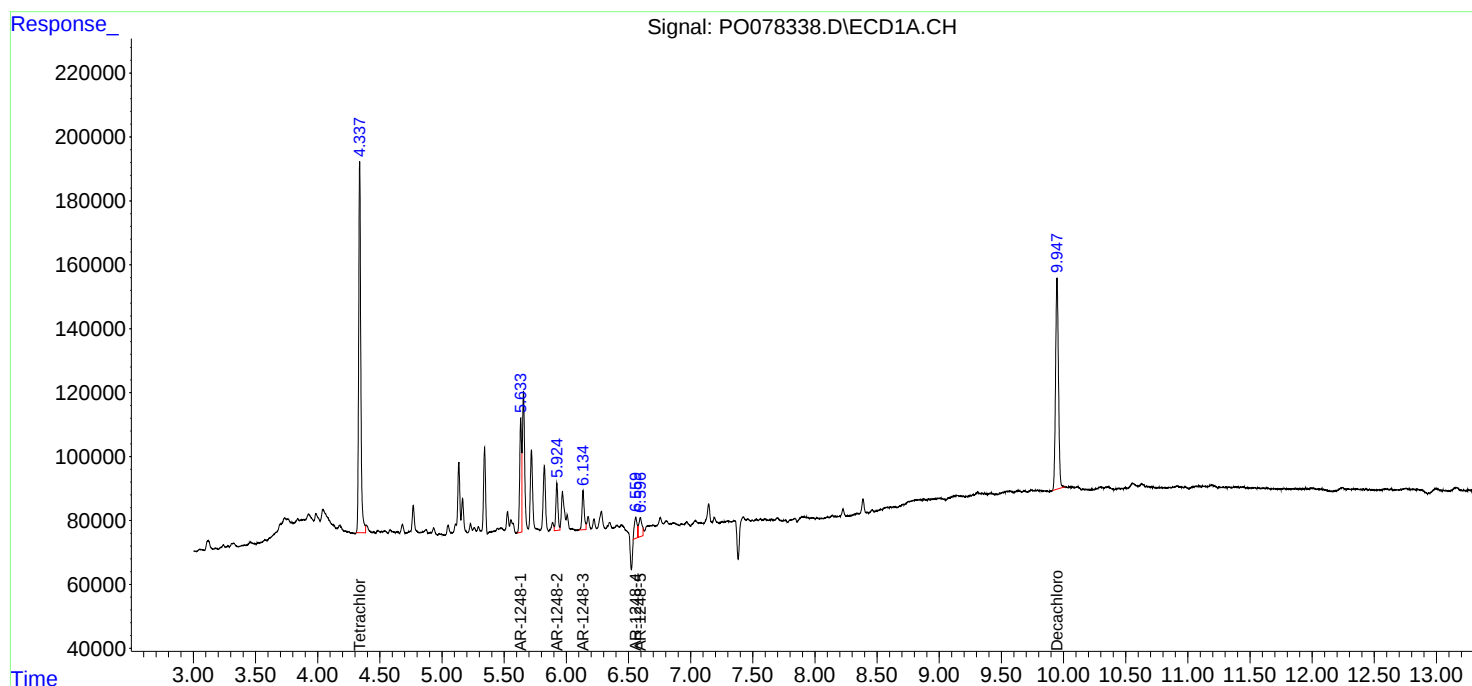

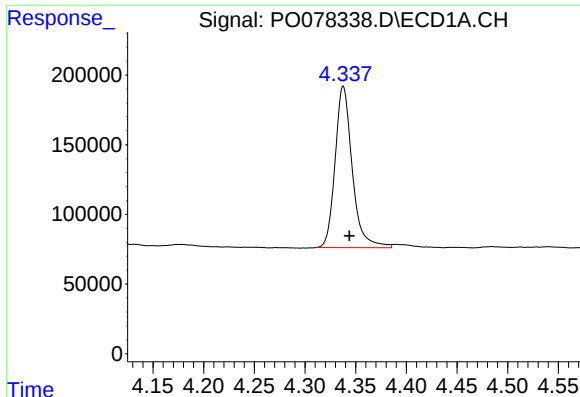


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 1363682
Conc: 18.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-118


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:17 PM

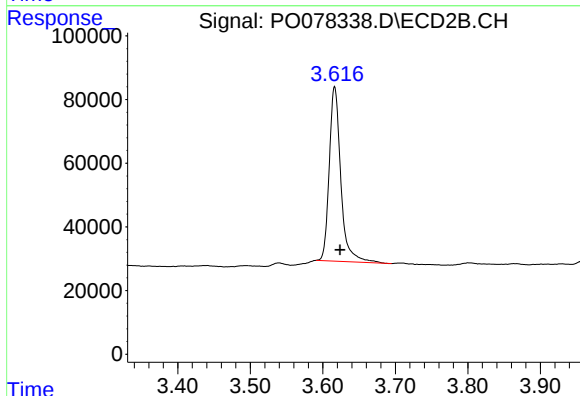


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.007 min
Response: 606296
Conc: 20.07 ng/ml

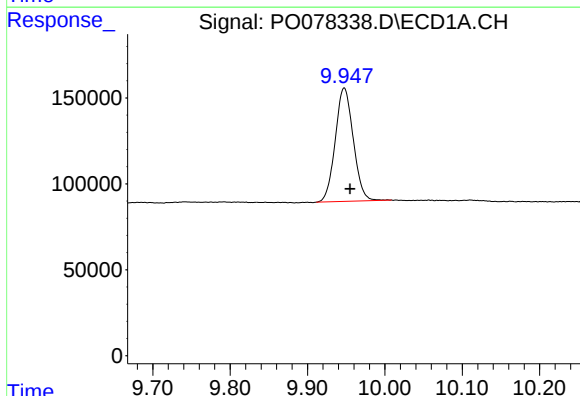


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 1071455
Conc: 21.67 ng/ml

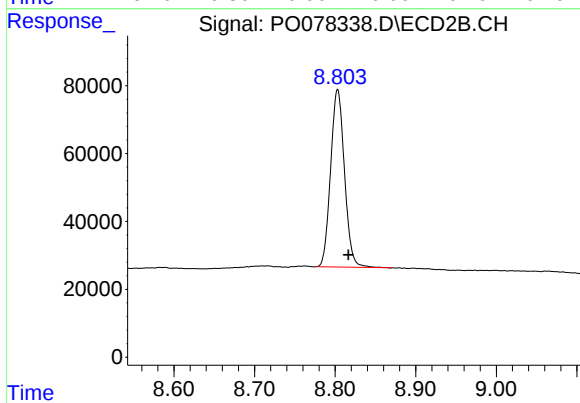

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.013 min
Response: 624219
Conc: 21.47 ng/ml

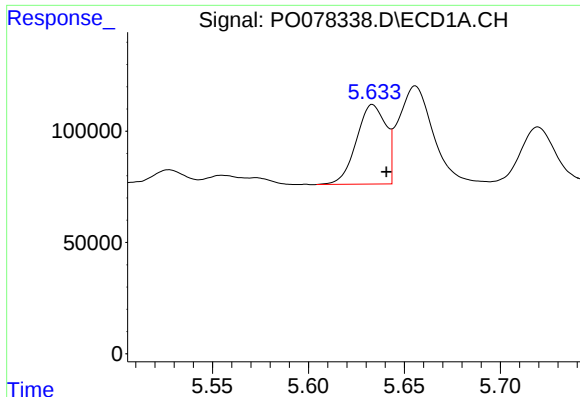


#21 AR-1248-1

R.T.: 5.633 min
Delta R.T.: -0.007 min
Response: 382242
Conc: 268.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-118


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:17 PM

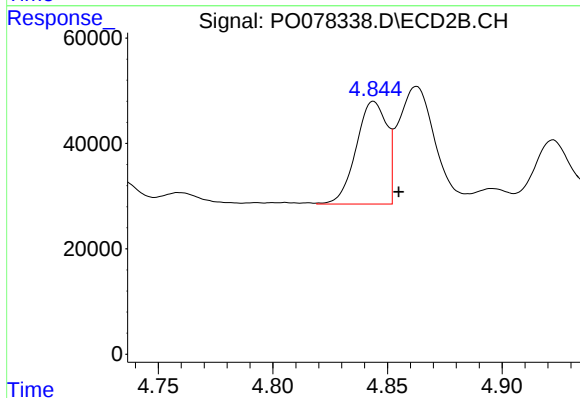


#21 AR-1248-1

R.T.: 4.844 min
Delta R.T.: -0.011 min
Response: 182933
Conc: 283.86 ng/ml m

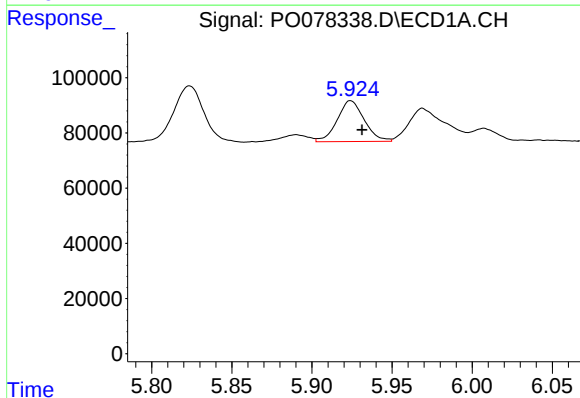


#22 AR-1248-2

R.T.: 5.924 min
Delta R.T.: -0.007 min
Response: 174327
Conc: 91.82 ng/ml

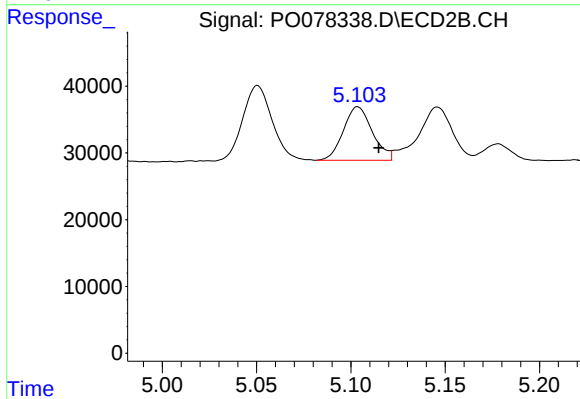

#22 AR-1248-2

R.T.: 5.104 min
Delta R.T.: -0.011 min
Response: 85873
Conc: 89.83 ng/ml

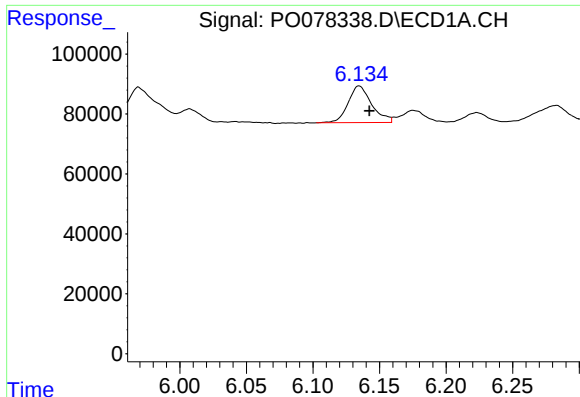


#23 AR-1248-3

R.T.: 6.135 min
Delta R.T.: -0.008 min
Response: 151277
Conc: 68.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-118


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:17 PM

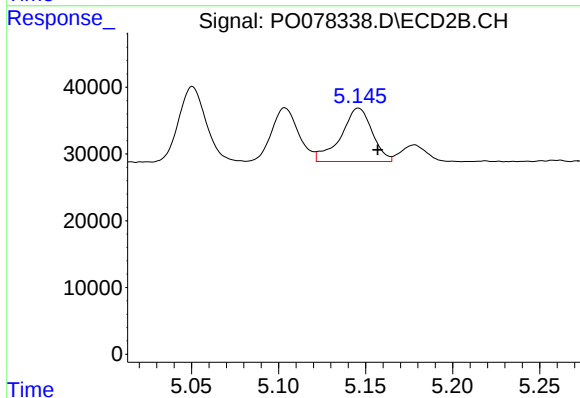


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: -0.011 min
Response: 100620
Conc: 104.68 ng/ml

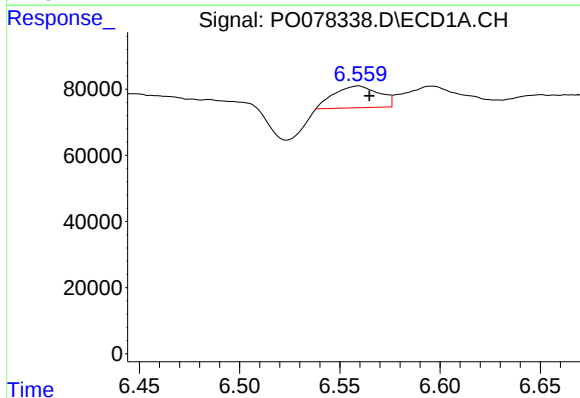


#24 AR-1248-4

R.T.: 6.559 min
Delta R.T.: -0.006 min
Response: 105408
Conc: 45.29 ng/ml m

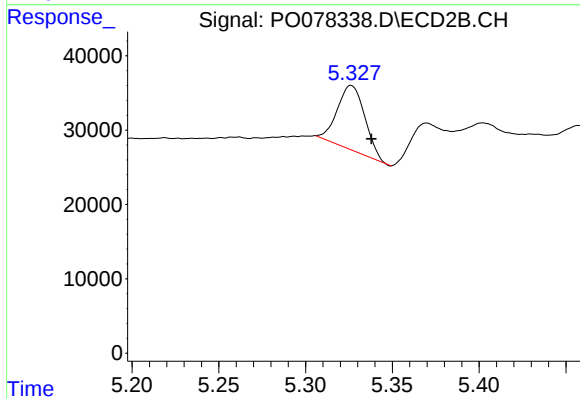

#24 AR-1248-4

R.T.: 5.326 min
Delta R.T.: -0.012 min
Response: 96168
Conc: 83.97 ng/ml

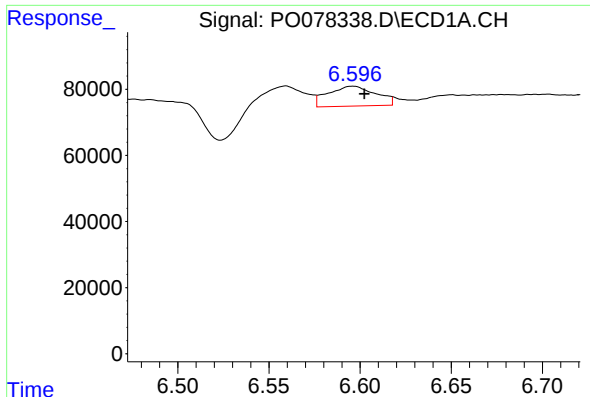


#25 AR-1248-5

R.T.: 6.596 min
Delta R.T.: -0.007 min
Response: 109936
Conc: 48.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PLA-118

Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:17 PM

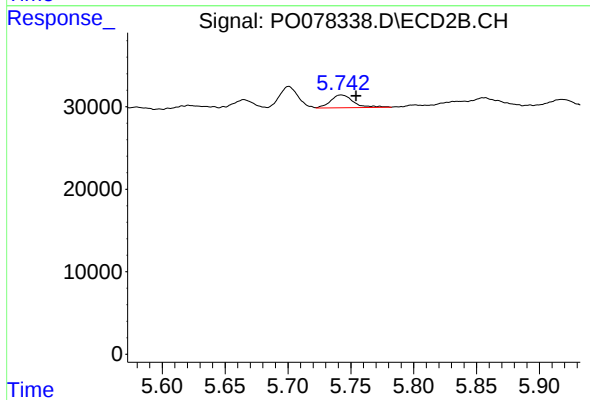

#25 AR-1248-5

R.T.: 5.742 min
Delta R.T.: -0.012 min
Response: 19443
Conc: 18.55 ng/ml