

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078339.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 12:06
 Operator : DD\AJ
 Sample : M2563-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PLA-119

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:19:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 05:55:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.339	3.617	1373734	599534	18.587	19.841
2)	SA Decachlor...	9.949	8.803	1014533	595970	20.520	20.496
Target Compounds							
21)	L5 AR-1248-1	5.634	4.844	125266	59617	87.912	92.509m
22)	L5 AR-1248-2	5.925	5.104	98314	44010	51.785	46.039
23)	L5 AR-1248-3	6.135	5.146	129055	52325	58.184	54.435
24)	L5 AR-1248-4	6.559	5.327	208821	70269	89.713	61.356 #
25)	L5 AR-1248-5	6.596	5.743	199080	66728	87.988	63.681 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
Data File : P0078339.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 12:06
Operator : DD\AJ
Sample : M2563-11
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
PLA-119


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 05:55:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

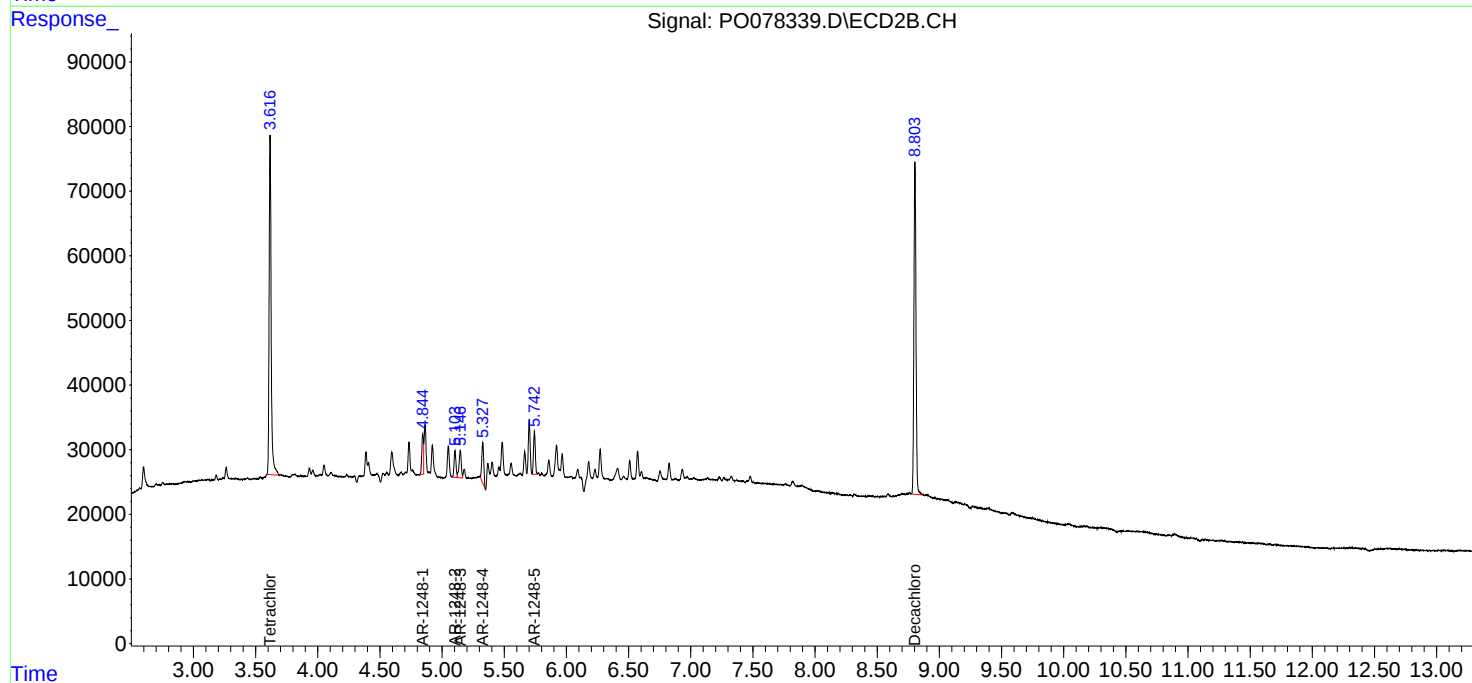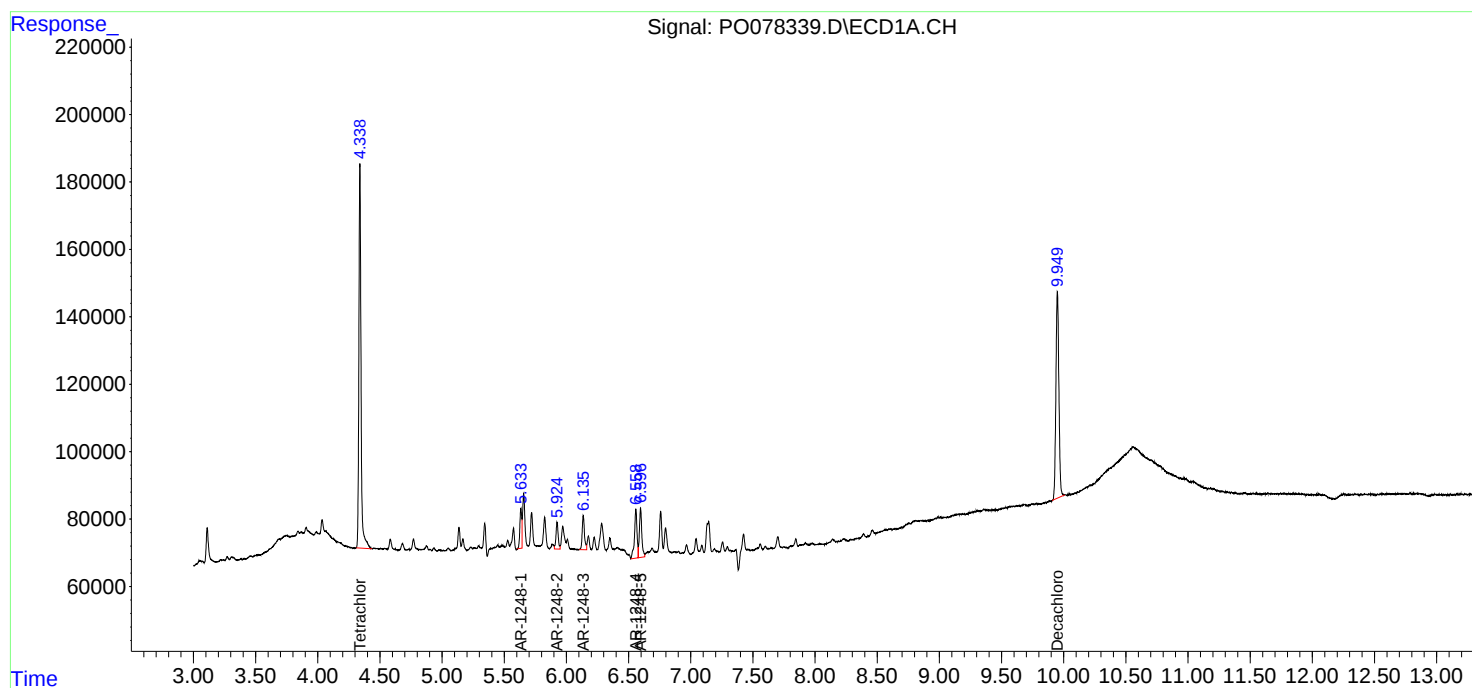

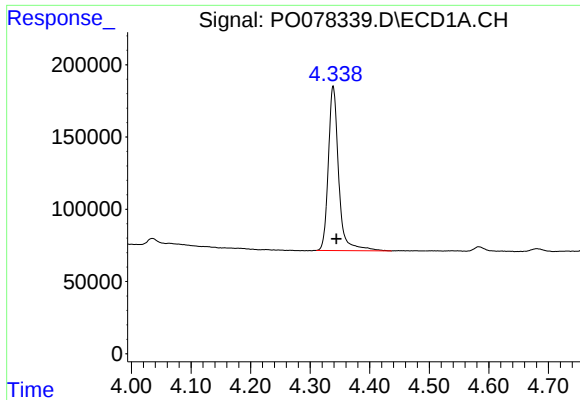


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 1373734
Conc: 18.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-119


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:19 PM

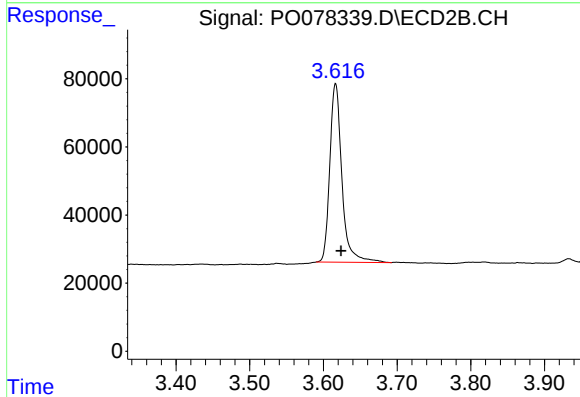


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.007 min
Response: 599534
Conc: 19.84 ng/ml

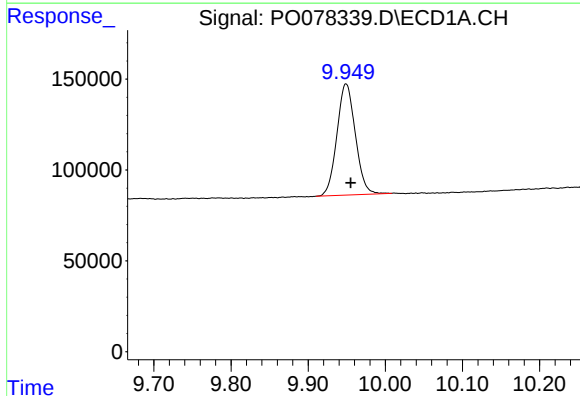


#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.006 min
Response: 1014533
Conc: 20.52 ng/ml

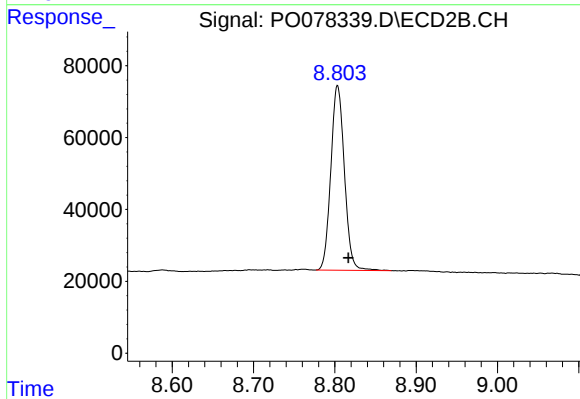

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.013 min
Response: 595970
Conc: 20.50 ng/ml

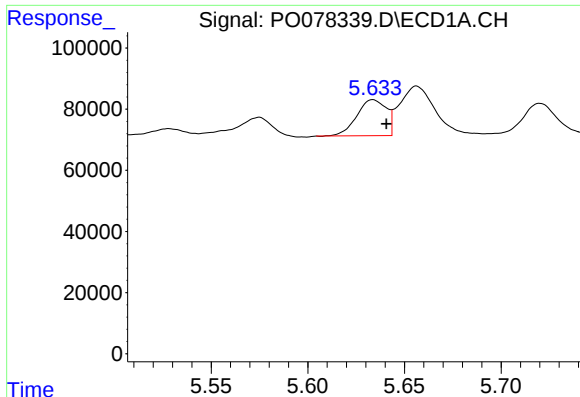


#21 AR-1248-1

R.T.: 5.634 min
Delta R.T.: -0.007 min
Response: 125266
Conc: 87.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-119


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:19 PM

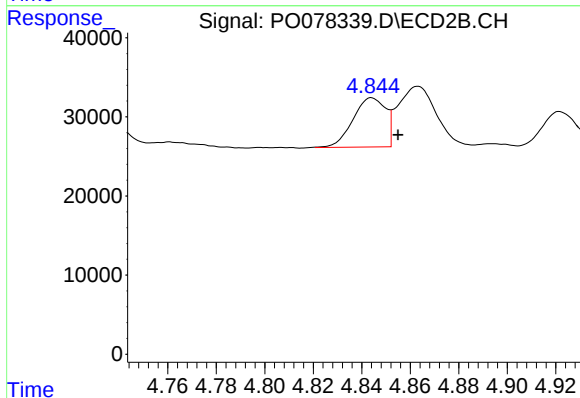


#21 AR-1248-1

R.T.: 4.844 min
Delta R.T.: -0.011 min
Response: 59617
Conc: 92.51 ng/ml m

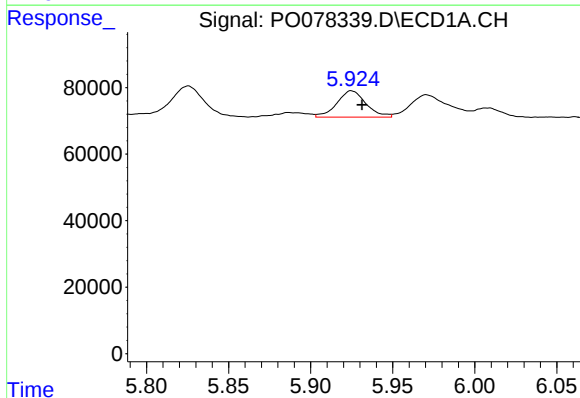


#22 AR-1248-2

R.T.: 5.925 min
Delta R.T.: -0.006 min
Response: 98314
Conc: 51.79 ng/ml

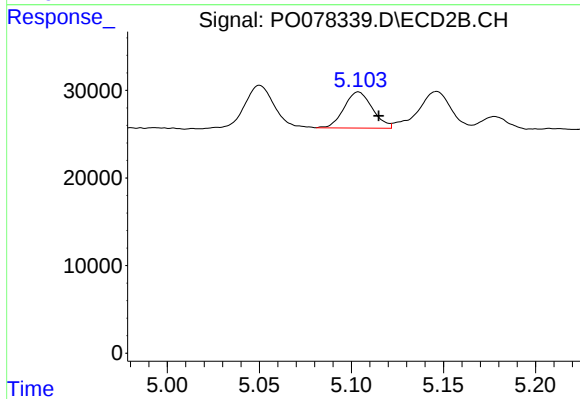

#22 AR-1248-2

R.T.: 5.104 min
Delta R.T.: -0.011 min
Response: 44010
Conc: 46.04 ng/ml

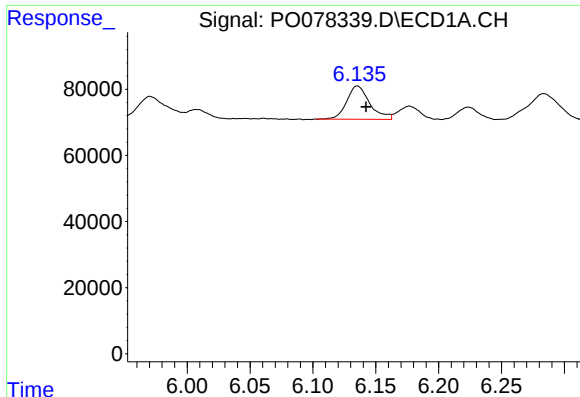


#23 AR-1248-3

R.T.: 6.135 min
Delta R.T.: -0.007 min
Response: 129055
Conc: 58.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-119


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:19 PM

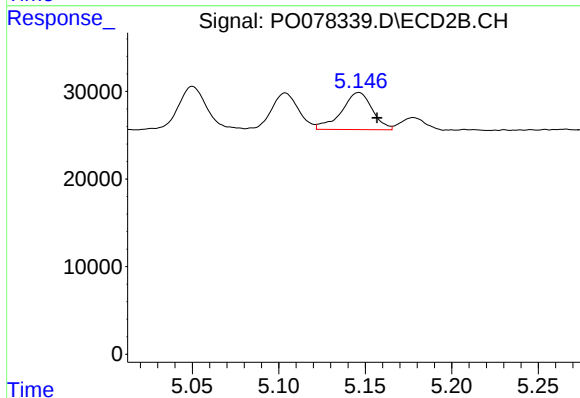


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: -0.011 min
Response: 52325
Conc: 54.43 ng/ml

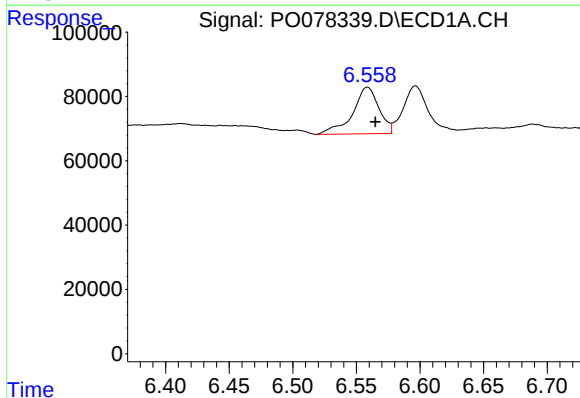


#24 AR-1248-4

R.T.: 6.559 min
Delta R.T.: -0.006 min
Response: 208821
Conc: 89.71 ng/ml

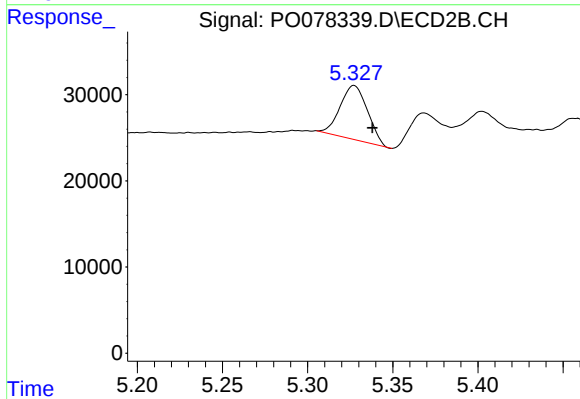

#24 AR-1248-4

R.T.: 5.327 min
Delta R.T.: -0.011 min
Response: 70269
Conc: 61.36 ng/ml

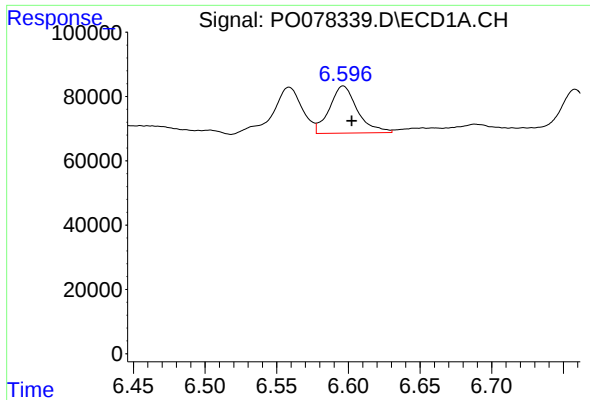


#25 AR-1248-5

R.T.: 6.596 min
Delta R.T.: -0.006 min
Response: 199080
Conc: 87.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PLA-119

Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:19 PM

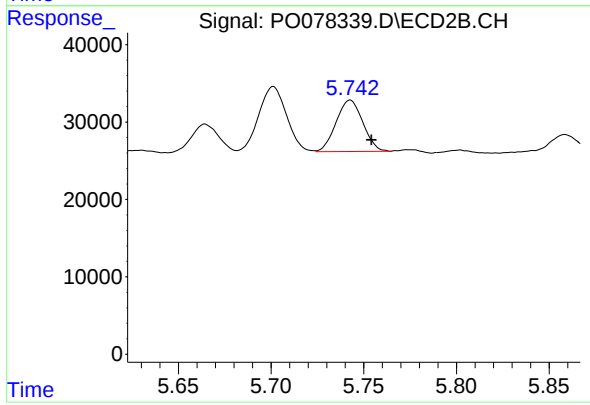

#25 AR-1248-5

R.T.: 5.743 min
Delta R.T.: -0.011 min
Response: 66728
Conc: 63.68 ng/ml