

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 16:07
 Operator : DD\AJ
 Sample : M2422-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 K328-13C

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:19:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:05:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.617	1433272	576090	19.393m	19.066
2) SA Decachlor...	9.947	8.803	988931	627427	20.002	21.578
Target Compounds						
41) L9 AR-1268-1	8.729	7.760	1058322	487298	149.301m	106.438 #
42) L9 AR-1268-2	8.809	7.823	743069	829401	114.827	200.459 #
43) L9 AR-1268-3	8.991	8.027	436590	223966	80.223	63.232
44) L9 AR-1268-4	9.354	8.318	354653	230745	157.478	152.513
45) L9 AR-1268-5	9.684	8.588	1000080	584092	57.186	55.446

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
Data File : P0078352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 16:07
Operator : DD\AJ
Sample : M2422-11
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
K328-13C


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:50 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:05:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

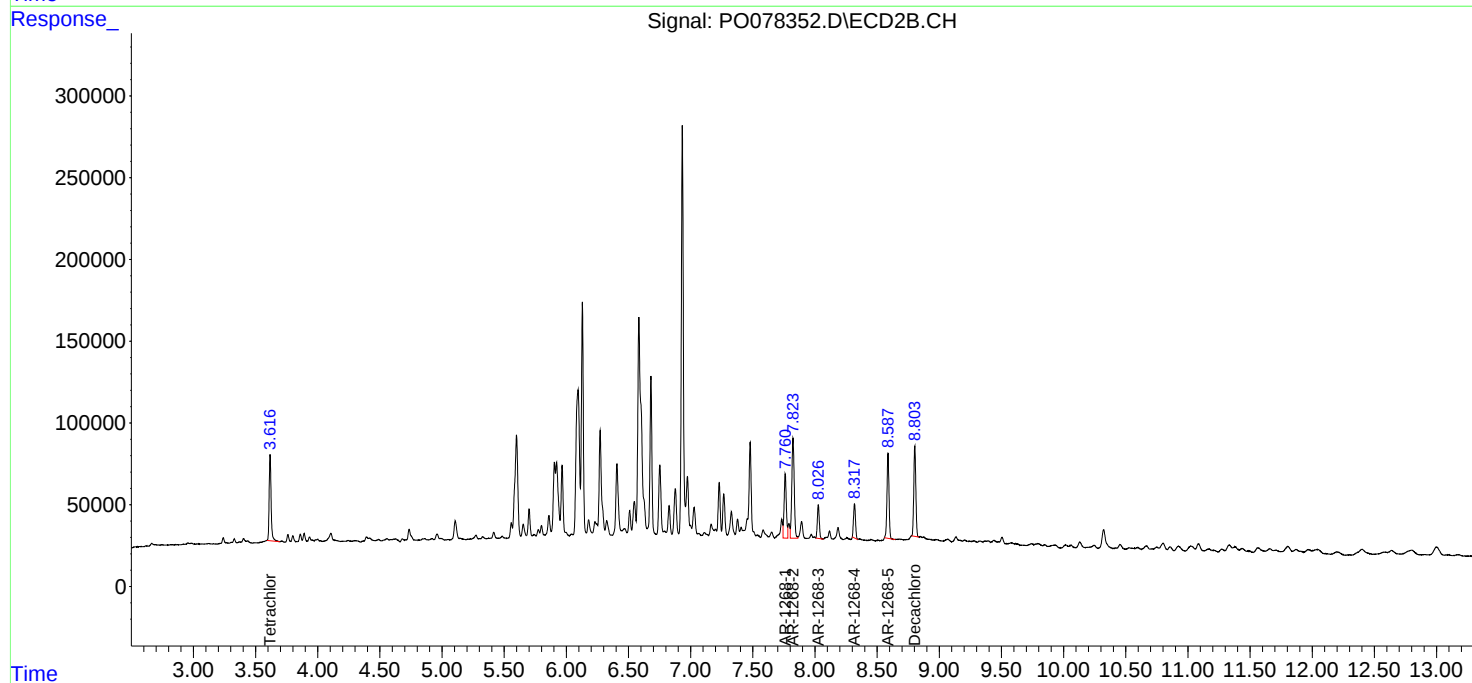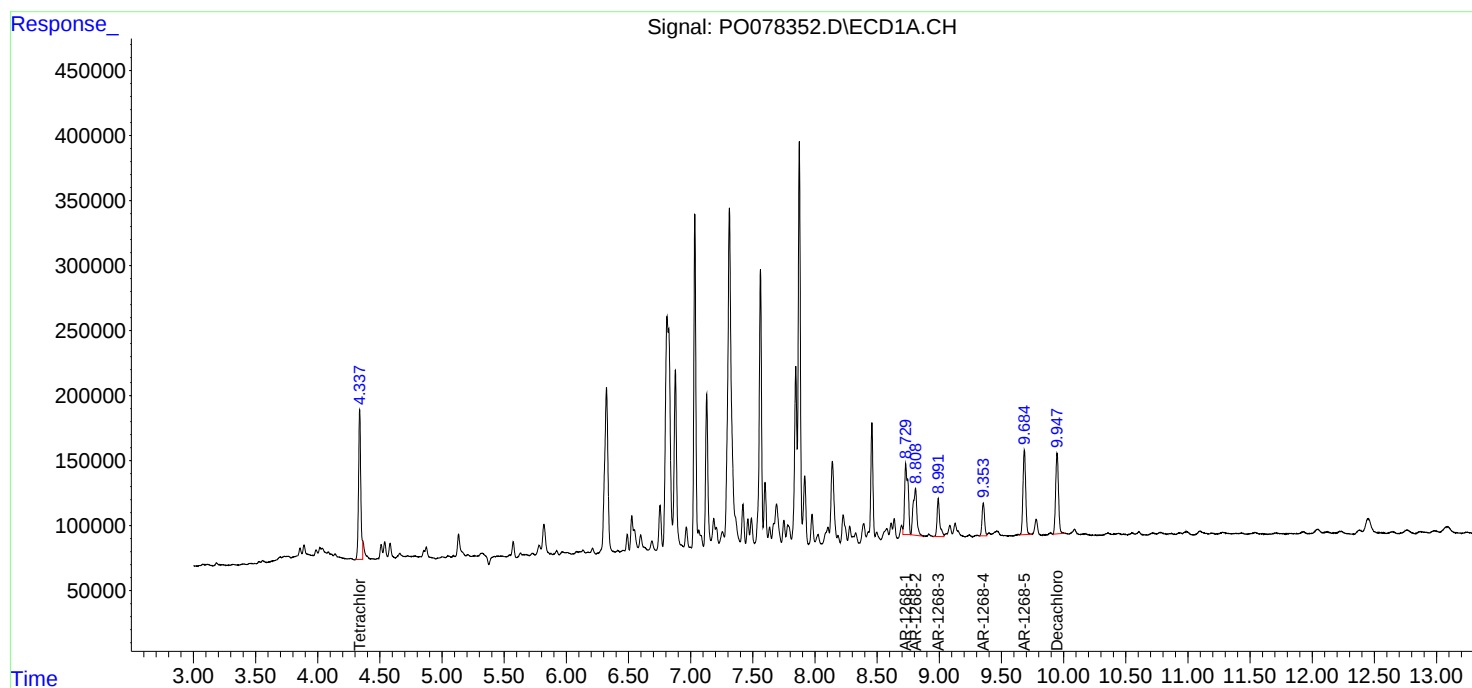

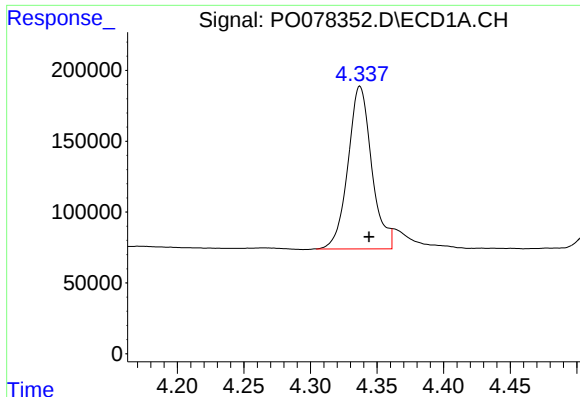


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.007 min
Response: 1433272
Conc: 19.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-13C


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:50 PM

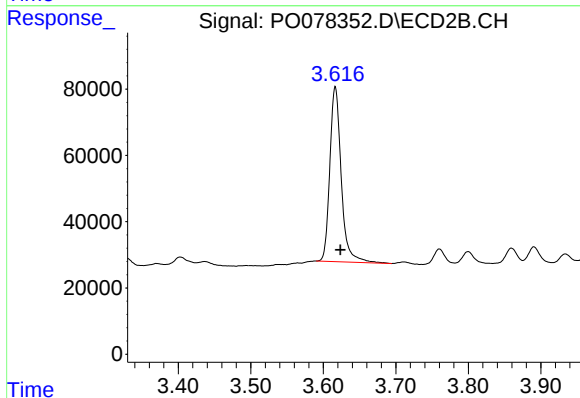


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.007 min
Response: 576090
Conc: 19.07 ng/ml

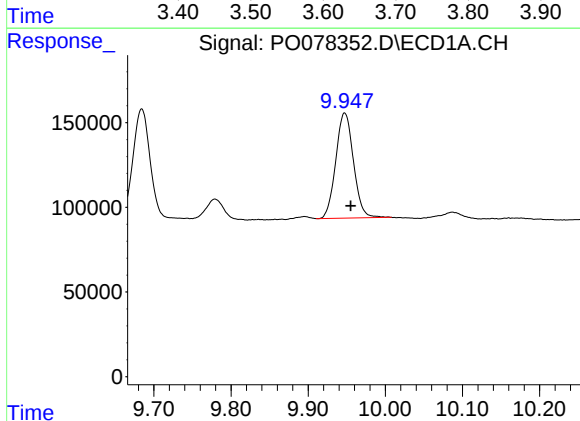


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 988931
Conc: 20.00 ng/ml

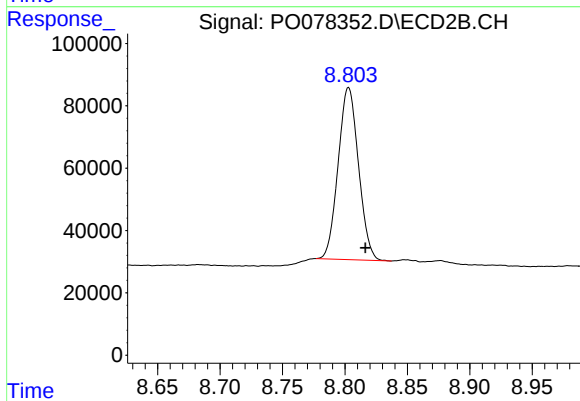

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.014 min
Response: 627427
Conc: 21.58 ng/ml

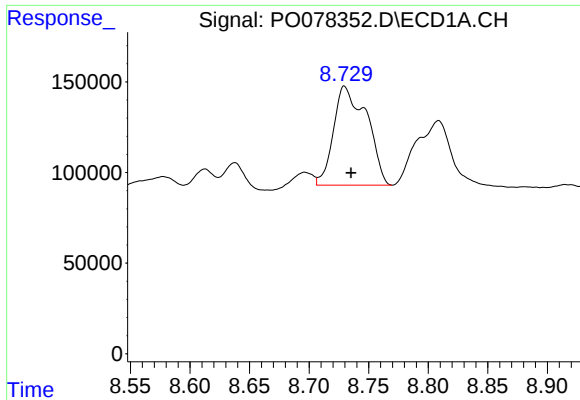


#41 AR-1268-1

R.T.: 8.729 min
Delta R.T.: -0.006 min
Response: 1058322
Conc: 149.30 ng/ml m

Instrument :
ECD_O
ClientSampleId :
K328-13C


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:50 PM

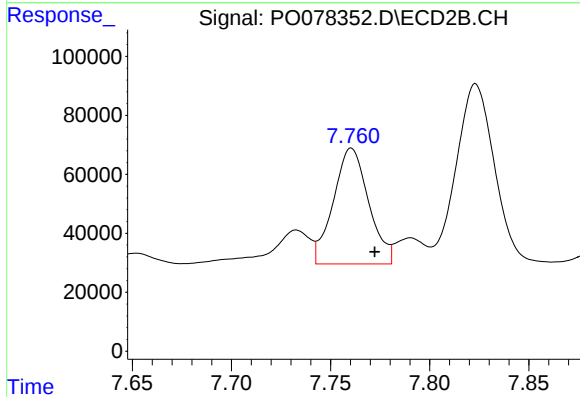


#41 AR-1268-1

R.T.: 7.760 min
Delta R.T.: -0.012 min
Response: 487298
Conc: 106.44 ng/ml

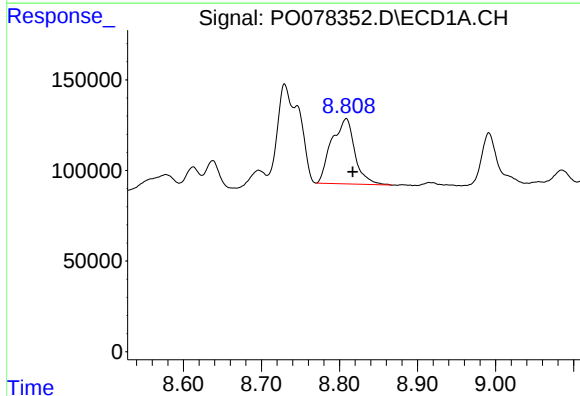


#42 AR-1268-2

R.T.: 8.809 min
Delta R.T.: -0.008 min
Response: 743069
Conc: 114.83 ng/ml

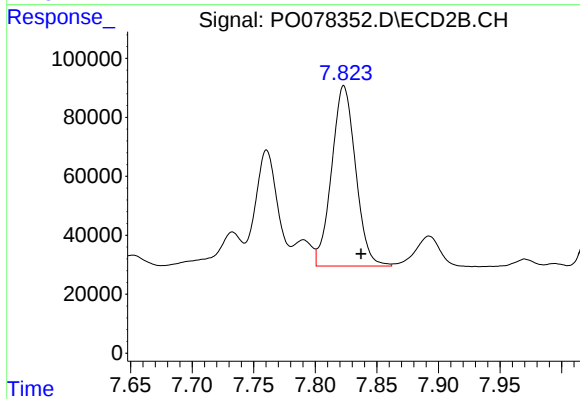

#42 AR-1268-2

R.T.: 7.823 min
Delta R.T.: -0.014 min
Response: 829401
Conc: 200.46 ng/ml

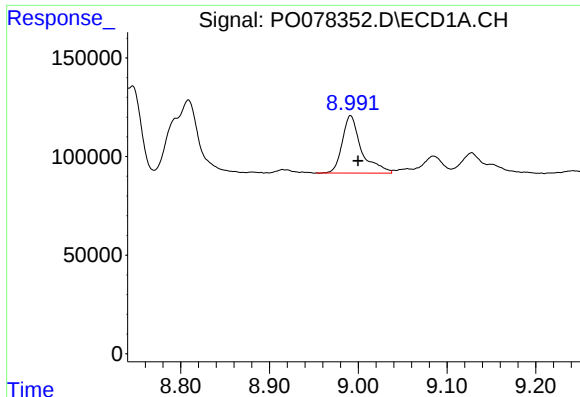


#43 AR-1268-3

R.T.: 8.991 min
Delta R.T.: -0.008 min
Response: 436590
Conc: 80.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-13C


Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:50 PM

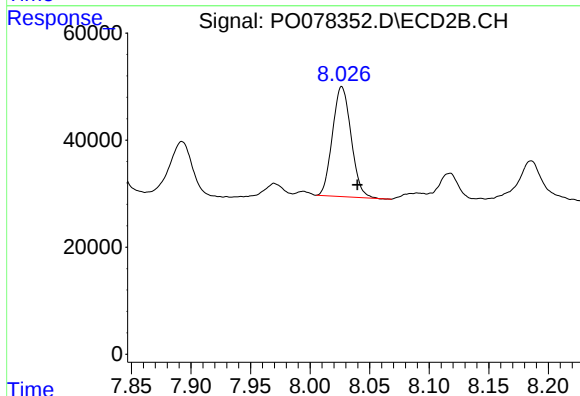


#43 AR-1268-3

R.T.: 8.027 min
Delta R.T.: -0.013 min
Response: 223966
Conc: 63.23 ng/ml

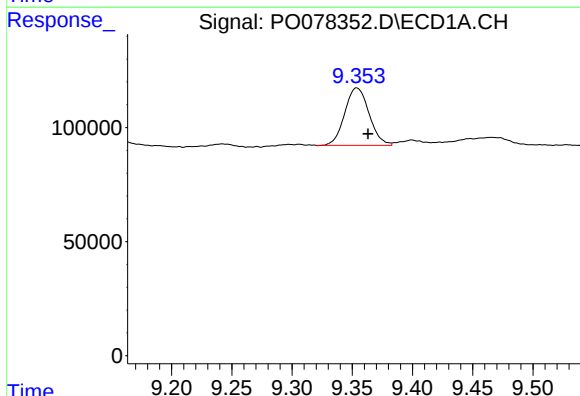


#44 AR-1268-4

R.T.: 9.354 min
Delta R.T.: -0.009 min
Response: 354653
Conc: 157.48 ng/ml

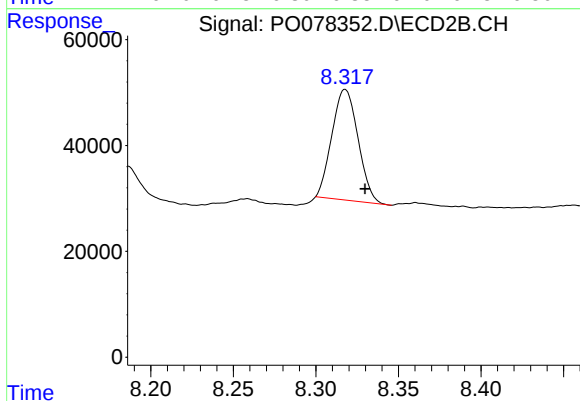

#44 AR-1268-4

R.T.: 8.318 min
Delta R.T.: -0.012 min
Response: 230745
Conc: 152.51 ng/ml

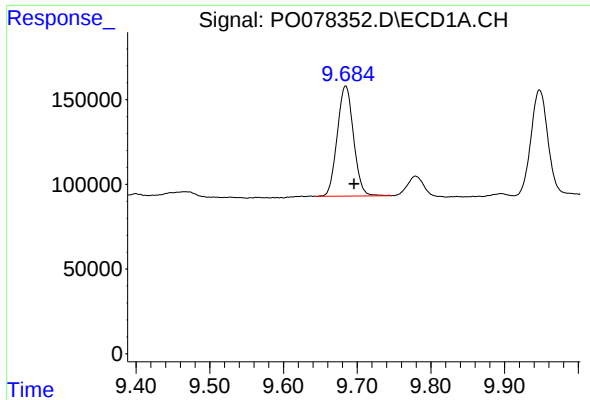


#45 AR-1268-5

R.T.: 9.684 min
Delta R.T.: -0.011 min
Response: 1000080
Conc: 57.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
K328-13C

Manual Integrations
APPROVED

Ankita
6/3/2021 2:19:50 PM

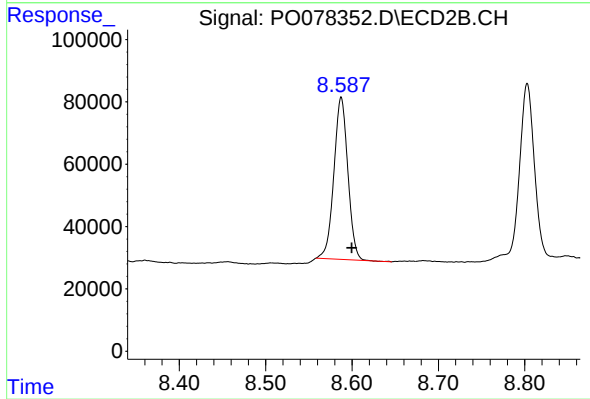

#45 AR-1268-5

R.T.: 8.588 min
Delta R.T.: -0.012 min
Response: 584092
Conc: 55.45 ng/ml