

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060221\
 Data File : P0078360.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jun 2021 19:00
 Operator : DD\AJ
 Sample : AR1242CCC500
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242CCC500

Manual Integrations
 APPROVED

Ankita
 6/3/2021 2:20:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 06:11:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.338	3.616	3526104	1484832	47.709	49.140
2)	SA Decachlor...	9.946	8.802	2265890	1289386	45.830	44.343
Target Compounds							
16)	L4 AR-1242-1	5.633	4.843	864225	415020	470.422	483.194m
17)	L4 AR-1242-2	5.655	4.863	1269119	588292	469.805	486.220
18)	L4 AR-1242-3	5.719	5.050	807650	300942	464.027	467.111
19)	L4 AR-1242-4	5.824	5.146	650927	315194	465.608	466.228
20)	L4 AR-1242-5	6.594	5.700	623811	402664	466.181	491.050

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060221\
Data File : PO078360.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jun 2021 19:00
Operator : DD\AJ
Sample : AR1242CCC500
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:20:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 06:11:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

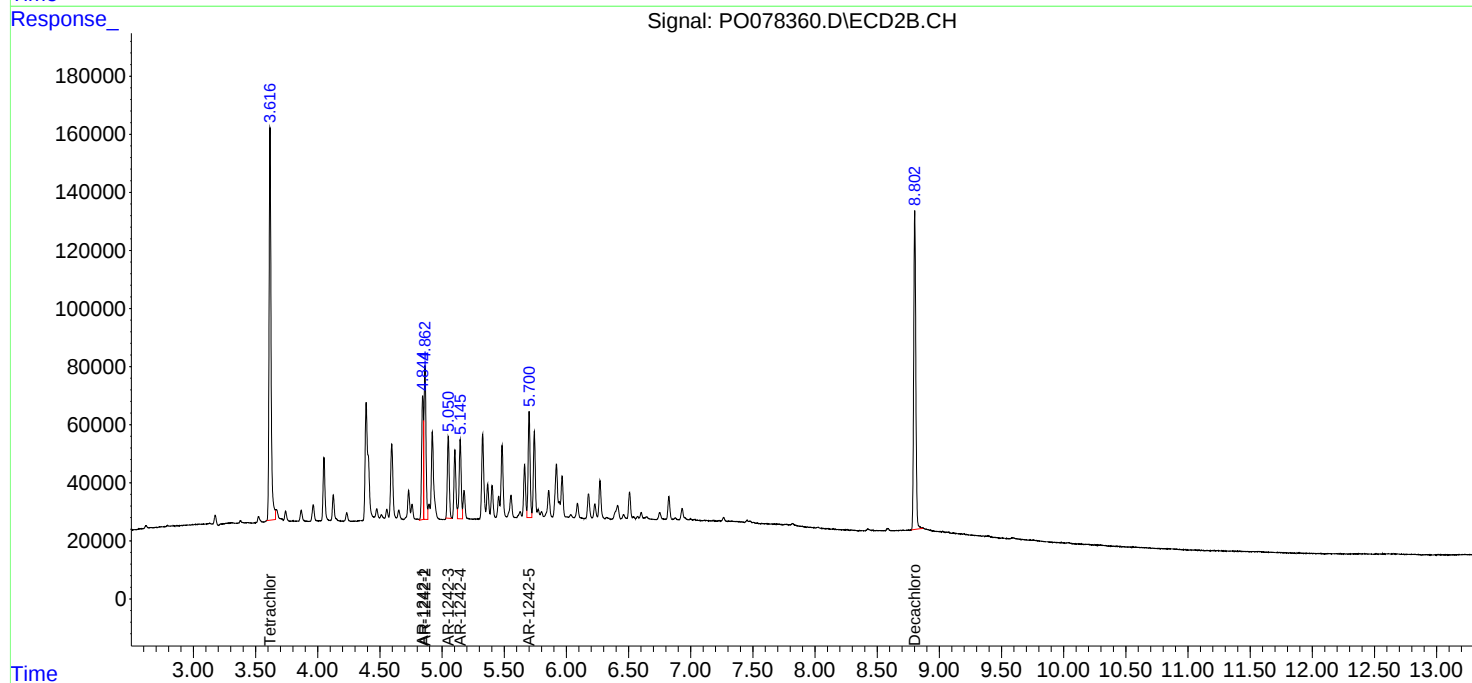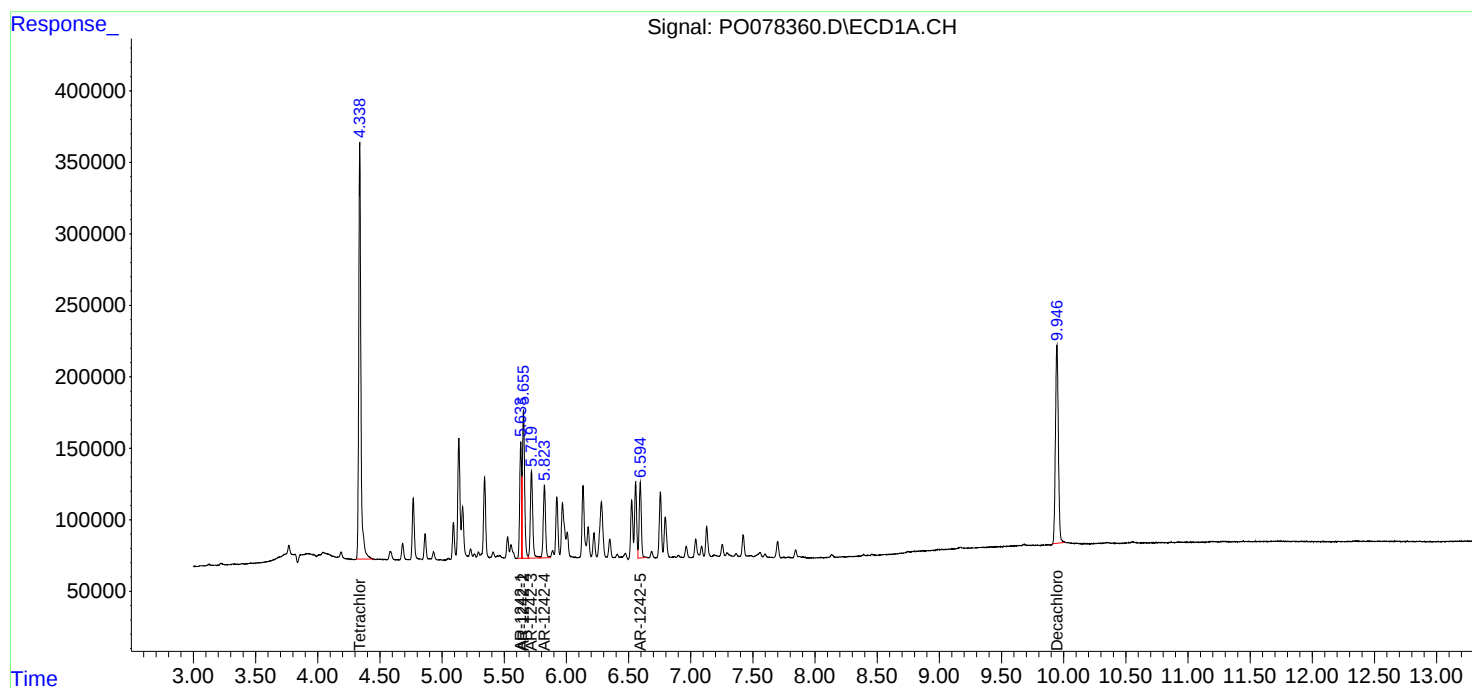

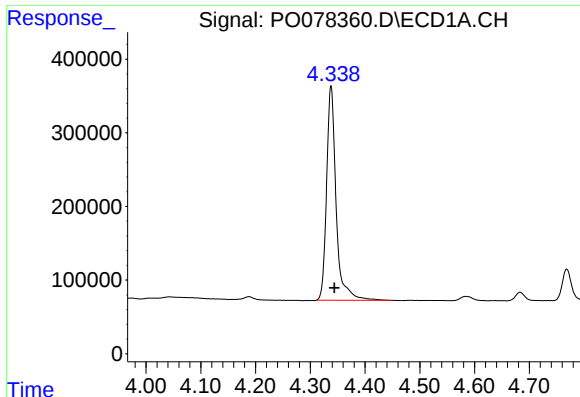


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 3526104
Conc: 47.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:20:11 PM

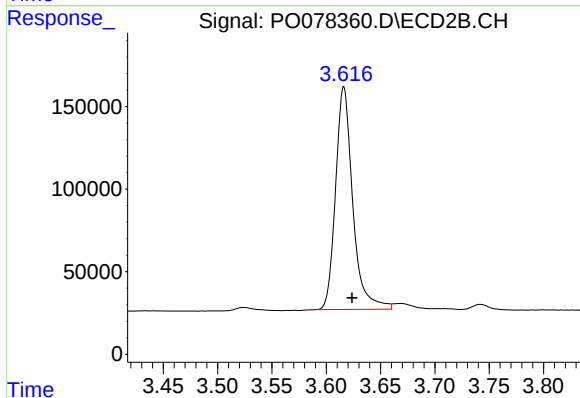


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.008 min
Response: 1484832
Conc: 49.14 ng/ml

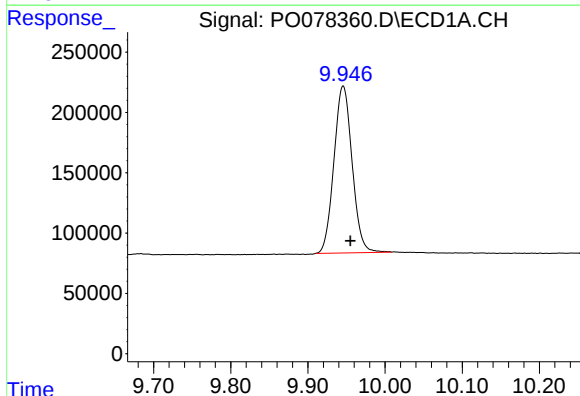


#2 Decachlorobiphenyl

R.T.: 9.946 min
Delta R.T.: -0.009 min
Response: 2265890
Conc: 45.83 ng/ml

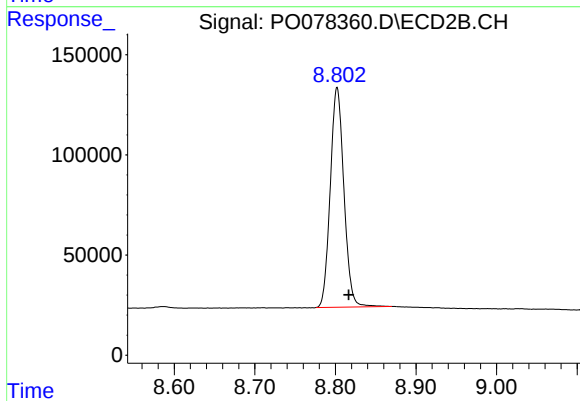

#2 Decachlorobiphenyl

R.T.: 8.802 min
Delta R.T.: -0.014 min
Response: 1289386
Conc: 44.34 ng/ml

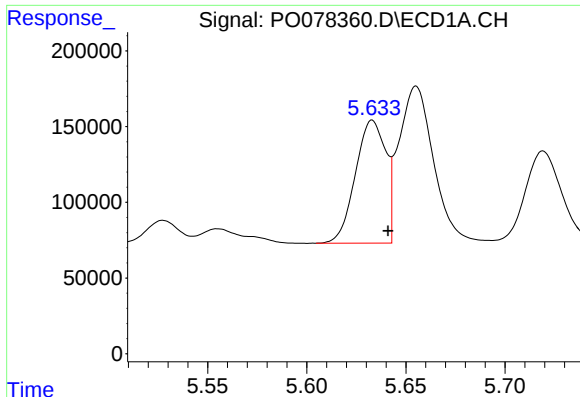


#16 AR-1242-1

R.T.: 5.633 min
Delta R.T.: -0.008 min
Response: 864225
Conc: 470.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:20:11 PM

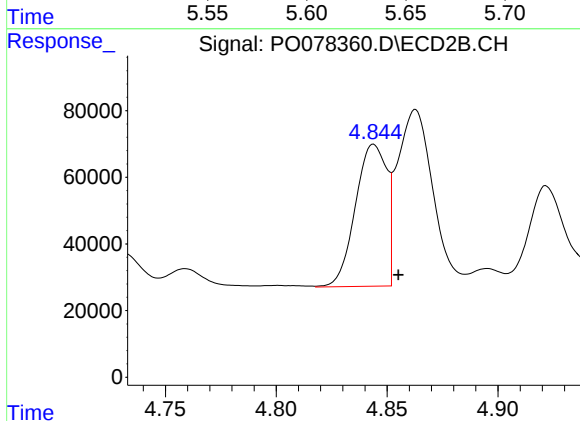


#16 AR-1242-1

R.T.: 4.843 min
Delta R.T.: -0.012 min
Response: 415020
Conc: 483.19 ng/ml m

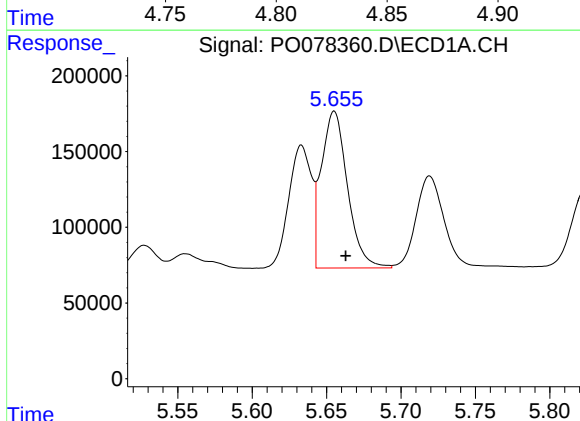


#17 AR-1242-2

R.T.: 5.655 min
Delta R.T.: -0.008 min
Response: 1269119
Conc: 469.81 ng/ml

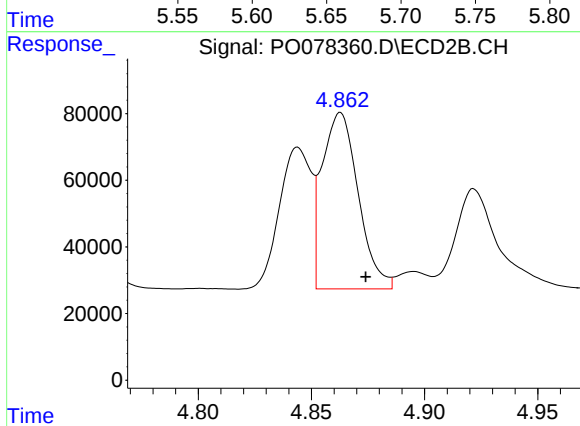

#17 AR-1242-2

R.T.: 4.863 min
Delta R.T.: -0.011 min
Response: 588292
Conc: 486.22 ng/ml

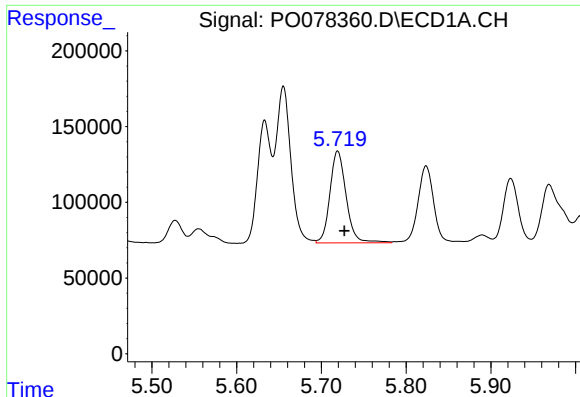


#18 AR-1242-3

R.T.: 5.719 min
Delta R.T.: -0.008 min
Response: 807650
Conc: 464.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500


Manual Integrations
APPROVED

Ankita
6/3/2021 2:20:11 PM

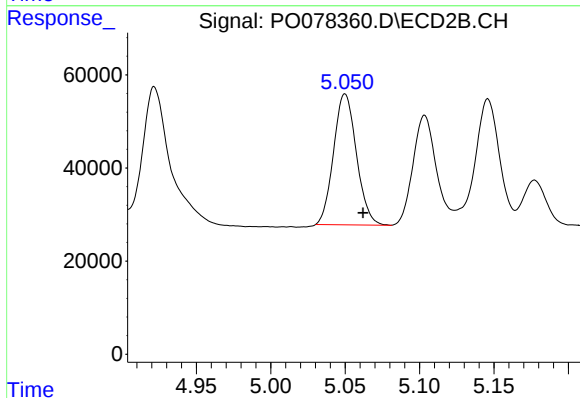


#18 AR-1242-3

R.T.: 5.050 min
Delta R.T.: -0.012 min
Response: 300942
Conc: 467.11 ng/ml

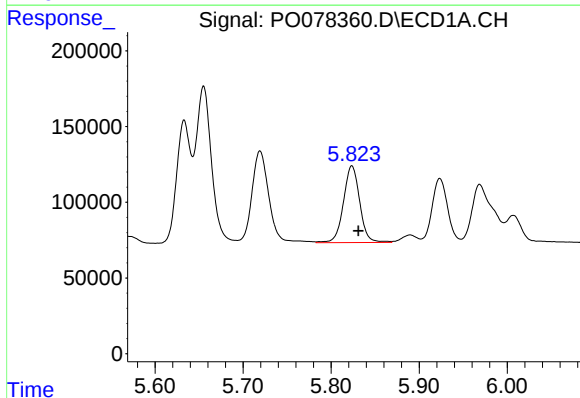


#19 AR-1242-4

R.T.: 5.824 min
Delta R.T.: -0.007 min
Response: 650927
Conc: 465.61 ng/ml

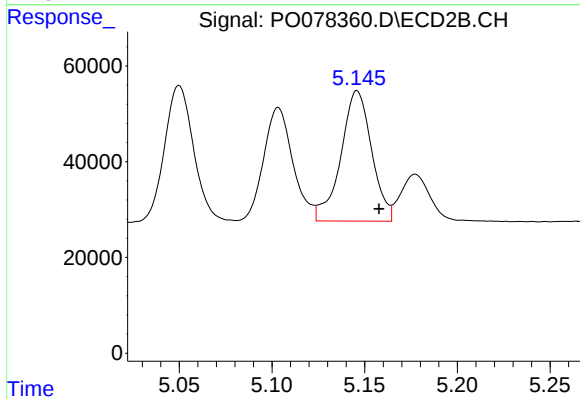

#19 AR-1242-4

R.T.: 5.146 min
Delta R.T.: -0.012 min
Response: 315194
Conc: 466.23 ng/ml

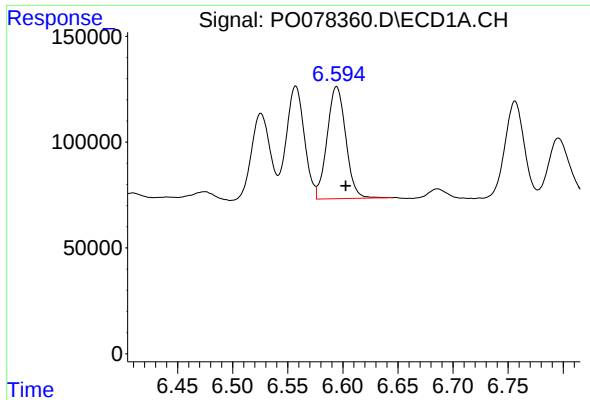


#20 AR-1242-5

R.T.: 6.594 min
Delta R.T.: -0.008 min
Response: 623811
Conc: 466.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242CCC500

Manual Integrations
APPROVED

Ankita
6/3/2021 2:20:11 PM

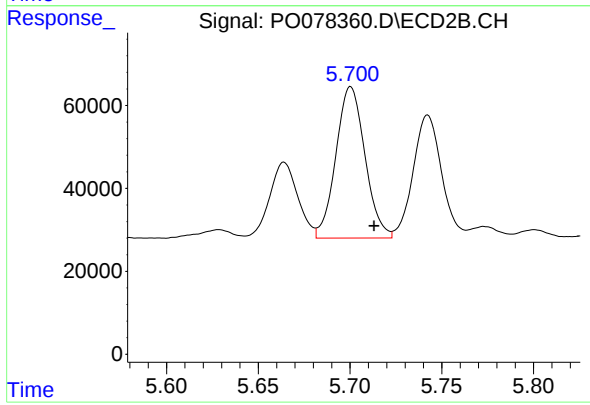

#20 AR-1242-5

R.T.: 5.700 min
Delta R.T.: -0.013 min
Response: 402664
Conc: 491.05 ng/ml