

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060223\
 Data File : P0095435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 14:20
 Operator : YP/AJ
 Sample : 03006-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-3-060123

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/05/2023
 Supervised By :Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 07:39:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 02 06:53:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.441	3.657	88618962	39549609	24.045	25.215
2) SA Decachlor...	10.290	8.718	58317148	26357409	21.547m	20.374

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060223\
Data File : PO095435.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 14:20
Operator : YP/AJ
Sample : 03006-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-3-060123


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/05/2023
Supervised By :Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 07:39:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 02 06:53:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

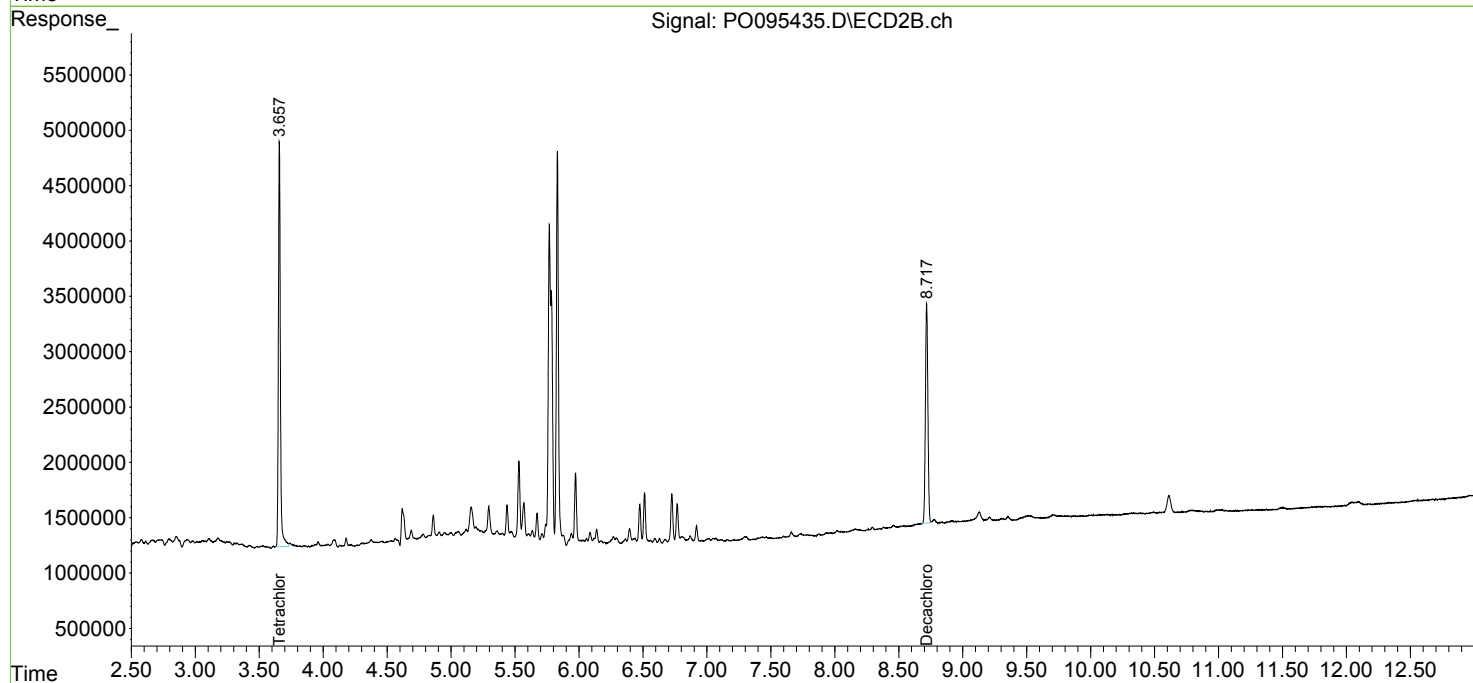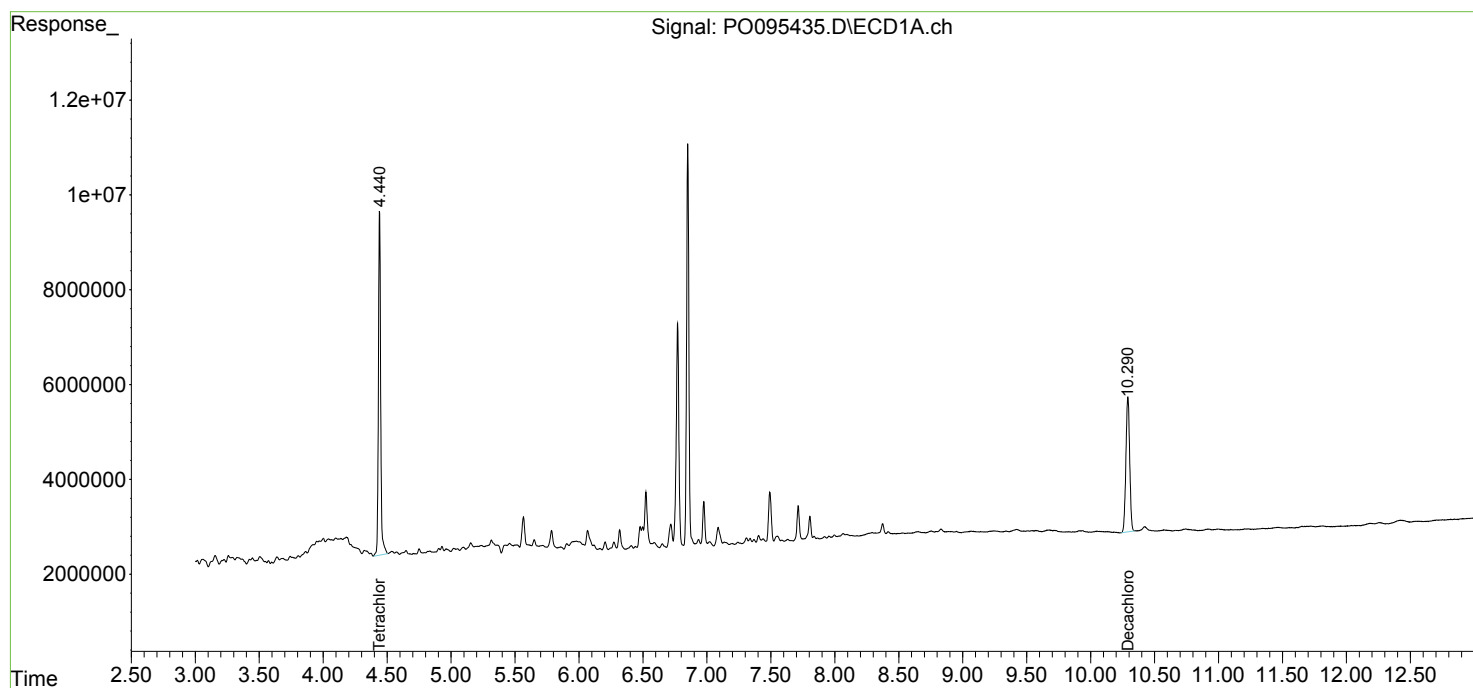

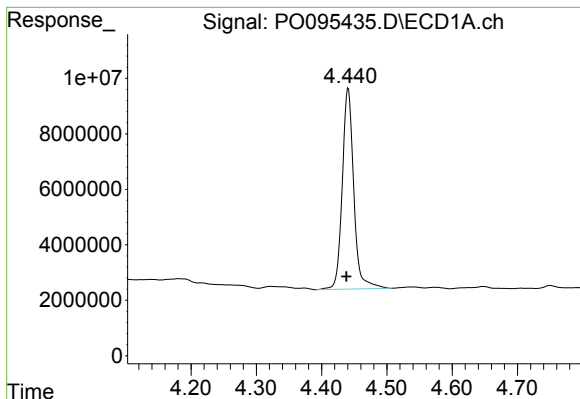

#1 Tetrachloro-m-xylene

R.T.: 4.441 min
Delta R.T.: 0.003 min
Response: 88618962
Conc: 24.04 ng/ml

Instrument :

ECD_O


ClientSampleId :

EO-3-060123

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 06/05/2023
Supervised By :Ankita Jodhani 06/05/2023

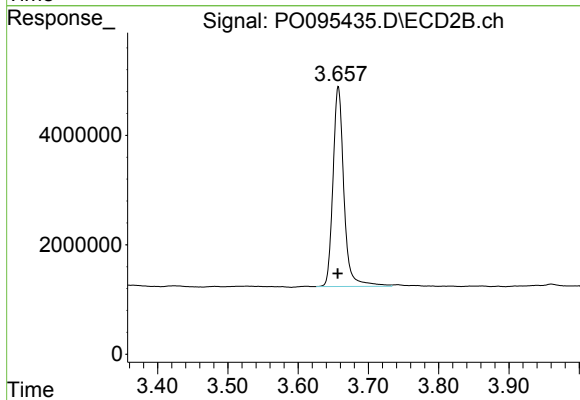


#1 Tetrachloro-m-xylene

R.T.: 3.657 min
Delta R.T.: 0.000 min
Response: 39549609
Conc: 25.21 ng/ml

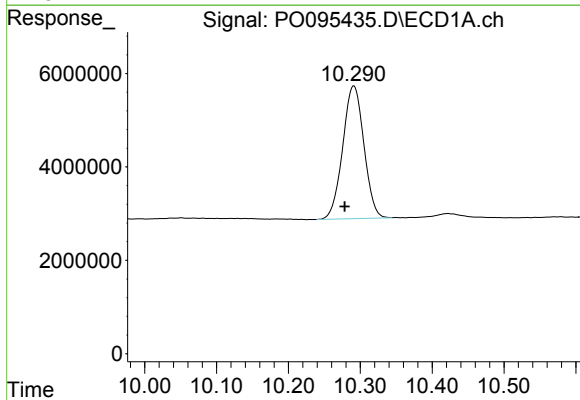

#2 Decachlorobiphenyl

R.T.: 10.290 min
Delta R.T.: 0.012 min
Response: 58317148
Conc: 21.55 ng/ml m

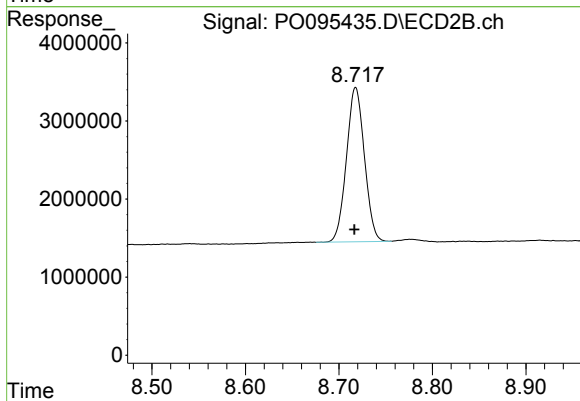

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: 0.001 min
Response: 26357409
Conc: 20.37 ng/ml