

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060223\
 Data File : P0095441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jun 2023 16:01
 Operator : YP/AJ
 Sample : 03002-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB05A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/05/2023
 Supervised By :Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 07:47:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 02 06:53:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.439	3.655	122.2E6	56528308	33.147	36.040
2) SA Decachlor...	10.285	8.714	73153992	36342241	27.029m	28.092m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060223\
Data File : P0095441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jun 2023 16:01
Operator : YP/AJ
Sample : 03002-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB05A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/05/2023
Supervised By :Ankita Jodhani 06/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 07:47:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 02 06:53:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

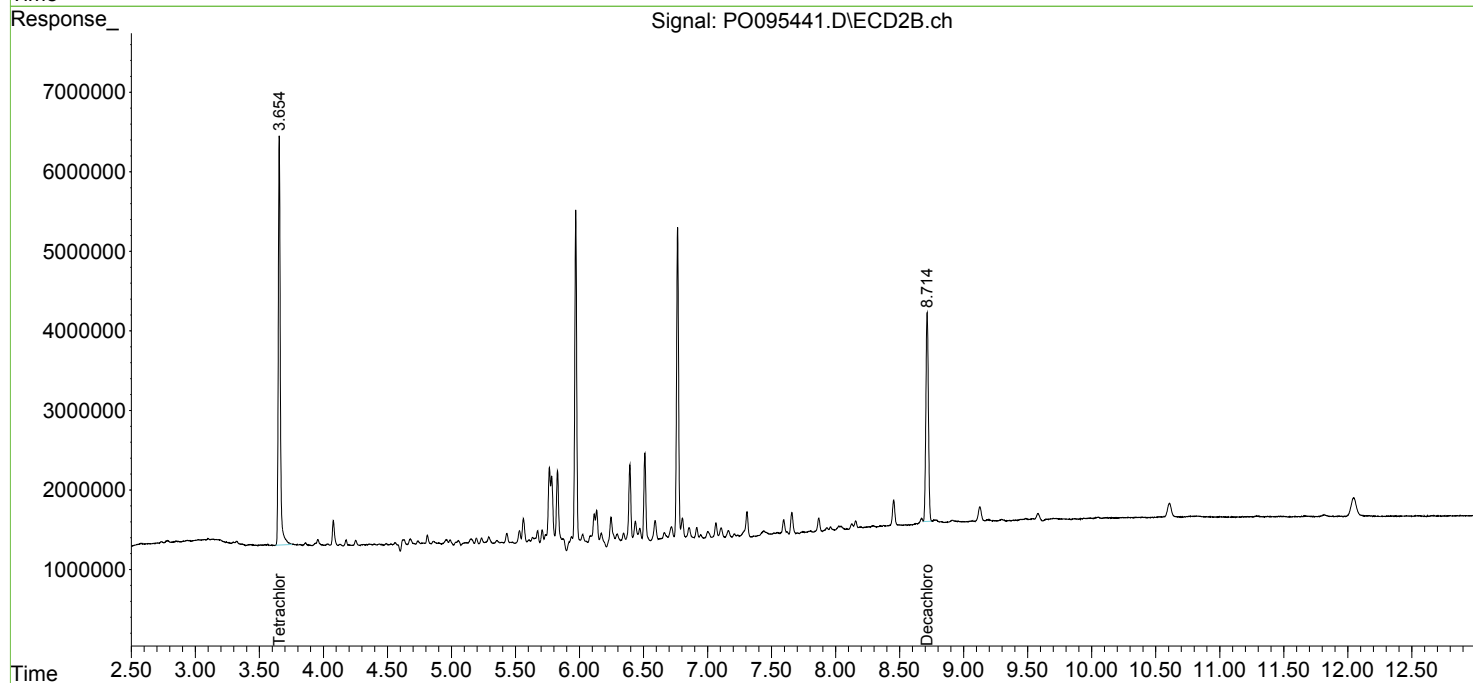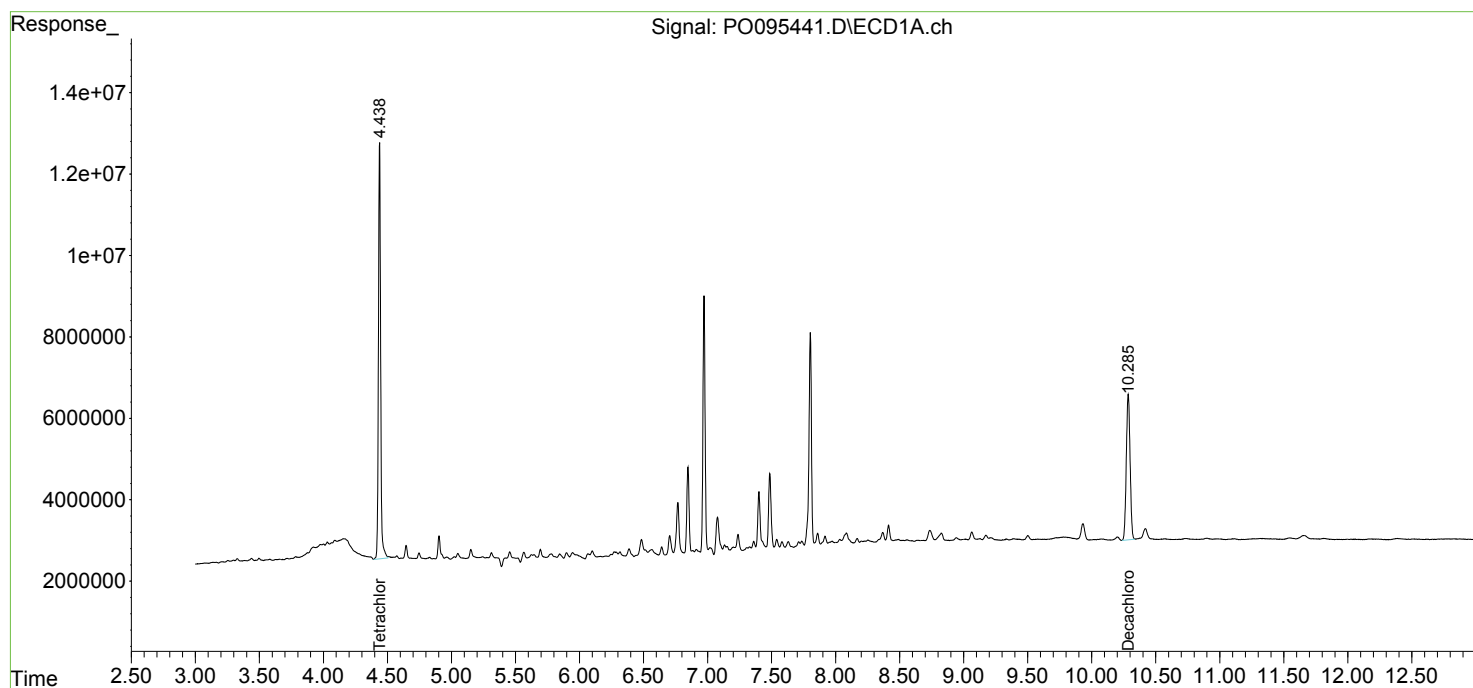

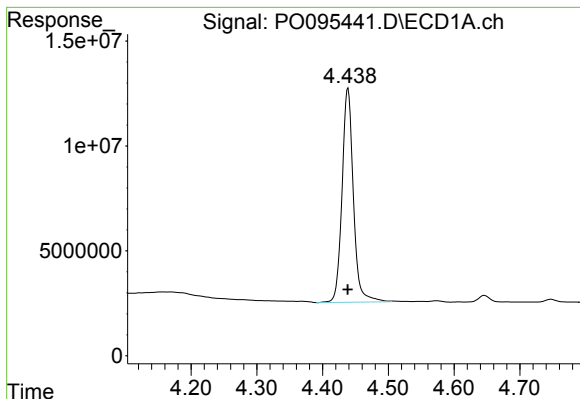


#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: 0.000 min
Response: 122166549
Conc: 33.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB05A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/05/2023
Supervised By :Ankita Jodhani 06/05/2023

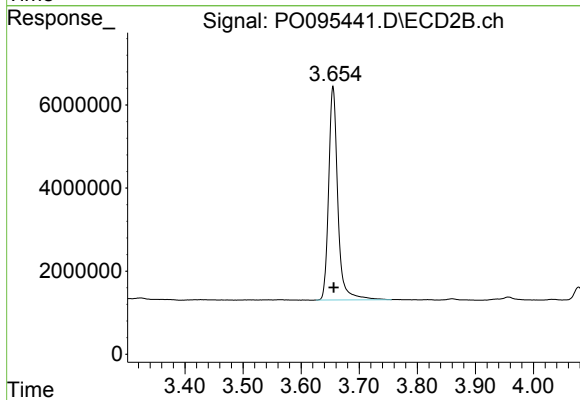


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: -0.002 min
Response: 56528308
Conc: 36.04 ng/ml

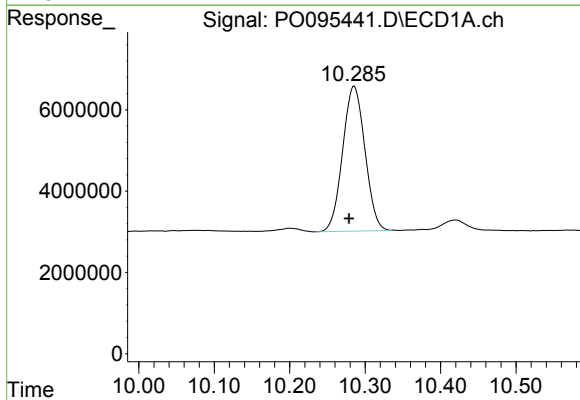

#2 Decachlorobiphenyl

R.T.: 10.285 min
Delta R.T.: 0.006 min
Response: 73153992
Conc: 27.03 ng/ml m

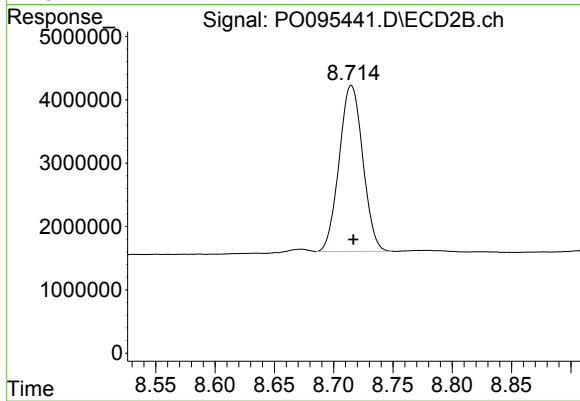

#2 Decachlorobiphenyl

R.T.: 8.714 min
Delta R.T.: -0.002 min
Response: 36342241
Conc: 28.09 ng/ml m