

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060321\
 Data File : P0078395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2021 10:54
 Operator : DD\AJ
 Sample : M2580-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 18-B2(0-2)

Manual Integrations
 APPROVED

Ankita
 6/4/2021 2:13:20 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 04:47:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.616	1942782	787011	26.287m	26.046
2) SA Decachlor...	9.947	8.801f	1278688	751488	25.863	25.844m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060321\
Data File : P0078395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2021 10:54
Operator : DD\AJ
Sample : M2580-04
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
18-B2(0-2)


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:20 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:47:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

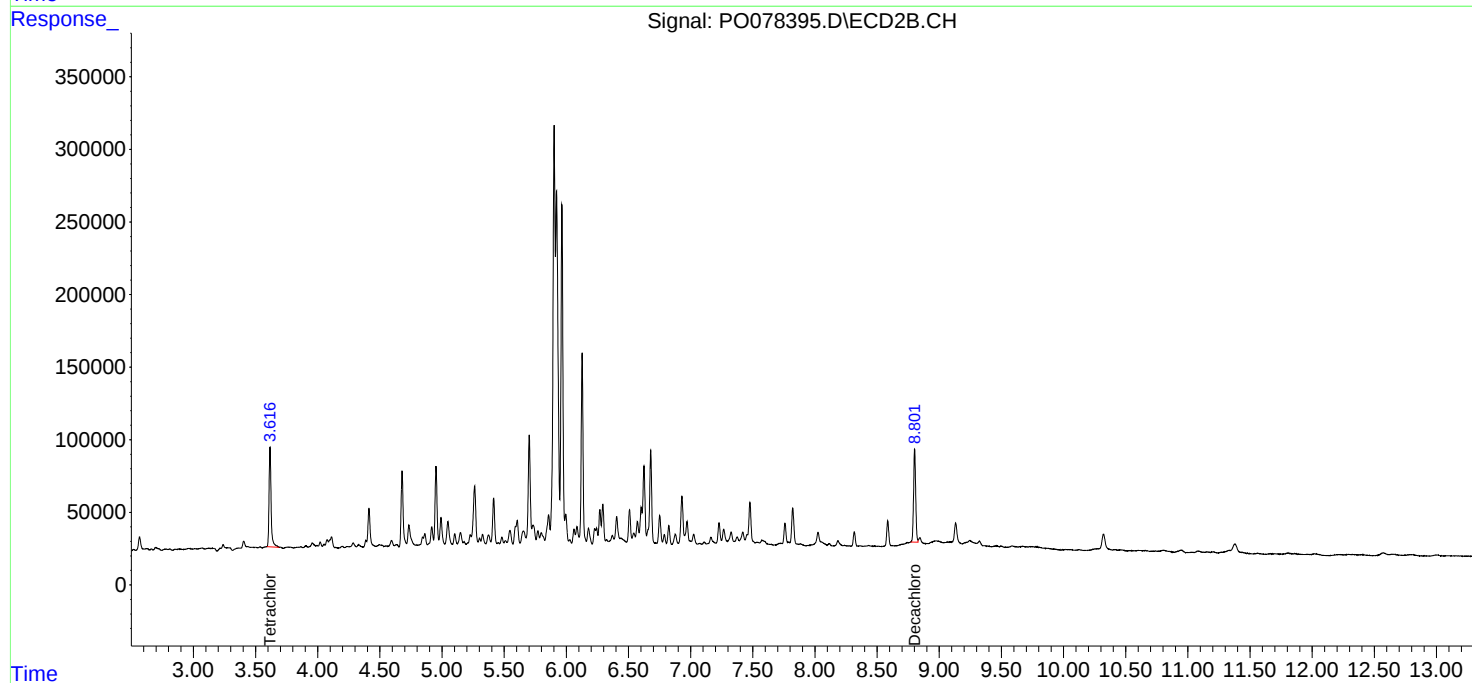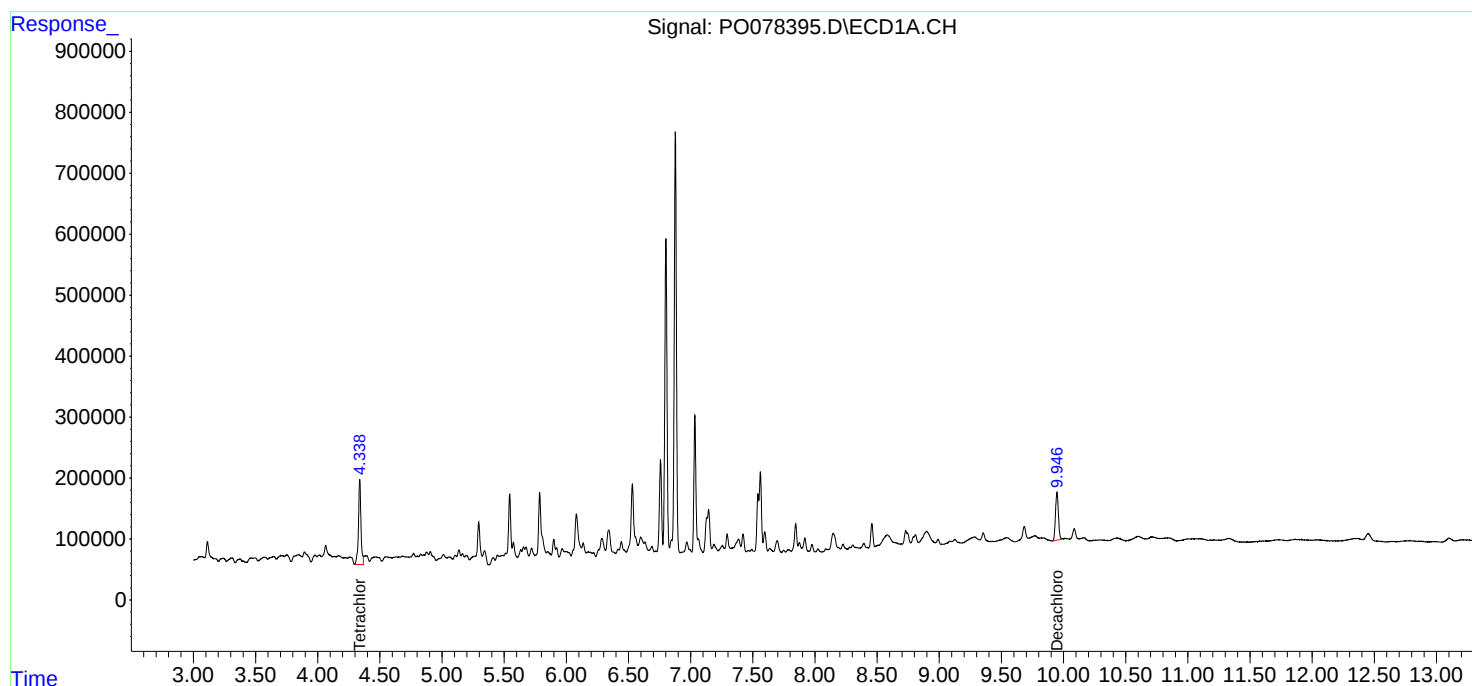

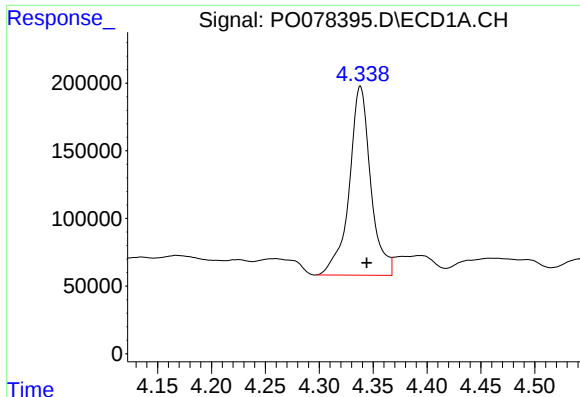


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 1942782
Conc: 26.29 ng/ml m

Instrument :
ECD_O
ClientSampleId :
18-B2(0-2)


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:20 PM

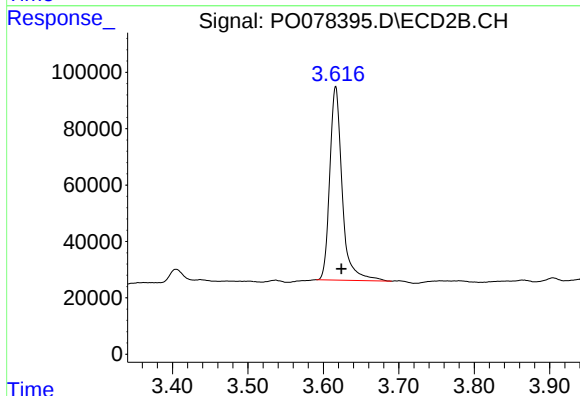


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.007 min
Response: 787011
Conc: 26.05 ng/ml

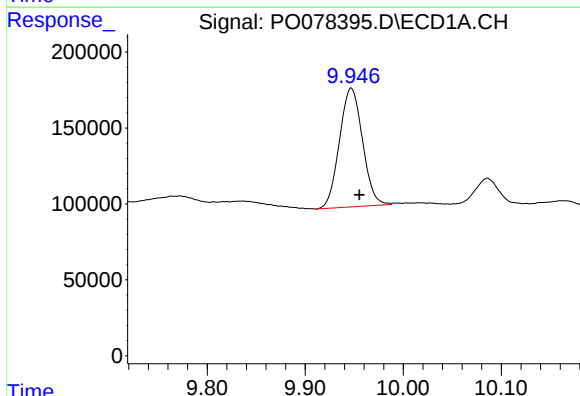

#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 1278688
Conc: 25.86 ng/ml

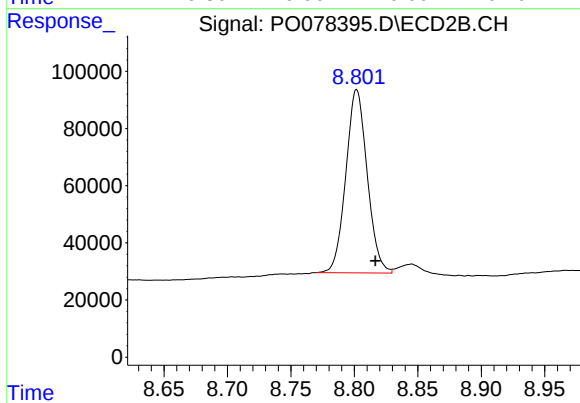

#2 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: -0.015 min
Response: 751488
Conc: 25.84 ng/ml m