

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060321\
 Data File : P0078421.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2021 20:28
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/4/2021 2:13:52 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 04 04:53:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.616	3667216	1627466	49.619	53.861
2) SA Decachlor...	9.947	8.803	2127359	1259715	43.028	43.322
Target Compounds						
21) L5 AR-1248-1	5.633	4.843	704872	338918	494.681	525.908m
22) L5 AR-1248-2	5.925	5.103	968456	480854	510.116	503.014
23) L5 AR-1248-3	6.135	5.145	1108273	483234	499.662	502.720
24) L5 AR-1248-4	6.558	5.326	1159676	563778	498.219	492.270
25) L5 AR-1248-5	6.595	5.742	1155598	547428	510.745	522.431

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060321\
Data File : P0078421.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2021 20:28
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:52 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 04 04:53:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

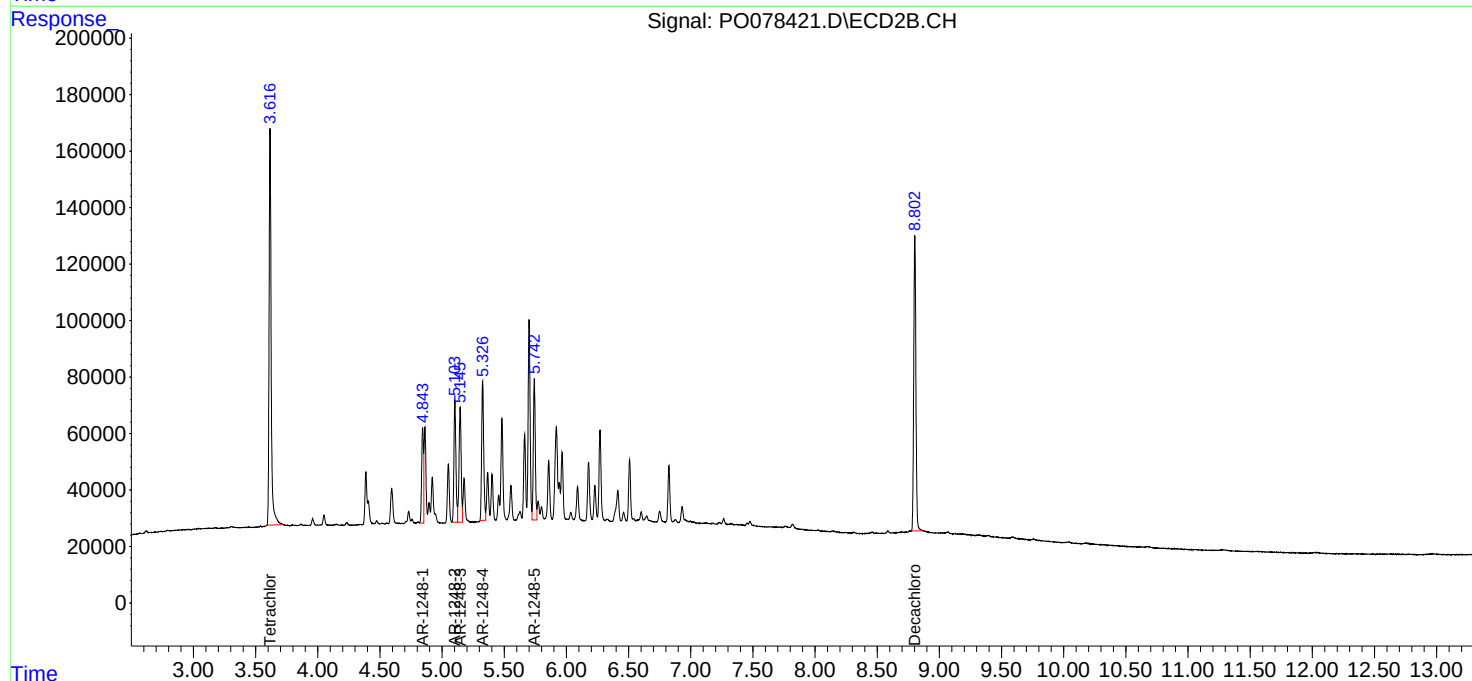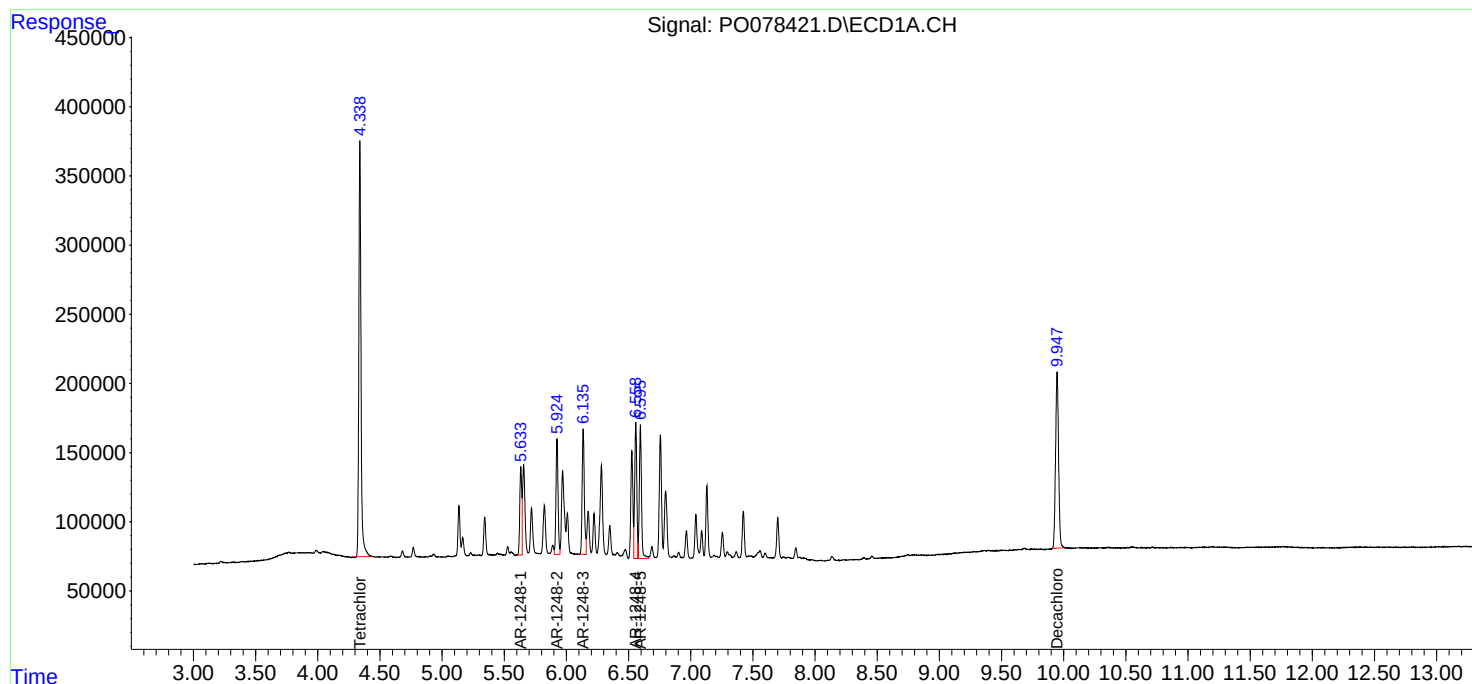

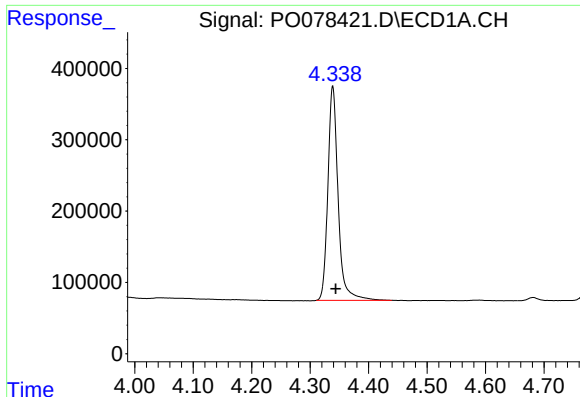


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 3667216
Conc: 49.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:52 PM

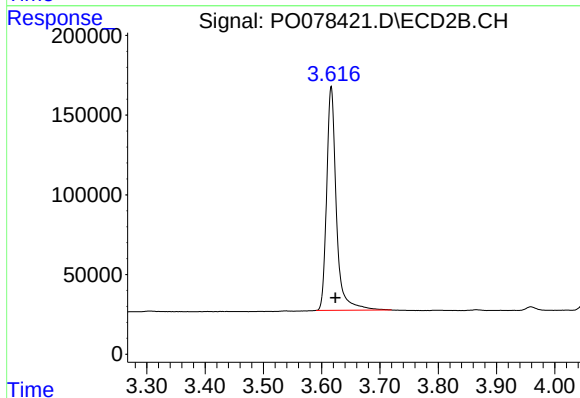


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.007 min
Response: 1627466
Conc: 53.86 ng/ml

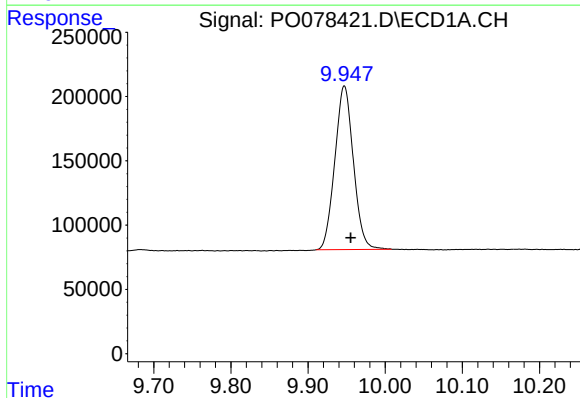


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 2127359
Conc: 43.03 ng/ml

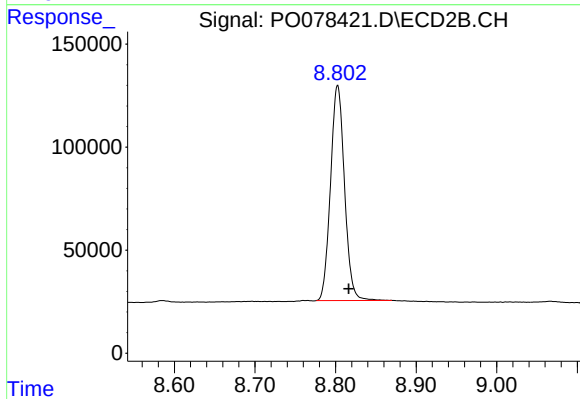

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.014 min
Response: 1259715
Conc: 43.32 ng/ml

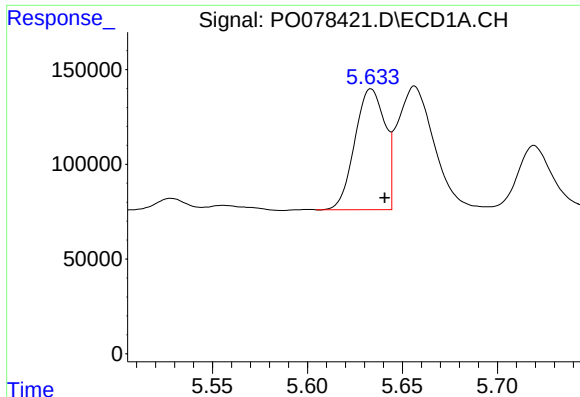


#21 AR-1248-1

R.T.: 5.633 min
Delta R.T.: -0.007 min
Response: 704872
Conc: 494.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:52 PM

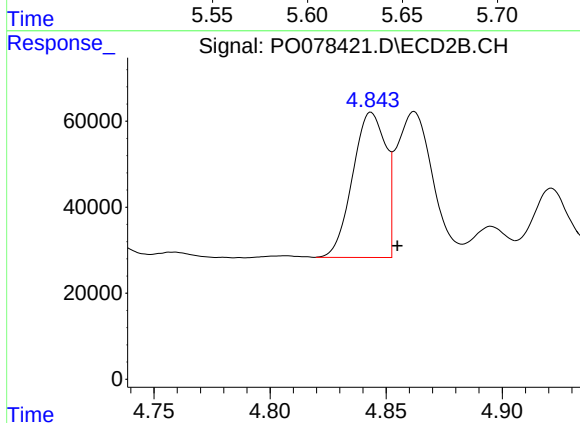


#21 AR-1248-1

R.T.: 4.843 min
Delta R.T.: -0.012 min
Response: 338918
Conc: 525.91 ng/ml m

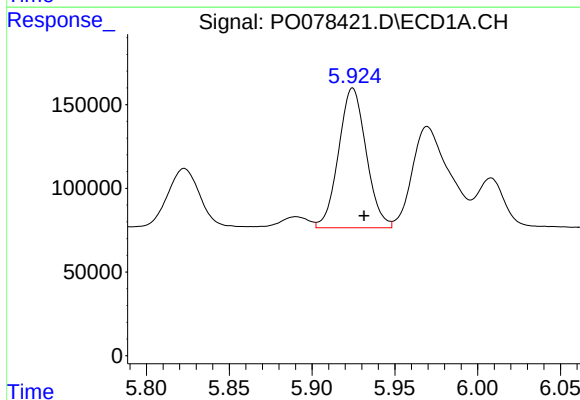


#22 AR-1248-2

R.T.: 5.925 min
Delta R.T.: -0.007 min
Response: 968456
Conc: 510.12 ng/ml

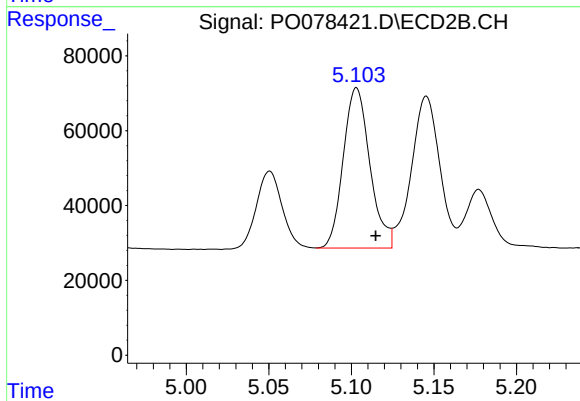

#22 AR-1248-2

R.T.: 5.103 min
Delta R.T.: -0.012 min
Response: 480854
Conc: 503.01 ng/ml

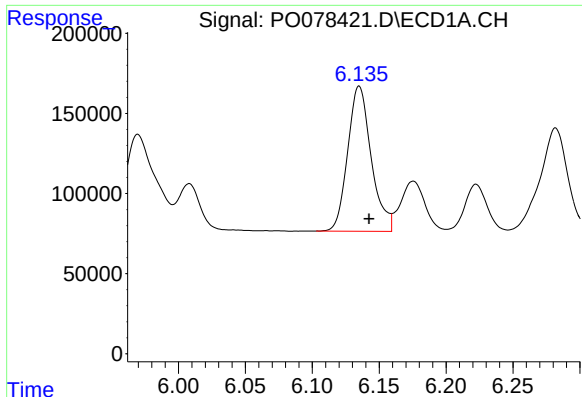


#23 AR-1248-3

R.T.: 6.135 min
Delta R.T.: -0.007 min
Response: 1108273
Conc: 499.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:52 PM

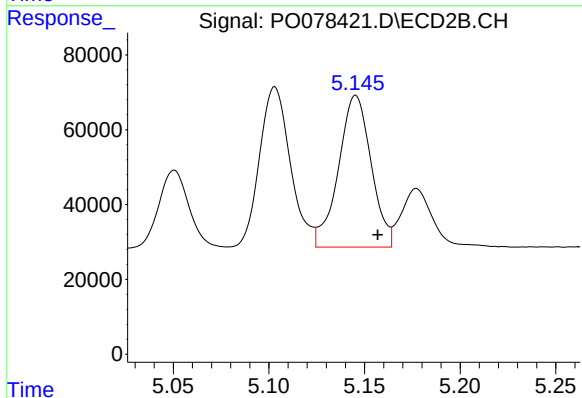


#23 AR-1248-3

R.T.: 5.145 min
Delta R.T.: -0.011 min
Response: 483234
Conc: 502.72 ng/ml

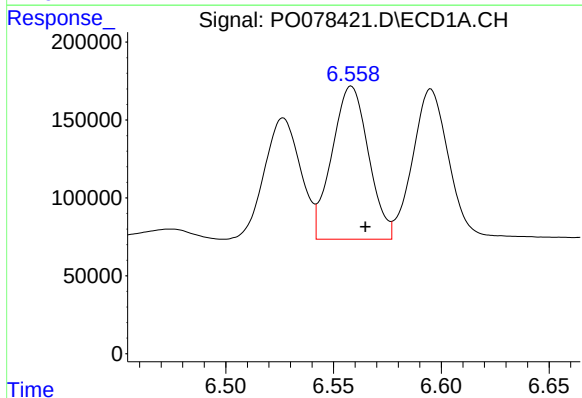


#24 AR-1248-4

R.T.: 6.558 min
Delta R.T.: -0.007 min
Response: 1159676
Conc: 498.22 ng/ml

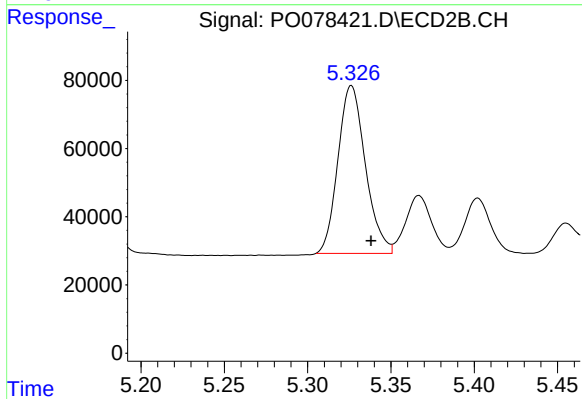

#24 AR-1248-4

R.T.: 5.326 min
Delta R.T.: -0.012 min
Response: 563778
Conc: 492.27 ng/ml

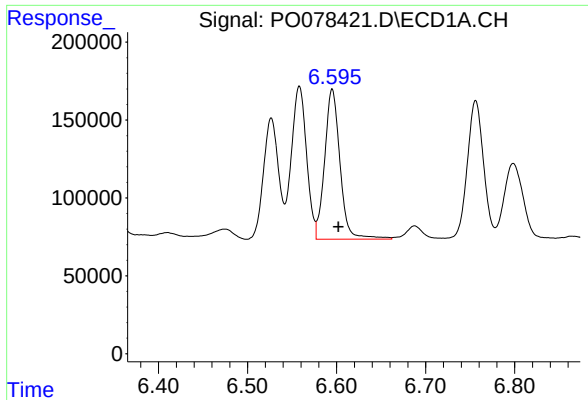


#25 AR-1248-5

R.T.: 6.595 min
Delta R.T.: -0.007 min
Response: 1155598
Conc: 510.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/4/2021 2:13:52 PM

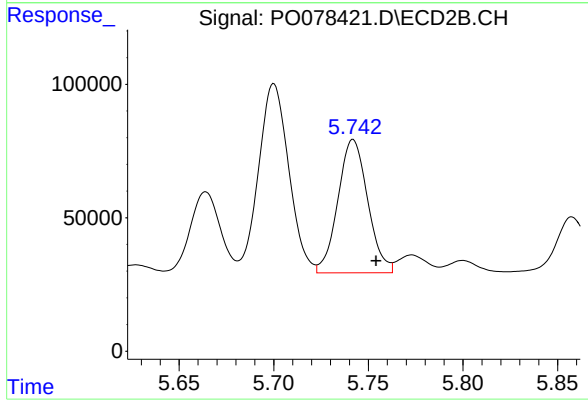

#25 AR-1248-5

R.T.: 5.742 min
Delta R.T.: -0.012 min
Response: 547428
Conc: 522.43 ng/ml