

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060322\
 Data File : P0086914.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Jun 2022 18:40
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 03 23:07:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.516	3.665	1143842	595343	20.000	18.625
2)	SA Decachlor...	10.393	8.692	971361	393691	21.280	17.558

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060322\
Data File : P0086914.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Jun 2022 18:40
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 03 23:07:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

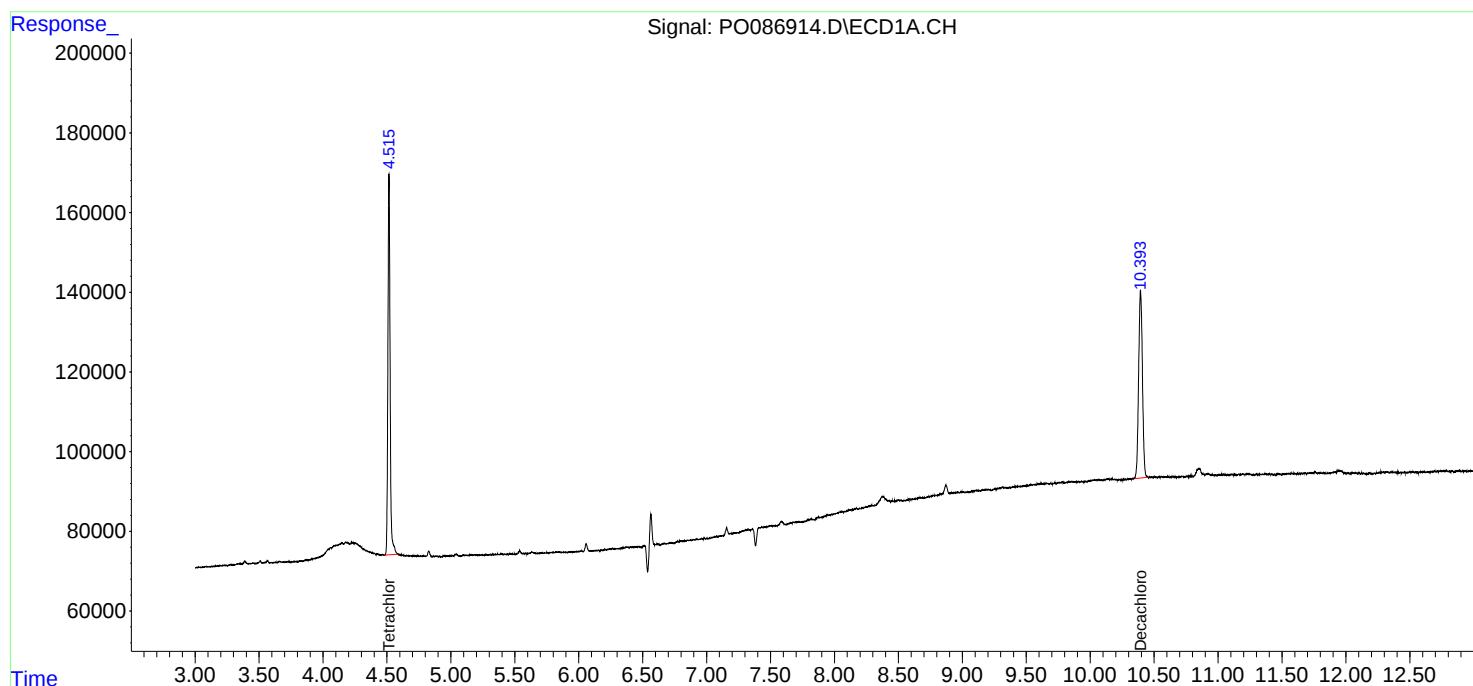


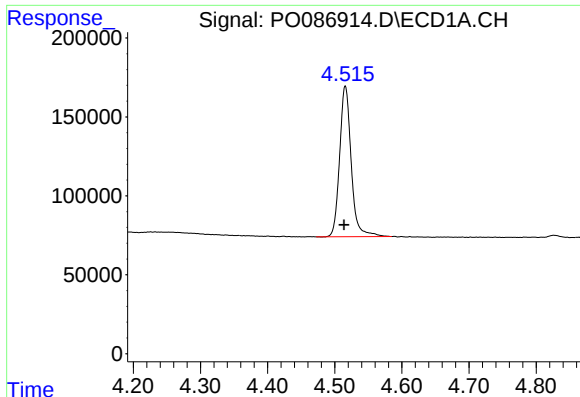

#1 Tetrachloro-m-xylene


R.T.: 4.516 min
Delta R.T.: 0.002 min
Response: 1143842
Conc: 20.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

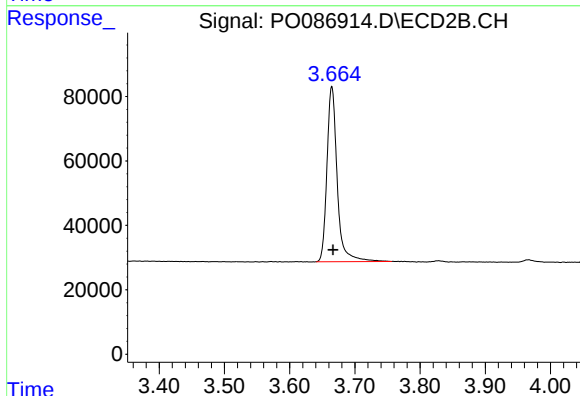


#1 Tetrachloro-m-xylene

R.T.: 3.665 min
Delta R.T.: -0.002 min
Response: 595343
Conc: 18.63 ng/ml

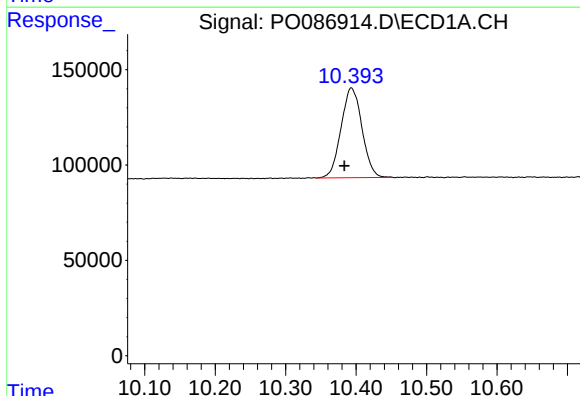

#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.010 min
Response: 971361
Conc: 21.28 ng/ml

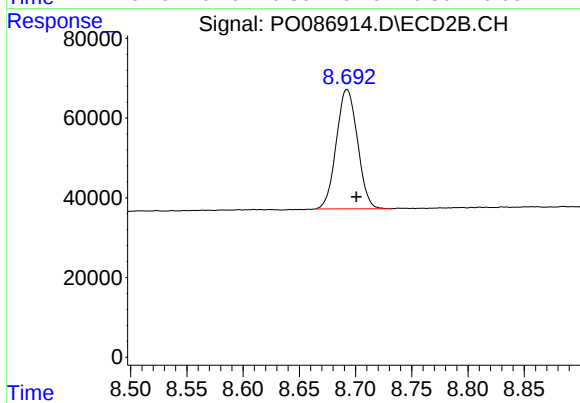

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: -0.008 min
Response: 393691
Conc: 17.56 ng/ml