

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060421\
 Data File : P0078442.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 14:15
 Operator : DD\AJ
 Sample : M2597-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 124042

Manual Integrations
 APPROVED

Ankita
 6/8/2021 12:30:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:38:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.617	1851290	824826	25.049	27.297
2) SA Decachlor...	9.949	8.804	1124171	659799	22.738m	22.691m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060421\
Data File : P0078442.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 14:15
Operator : DD\AJ
Sample : M2597-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
124042


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:38:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

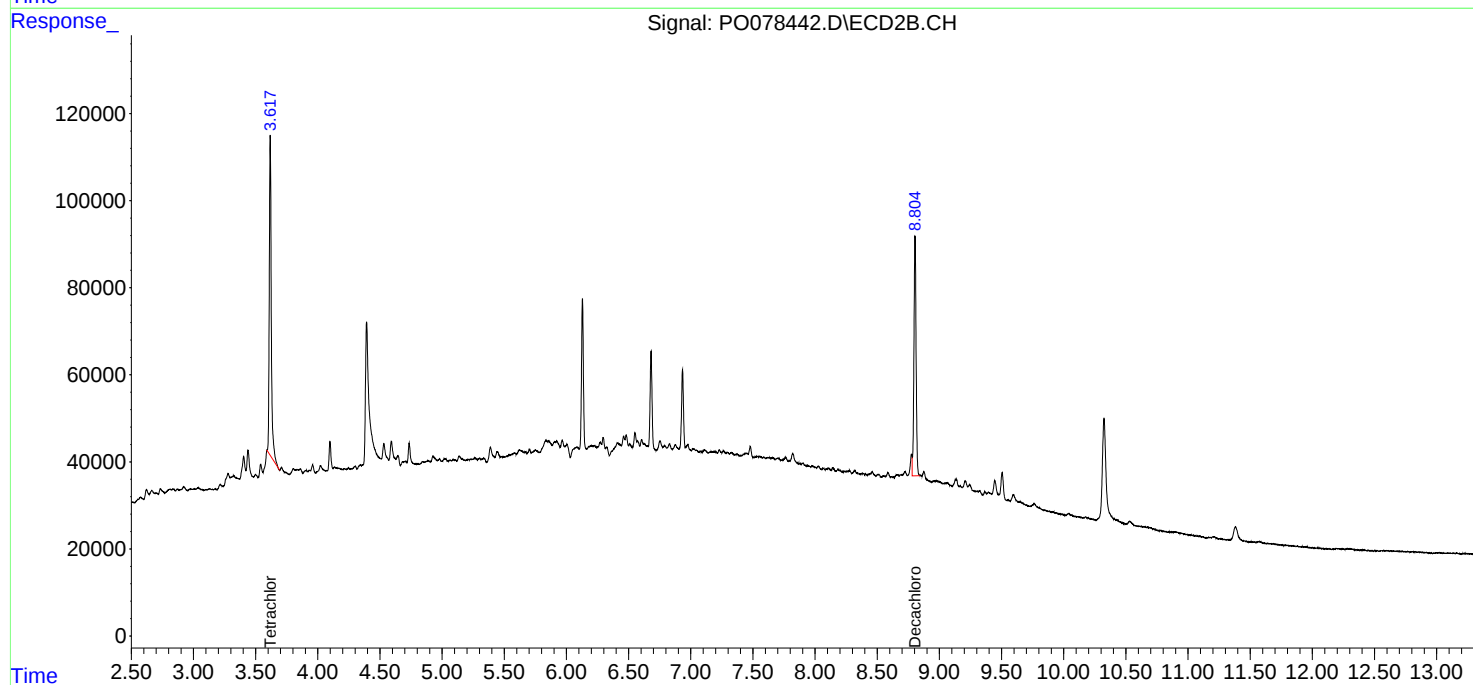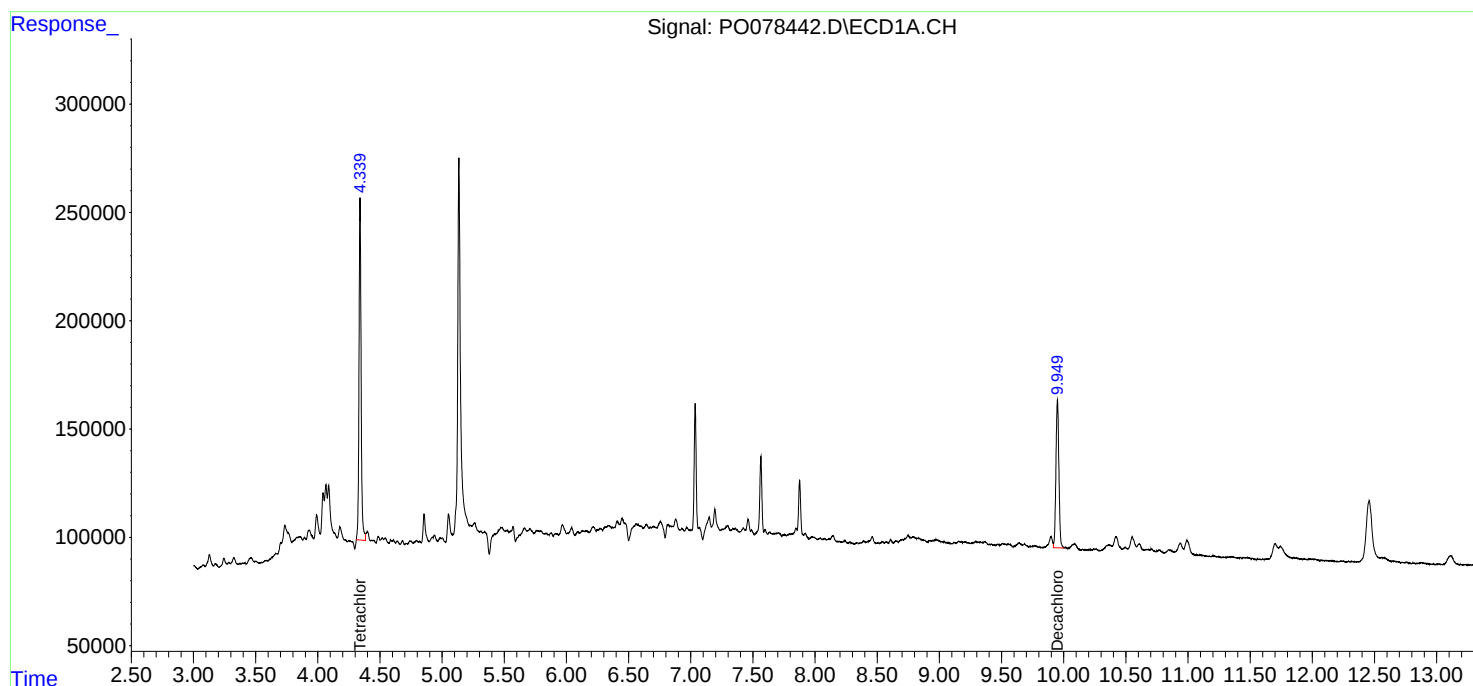

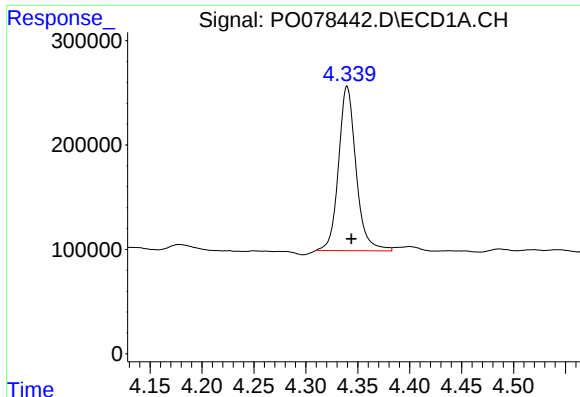


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 1851290
Conc: 25.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
124042


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:15 PM

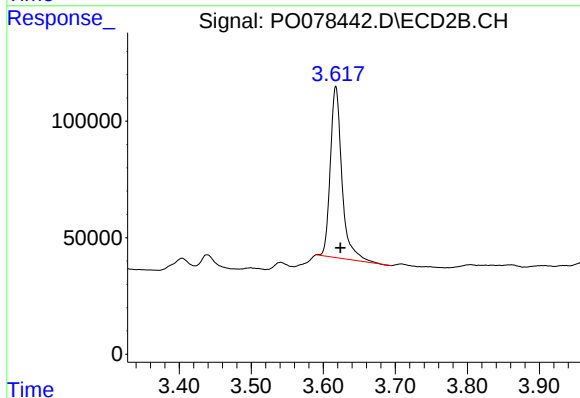


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.006 min
Response: 824826
Conc: 27.30 ng/ml

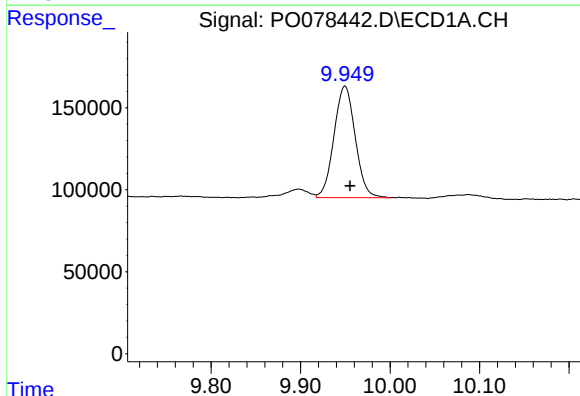

#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.006 min
Response: 1124171
Conc: 22.74 ng/ml m

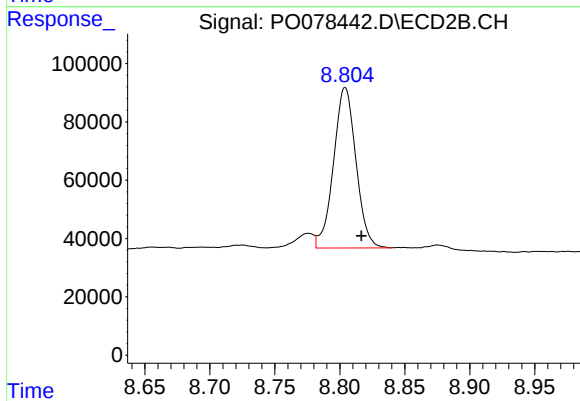

#2 Decachlorobiphenyl

R.T.: 8.804 min
Delta R.T.: -0.013 min
Response: 659799
Conc: 22.69 ng/ml m