

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060421\
 Data File : P0078450.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Jun 2021 17:08
 Operator : DD\AJ
 Sample : AR1248CCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1248CCC500

Manual Integrations
 APPROVED

Ankita
 6/8/2021 12:30:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 01:44:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.339	3.617	3720969	1596275	50.346	52.828
2) SA Decachlor...	9.949	8.803	2375923	1368963	48.056	47.080
Target Compounds						
21) L5 AR-1248-1	5.635	4.844	725642	352190	509.257	546.503m
22) L5 AR-1248-2	5.925	5.104	996955	478155	525.127	500.191
23) L5 AR-1248-3	6.136	5.146	1191170	486839	537.035	506.471
24) L5 AR-1248-4	6.558	5.327	1256150	563018	539.667m	491.606
25) L5 AR-1248-5	6.596	5.743	1236668	564296	546.576m	538.529

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO078450.D
Data File : PO078450.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Jun 2021 17:08
Operator : DD\AJ
Sample : AR1248CCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 01:44:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

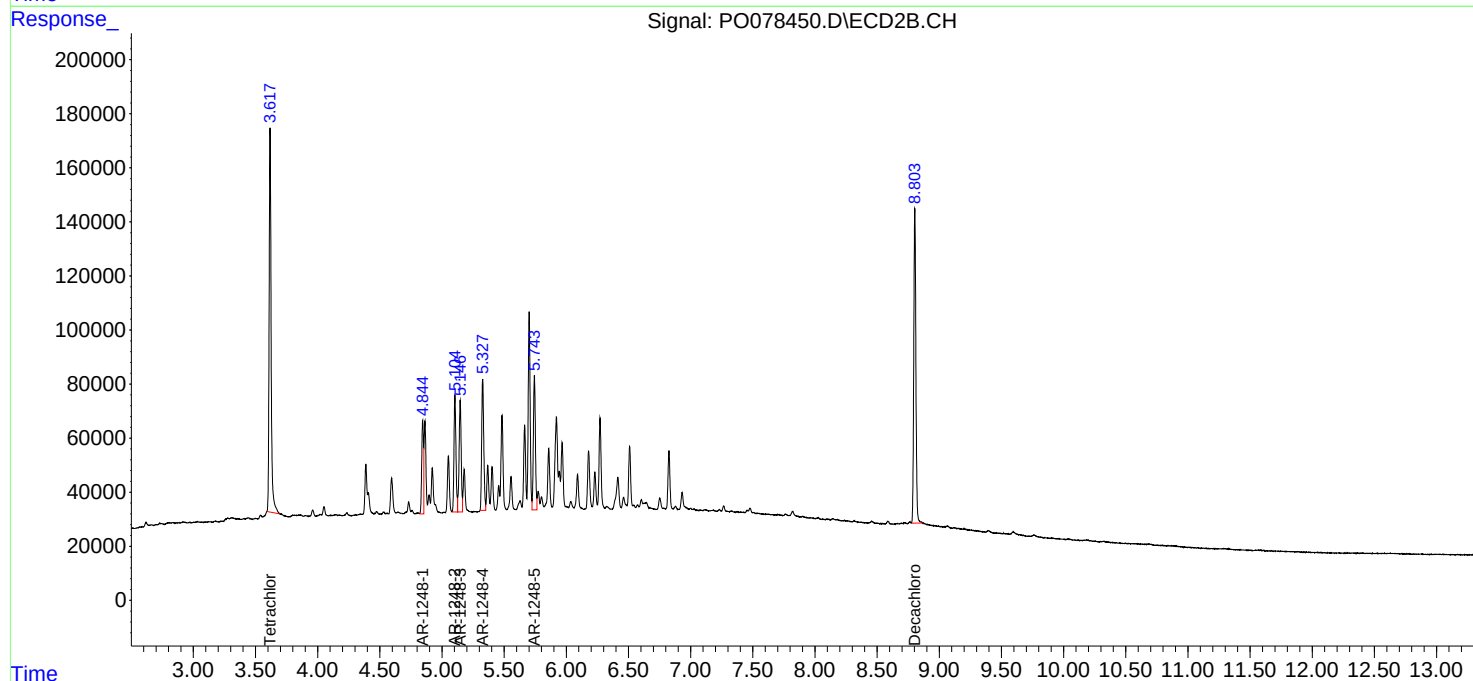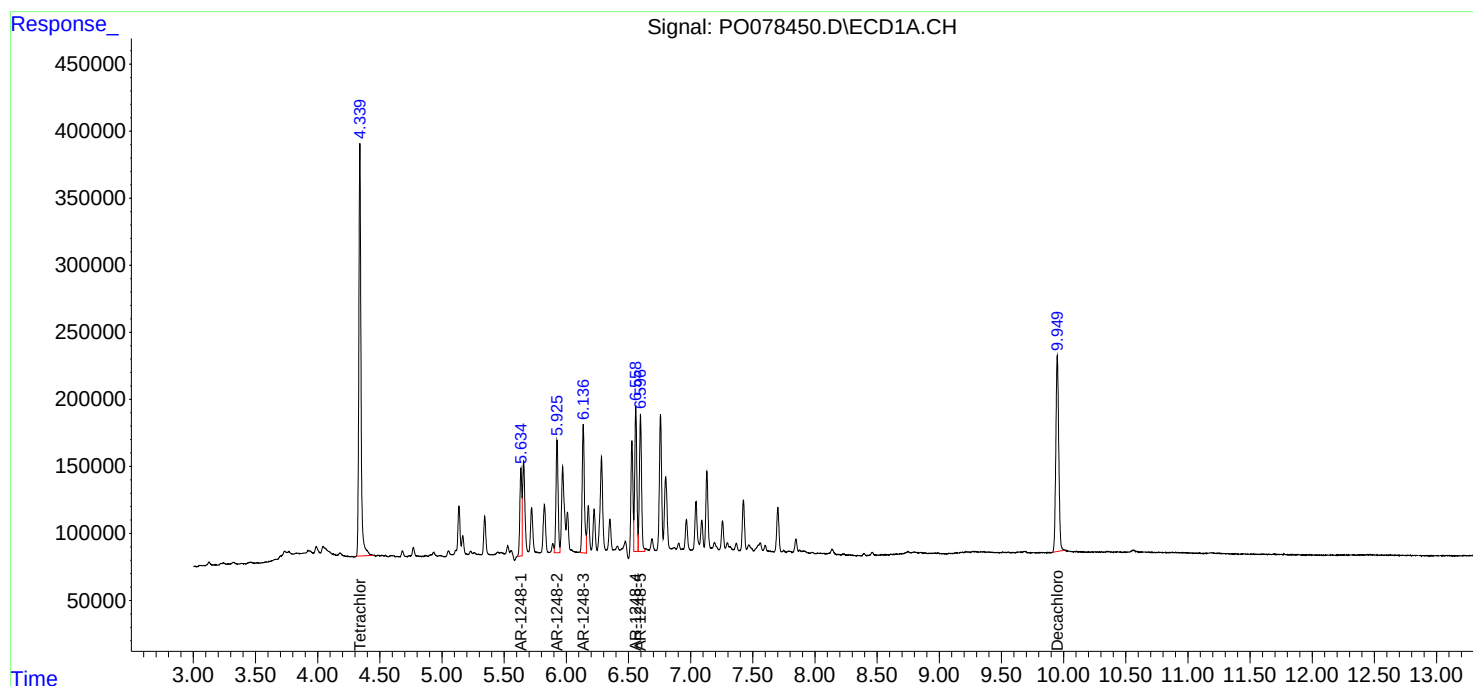

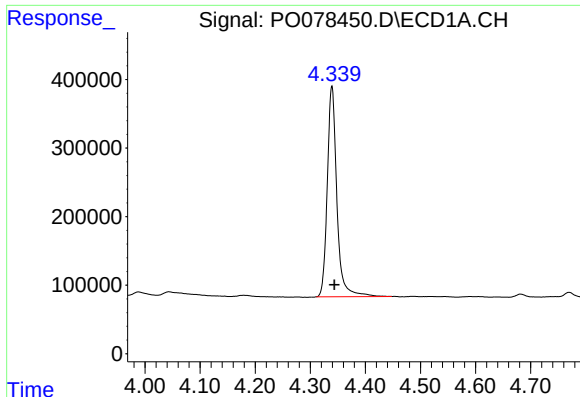


#1 Tetrachloro-m-xylene

R.T.: 4.339 min
Delta R.T.: -0.005 min
Response: 3720969
Conc: 50.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:37 PM

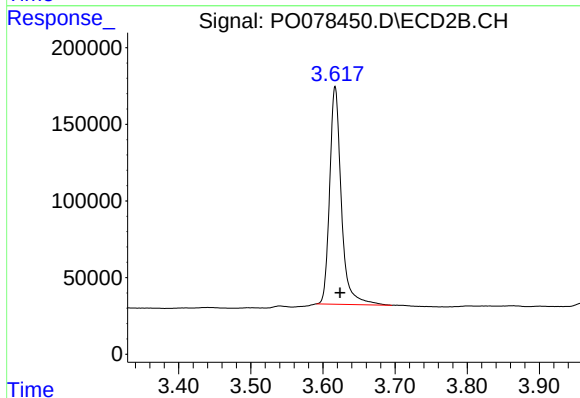


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.007 min
Response: 1596275
Conc: 52.83 ng/ml

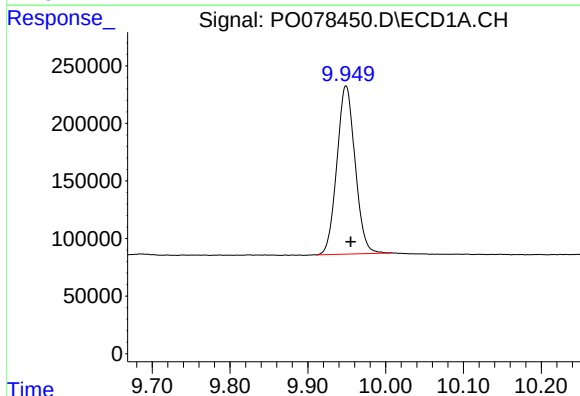


#2 Decachlorobiphenyl

R.T.: 9.949 min
Delta R.T.: -0.006 min
Response: 2375923
Conc: 48.06 ng/ml

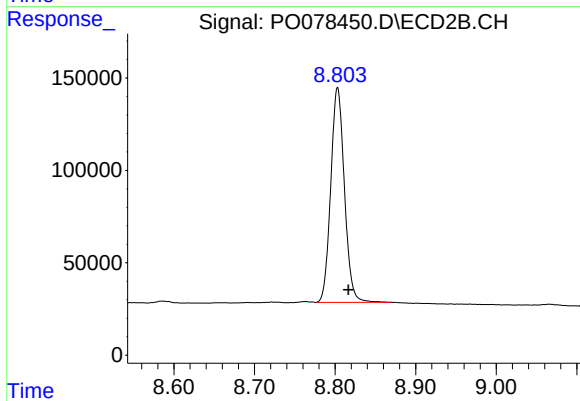

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.013 min
Response: 1368963
Conc: 47.08 ng/ml

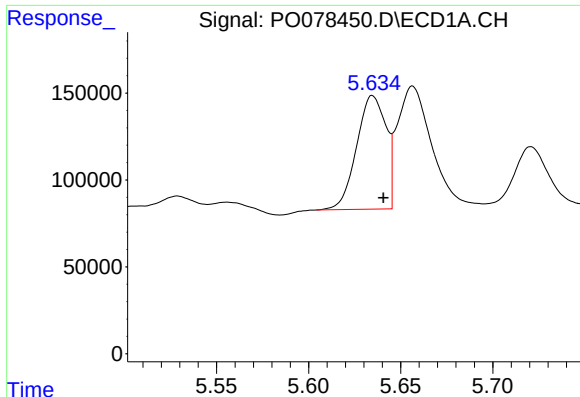


#21 AR-1248-1

R.T.: 5.635 min
Delta R.T.: -0.006 min
Response: 725642
Conc: 509.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:37 PM

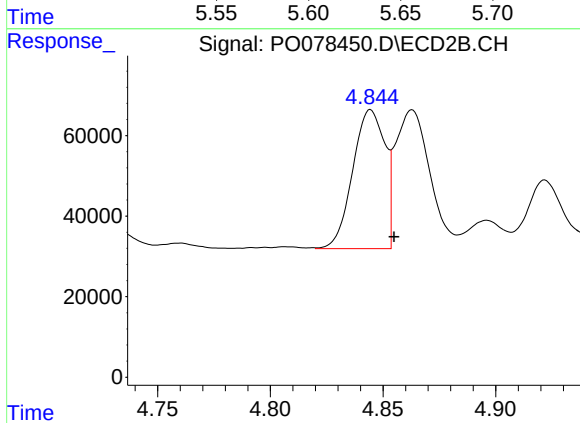


#21 AR-1248-1

R.T.: 4.844 min
Delta R.T.: -0.011 min
Response: 352190
Conc: 546.50 ng/ml m

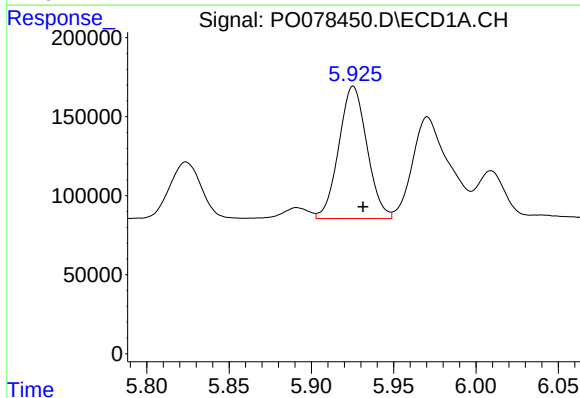


#22 AR-1248-2

R.T.: 5.925 min
Delta R.T.: -0.006 min
Response: 996955
Conc: 525.13 ng/ml

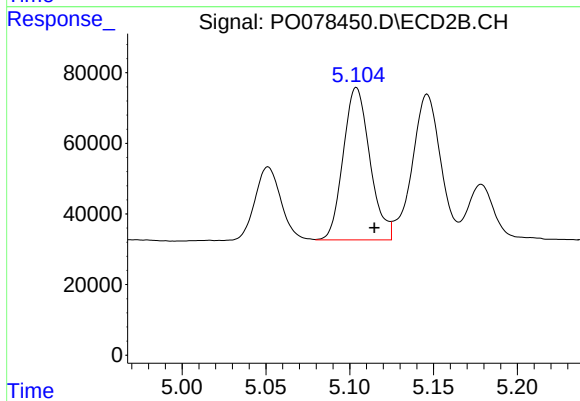

#22 AR-1248-2

R.T.: 5.104 min
Delta R.T.: -0.011 min
Response: 478155
Conc: 500.19 ng/ml

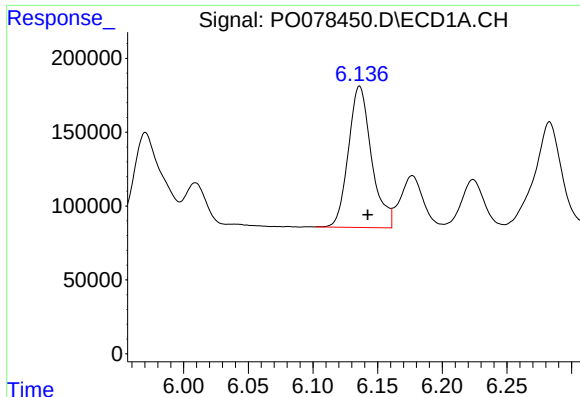


#23 AR-1248-3

R.T.: 6.136 min
Delta R.T.: -0.006 min
Response: 1191170
Conc: 537.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500


Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:37 PM

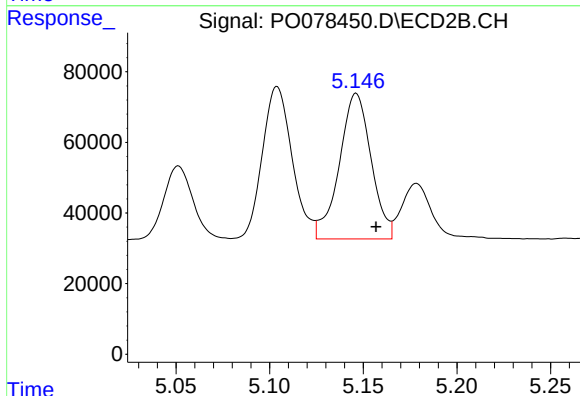


#23 AR-1248-3

R.T.: 5.146 min
Delta R.T.: -0.011 min
Response: 486839
Conc: 506.47 ng/ml

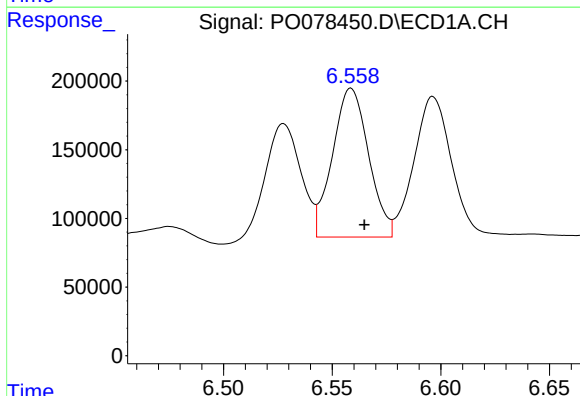


#24 AR-1248-4

R.T.: 6.558 min
Delta R.T.: -0.007 min
Response: 1256150
Conc: 539.67 ng/ml m

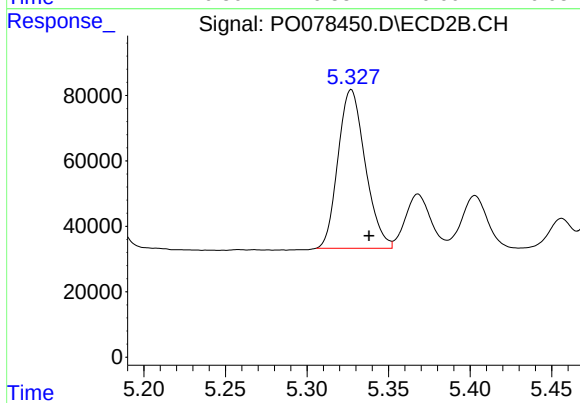

#24 AR-1248-4

R.T.: 5.327 min
Delta R.T.: -0.011 min
Response: 563018
Conc: 491.61 ng/ml

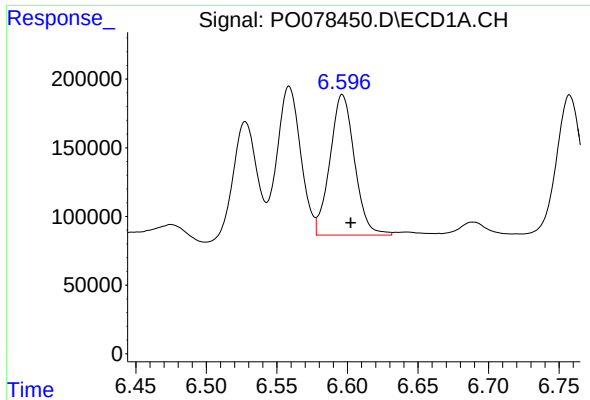


#25 AR-1248-5

R.T.: 6.596 min
Delta R.T.: -0.006 min
Response: 1236668
Conc: 546.58 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1248CCC500

Manual Integrations
APPROVED

Ankita
6/8/2021 12:30:37 PM

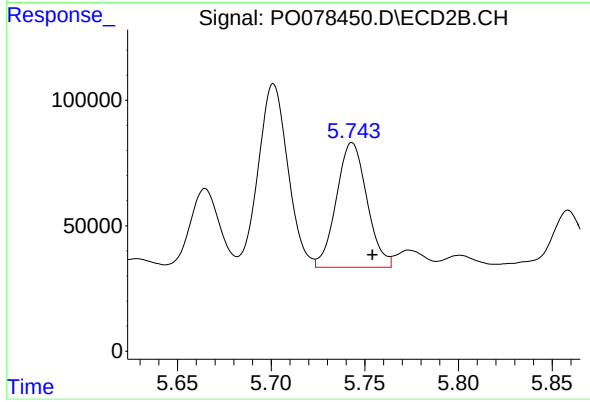

#25 AR-1248-5

R.T.: 5.743 min
Delta R.T.: -0.011 min
Response: 564296
Conc: 538.53 ng/ml