

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0060521\
 Data File : P0078460.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2021 8:18
 Operator : DD\AJ
 Sample : M2598-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 23

Manual Integrations
 APPROVED

Ankita
 6/10/2021 3:15:09 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:25:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.617	1665155	729827	22.530	24.154
2) SA Decachlor...	9.947	8.803	1024560	637140	20.723m	21.912
Target Compounds						
26) L6 AR-1254-1	6.542	5.701	77142	32751	31.081m	18.990 #
27) L6 AR-1254-2	6.757	5.859	82257	19158	21.197m	11.952m#
28) L6 AR-1254-3	7.147	6.270	286554	33832	73.038m	14.175m#
29) L6 AR-1254-4	7.422	6.510	58546	20840	21.559m	14.354m#
30) L6 AR-1254-5	7.846	6.932	84786	98216	28.992	43.211 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060521\
Data File : P0078460.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2021 8:18
Operator : DD\AJ
Sample : M2598-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
23


Manual Integrations
APPROVED

Ankita
6/10/2021 3:15:09 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:25:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

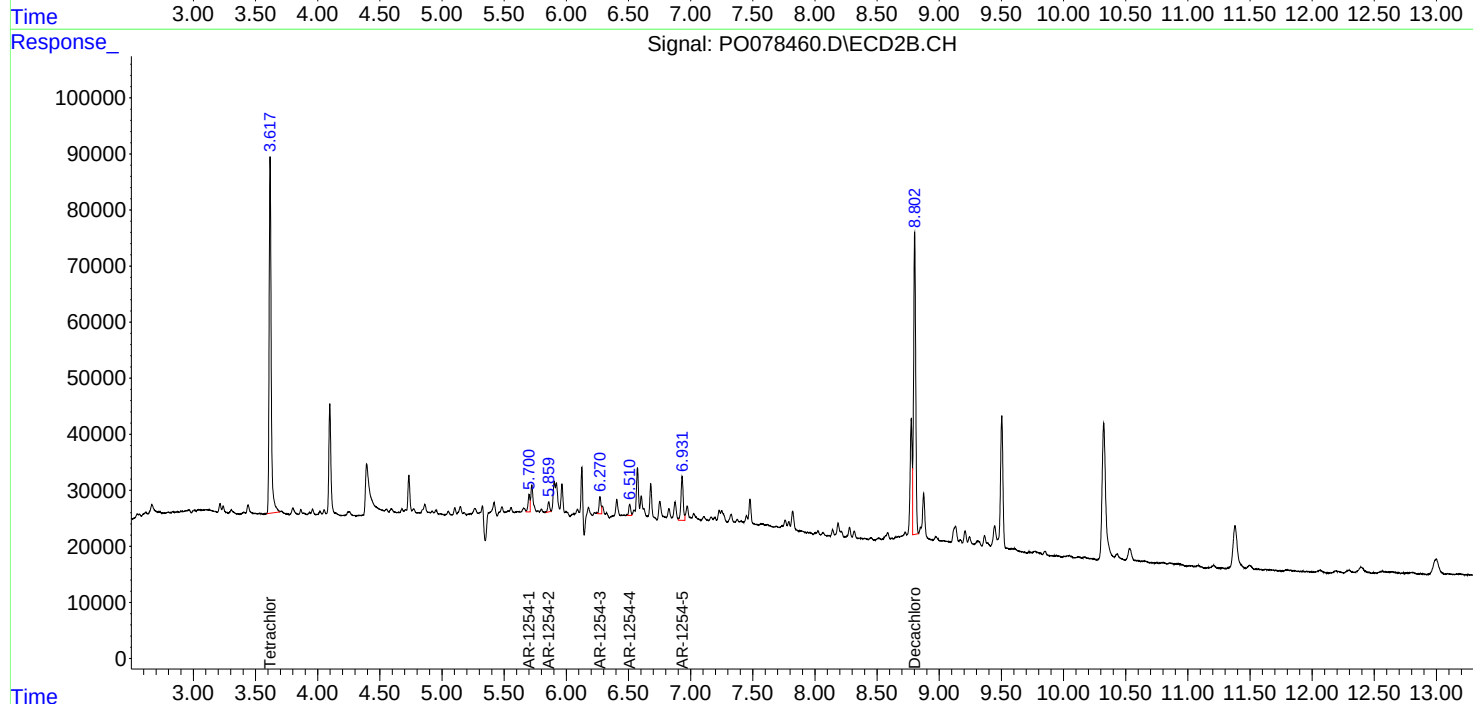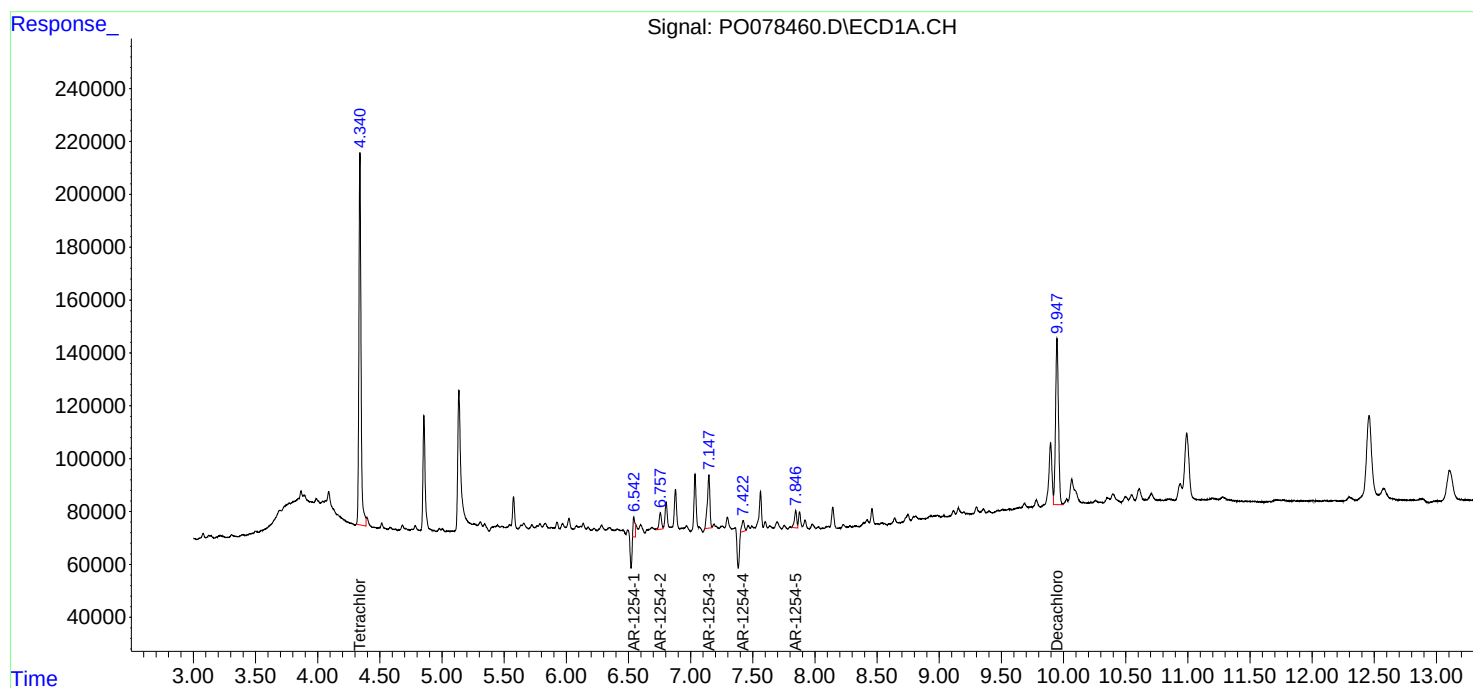

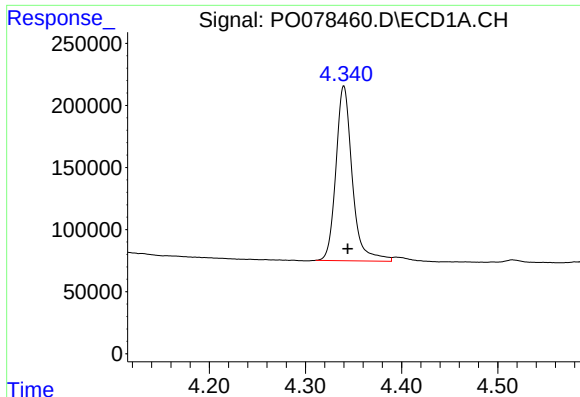


#1 Tetrachloro-m-xylene

R.T.: 4.340 min
Delta R.T.: -0.004 min
Response: 1665155
Conc: 22.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/10/2021 3:15:09 PM

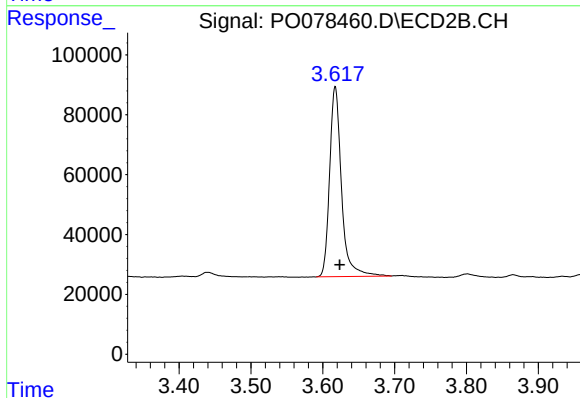


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: -0.006 min
Response: 729827
Conc: 24.15 ng/ml

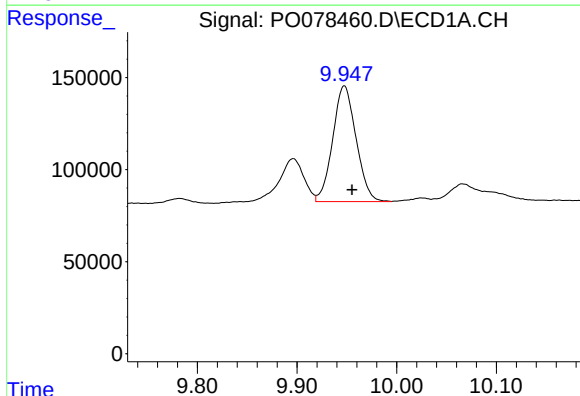


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 1024560
Conc: 20.72 ng/ml m

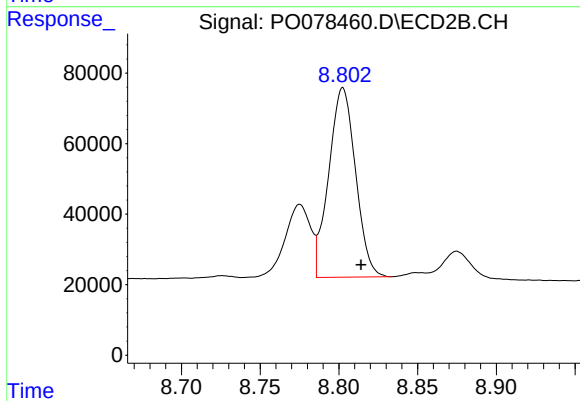

#2 Decachlorobiphenyl

R.T.: 8.803 min
Delta R.T.: -0.011 min
Response: 637140
Conc: 21.91 ng/ml

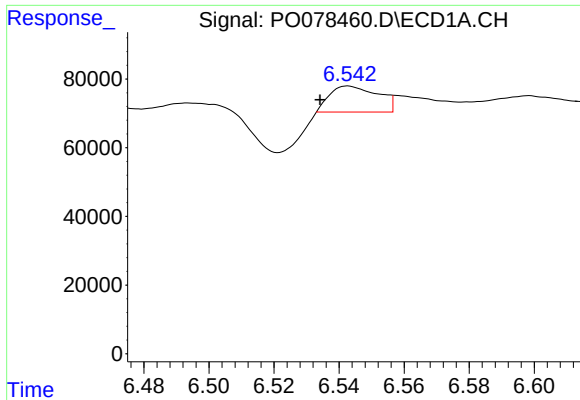


#26 AR-1254-1

R.T.: 6.542 min
Delta R.T.: 0.008 min
Response: 77142
Conc: 31.08 ng/ml m

Instrument :
ECD_O
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/10/2021 3:15:09 PM

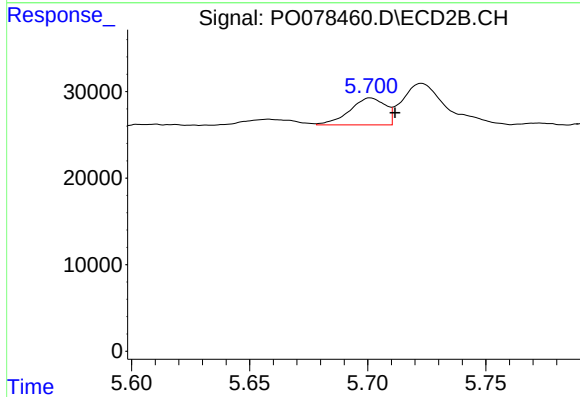


#26 AR-1254-1

R.T.: 5.701 min
Delta R.T.: -0.011 min
Response: 32751
Conc: 18.99 ng/ml

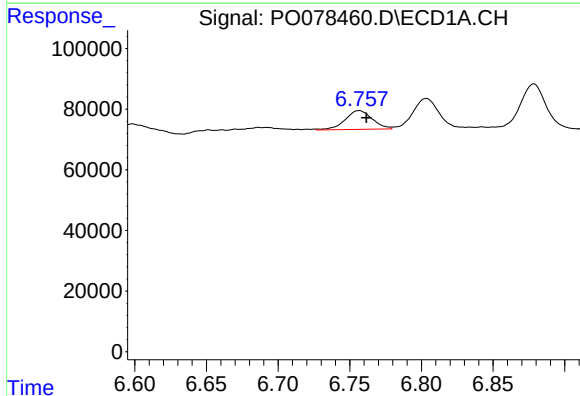


#27 AR-1254-2

R.T.: 6.757 min
Delta R.T.: -0.005 min
Response: 82257
Conc: 21.20 ng/ml m

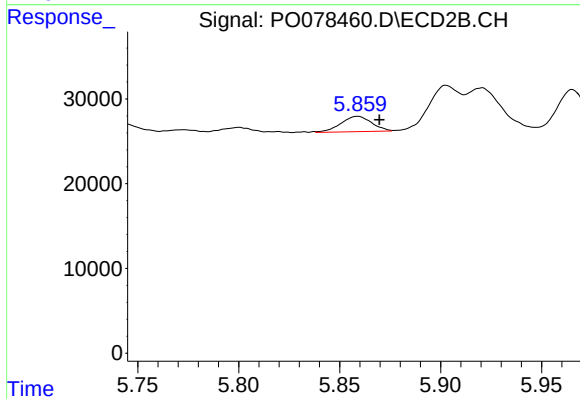

#27 AR-1254-2

R.T.: 5.859 min
Delta R.T.: -0.011 min
Response: 19158
Conc: 11.95 ng/ml m

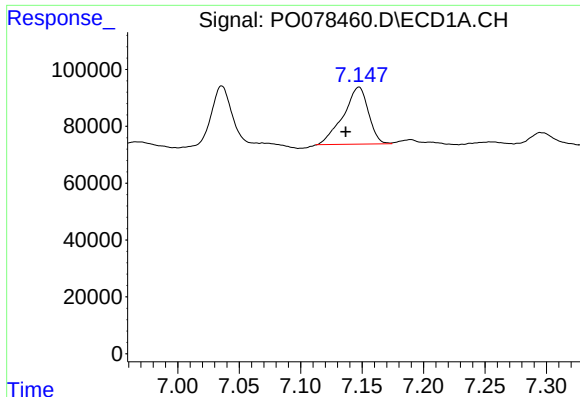


#28 AR-1254-3

R.T.: 7.147 min
Delta R.T.: 0.010 min
Response: 286554
Conc: 73.04 ng/ml m

Instrument :
ECD_O
ClientSampleId :
23


Manual Integrations
APPROVED

Ankita
6/10/2021 3:15:09 PM

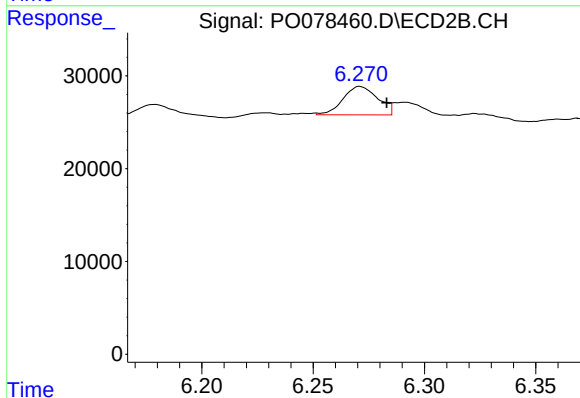


#28 AR-1254-3

R.T.: 6.270 min
Delta R.T.: -0.013 min
Response: 33832
Conc: 14.17 ng/ml m

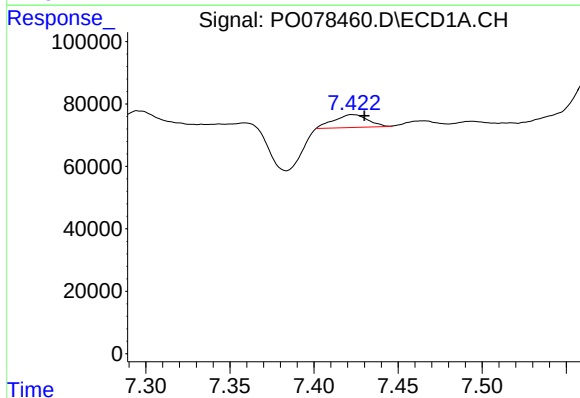


#29 AR-1254-4

R.T.: 7.422 min
Delta R.T.: -0.008 min
Response: 58546
Conc: 21.56 ng/ml m

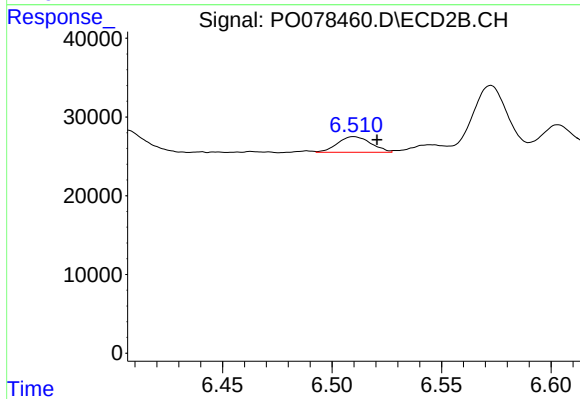

#29 AR-1254-4

R.T.: 6.510 min
Delta R.T.: -0.011 min
Response: 20840
Conc: 14.35 ng/ml m

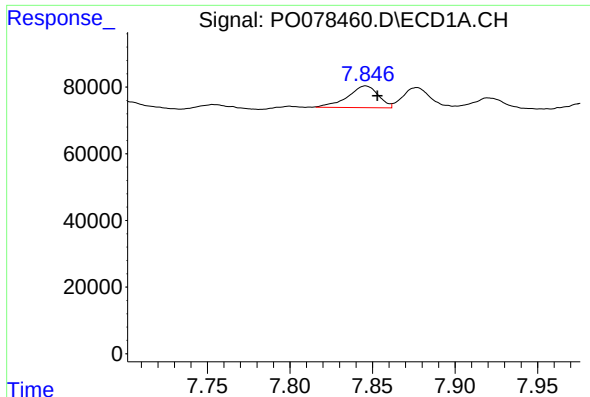


#30 AR-1254-5

R.T.: 7.846 min
Delta R.T.: -0.007 min
Response: 84786
Conc: 28.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
23

Manual Integrations
APPROVED

Ankita
6/10/2021 3:15:09 PM

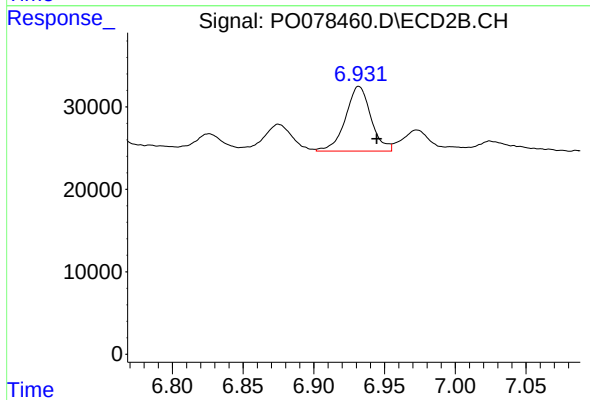

#30 AR-1254-5

R.T.: 6.932 min
Delta R.T.: -0.013 min
Response: 98216
Conc: 43.21 ng/ml