

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060521\
 Data File : P0078463.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Jun 2021 9:10
 Operator : DD\AJ
 Sample : M2601-09
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RO-VNJ-212

Manual Integrations
 APPROVED

Ankita
 6/8/2021 12:04:13 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 06:34:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed May 19 06:28:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.338	3.616	1113744	542399	15.069	17.951
2) SA Decachlor...	9.947	8.801	1044840	655413	21.133	22.540m
Target Compounds						
31) L7 AR-1260-1	7.294	6.404	368458	239637	131.299	149.562
32) L7 AR-1260-2	7.559	6.601	690866	379651	205.365	196.652
33) L7 AR-1260-3	7.919	6.752	562662	263274	230.601	143.502 #
34) L7 AR-1260-4	8.143	7.229	796614	308444	297.384	204.613 #
35) L7 AR-1260-5	8.458	7.477	942390	612732	183.491	175.707

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060521\
Data File : P0078463.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Jun 2021 9:10
Operator : DD\AJ
Sample : M2601-09
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 12:04:13 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 06:34:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051821.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed May 19 06:28:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

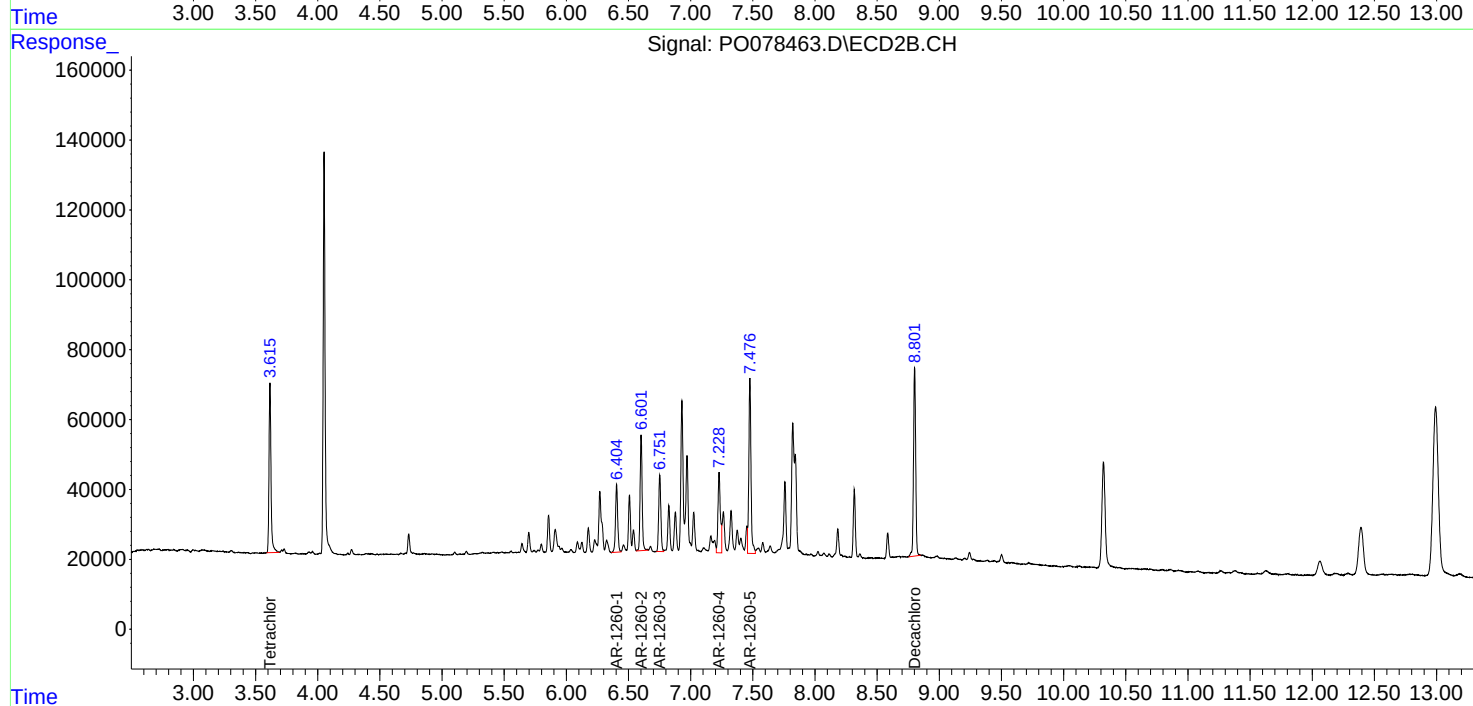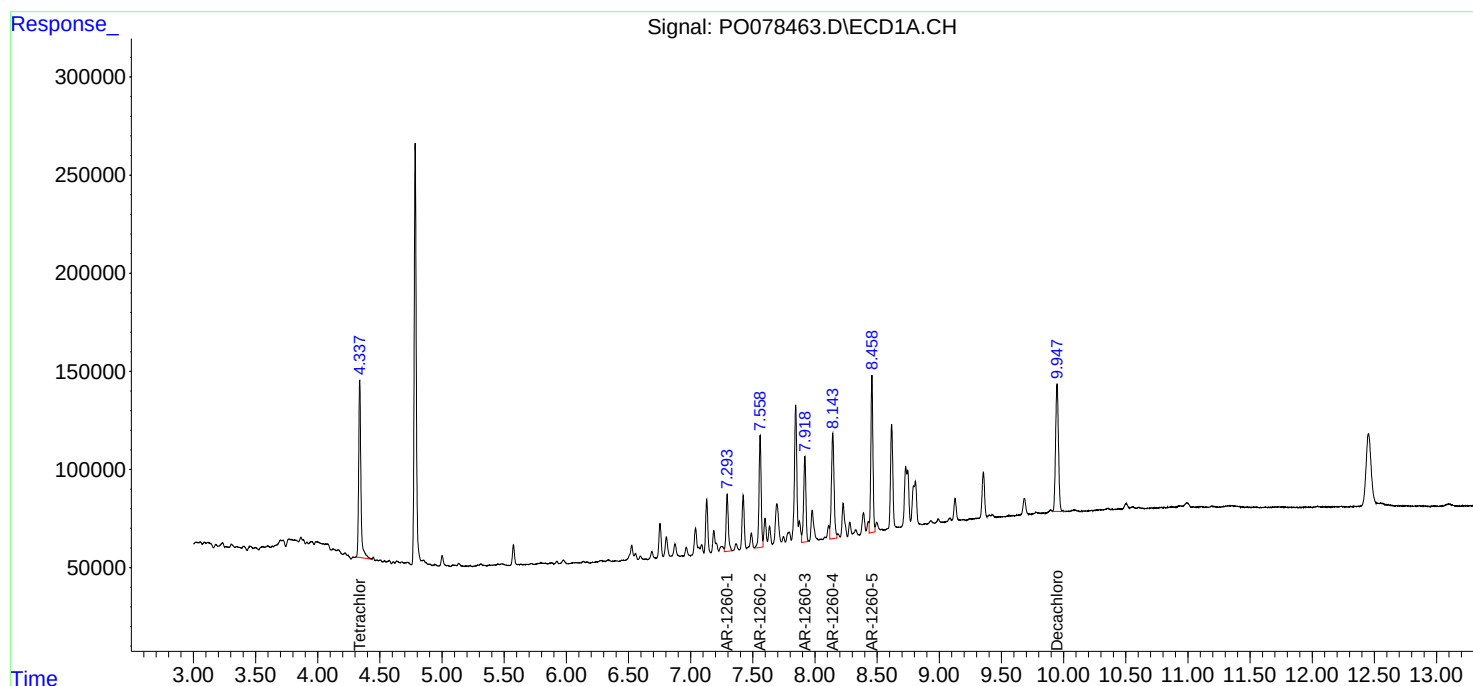

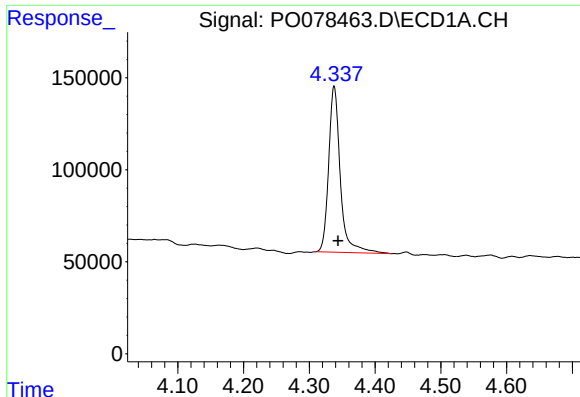


#1 Tetrachloro-m-xylene

R.T.: 4.338 min
Delta R.T.: -0.006 min
Response: 1113744
Conc: 15.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 12:04:13 PM

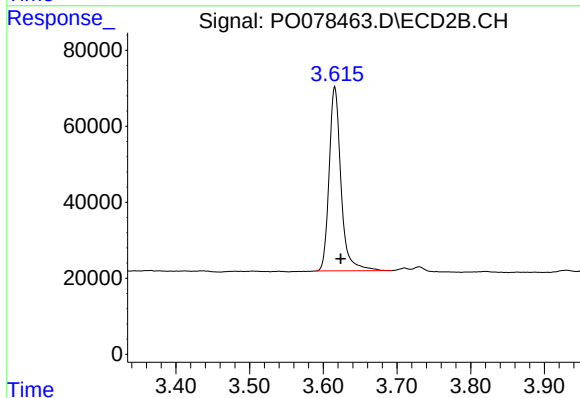


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.008 min
Response: 542399
Conc: 17.95 ng/ml

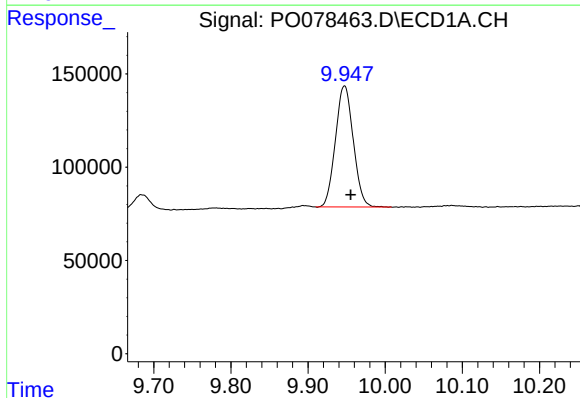


#2 Decachlorobiphenyl

R.T.: 9.947 min
Delta R.T.: -0.008 min
Response: 1044840
Conc: 21.13 ng/ml

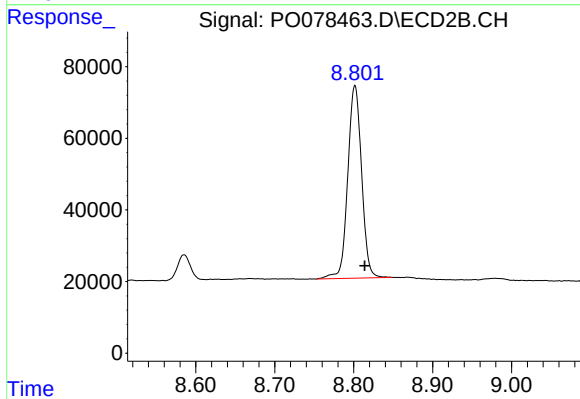

#2 Decachlorobiphenyl

R.T.: 8.801 min
Delta R.T.: -0.013 min
Response: 655413
Conc: 22.54 ng/ml m

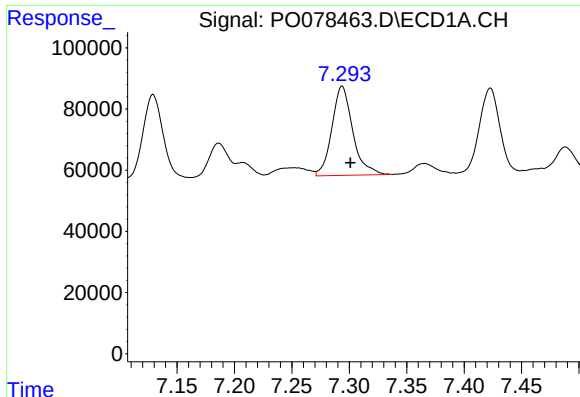


#31 AR-1260-1

R.T.: 7.294 min
Delta R.T.: -0.007 min
Response: 368458
Conc: 131.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 12:04:13 PM

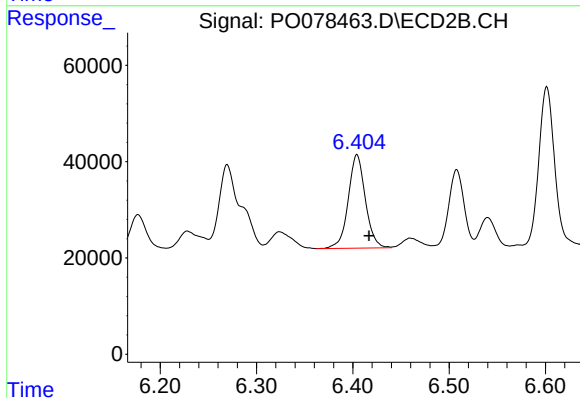


#31 AR-1260-1

R.T.: 6.404 min
Delta R.T.: -0.012 min
Response: 239637
Conc: 149.56 ng/ml

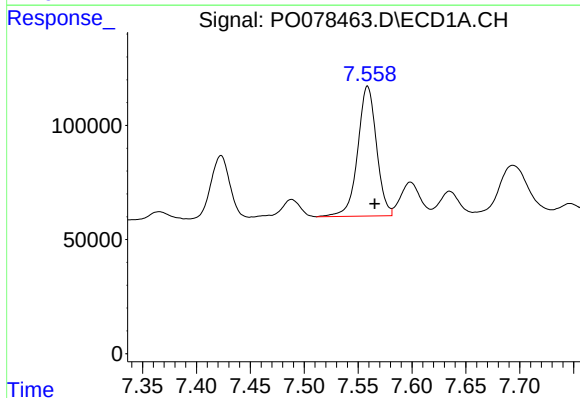


#32 AR-1260-2

R.T.: 7.559 min
Delta R.T.: -0.007 min
Response: 690866
Conc: 205.36 ng/ml

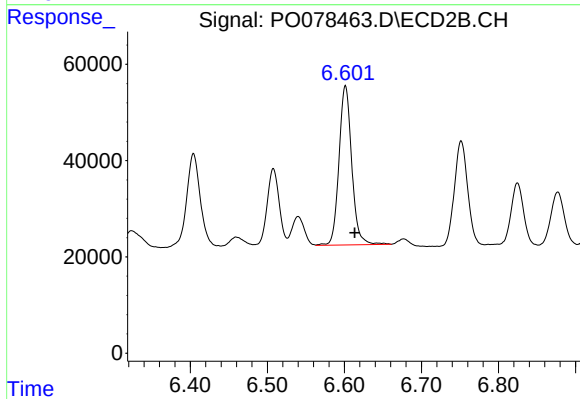

#32 AR-1260-2

R.T.: 6.601 min
Delta R.T.: -0.012 min
Response: 379651
Conc: 196.65 ng/ml

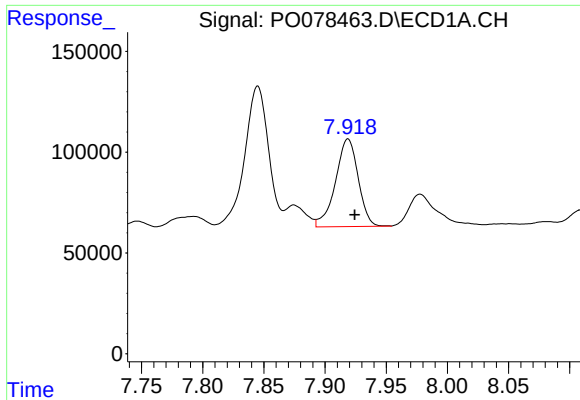


#33 AR-1260-3

R.T.: 7.919 min
Delta R.T.: -0.006 min
Response: 562662
Conc: 230.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-VNJ-212


Manual Integrations
APPROVED

Ankita
6/8/2021 12:04:13 PM

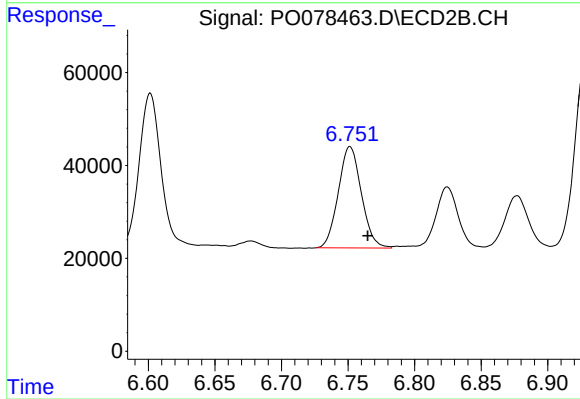


#33 AR-1260-3

R.T.: 6.752 min
Delta R.T.: -0.013 min
Response: 263274
Conc: 143.50 ng/ml

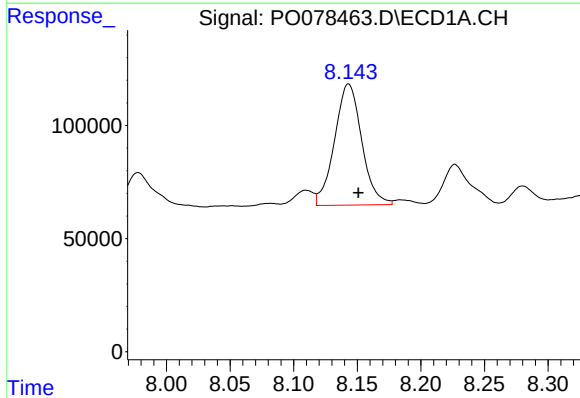


#34 AR-1260-4

R.T.: 8.143 min
Delta R.T.: -0.008 min
Response: 796614
Conc: 297.38 ng/ml

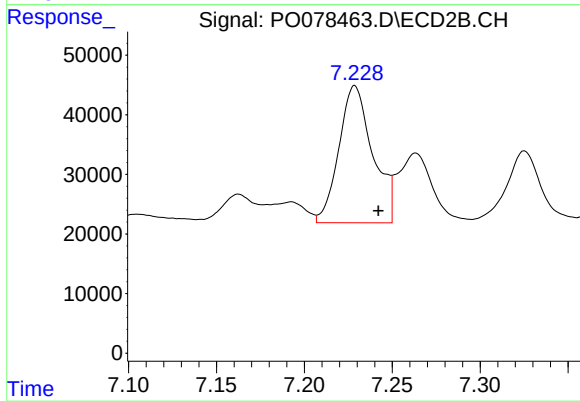

#34 AR-1260-4

R.T.: 7.229 min
Delta R.T.: -0.013 min
Response: 308444
Conc: 204.61 ng/ml

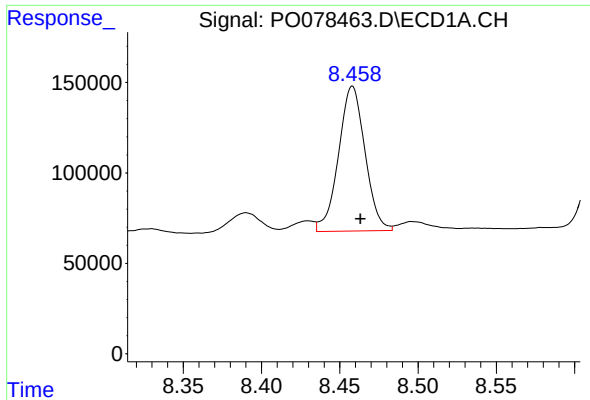


#35 AR-1260-5

R.T.: 8.458 min
Delta R.T.: -0.005 min
Response: 942390
Conc: 183.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
RO-VNJ-212

Manual Integrations
APPROVED

Ankita
6/8/2021 12:04:13 PM

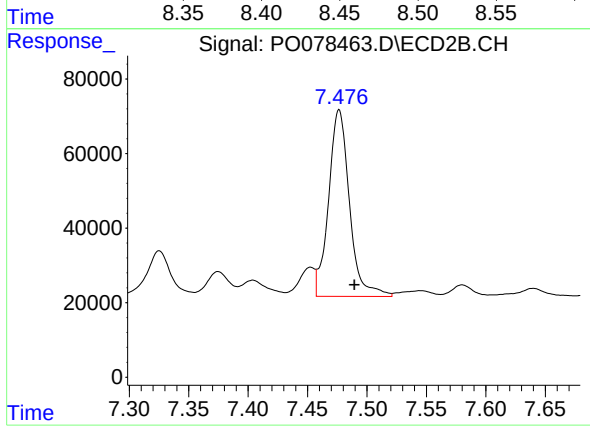

#35 AR-1260-5

R.T.: 7.477 min
Delta R.T.: -0.013 min
Response: 612732
Conc: 175.71 ng/ml