

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060525\
 Data File : P0111497.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jun 2025 15:07
 Operator : YP/AJ
 Sample : Q2218-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 72-11934

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/06/2025
 Supervised By :mohammad ahmed 06/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 05 16:19:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.680	3.676	129.6E6	112.4E6	22.032	20.610
2) SA Decachlor...	8.715	8.665	76916252	29225888	14.898	15.797m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060525\
Data File : PO111497.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jun 2025 15:07
Operator : YP/AJ
Sample : Q2218-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
72-11934


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2025
Supervised By :mohammad ahmed 06/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 05 16:19:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

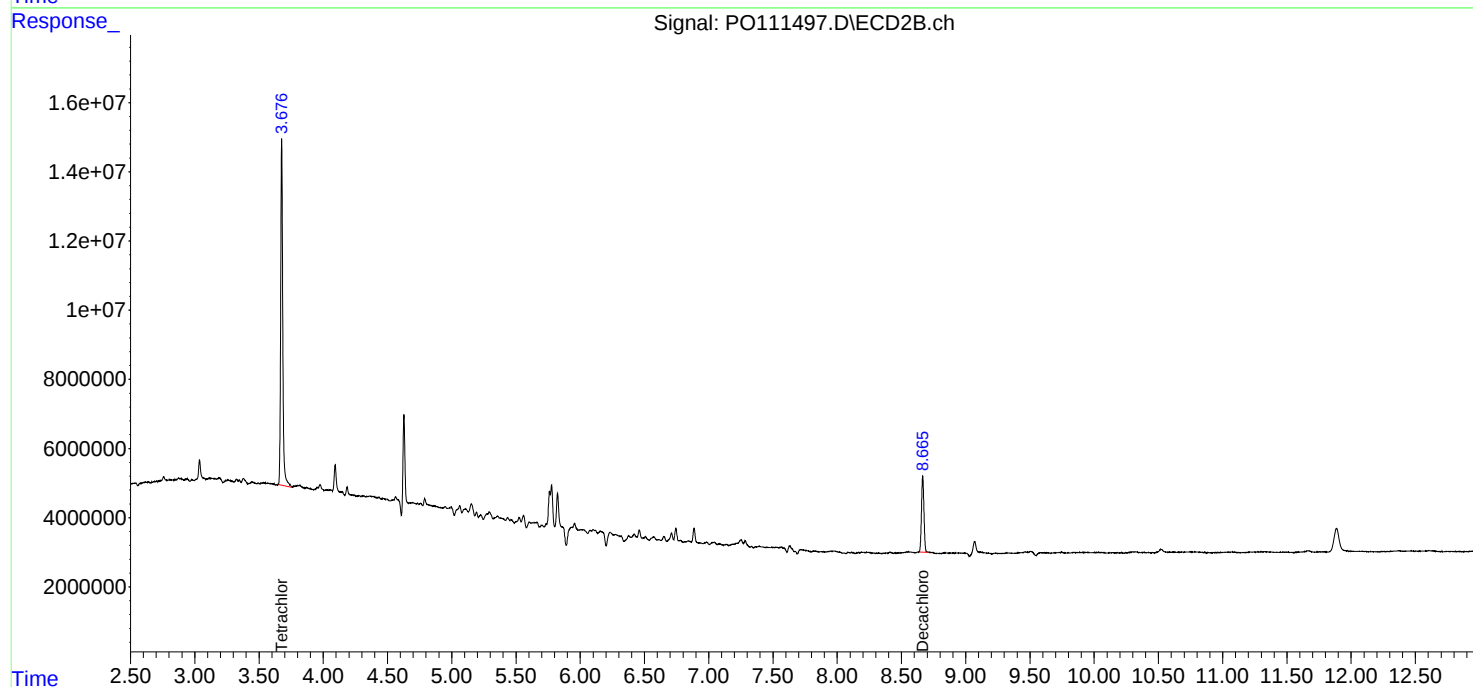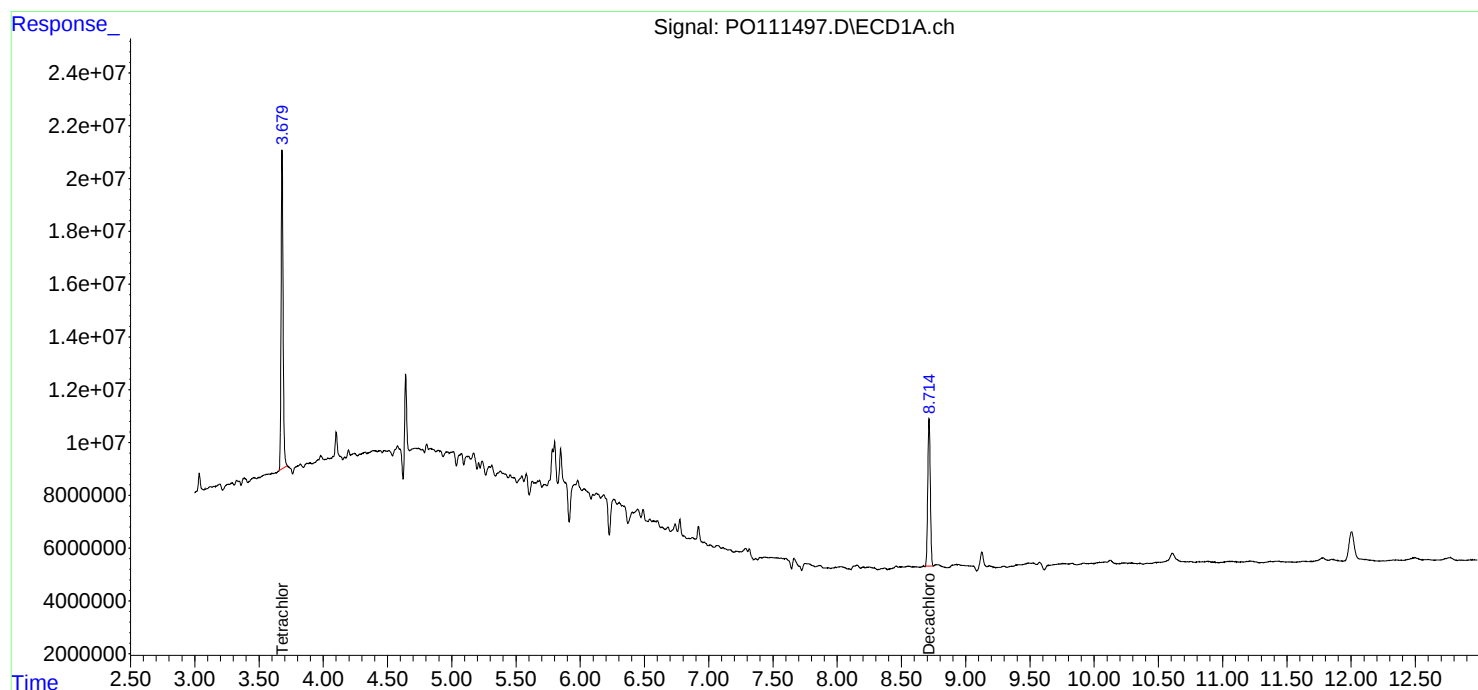

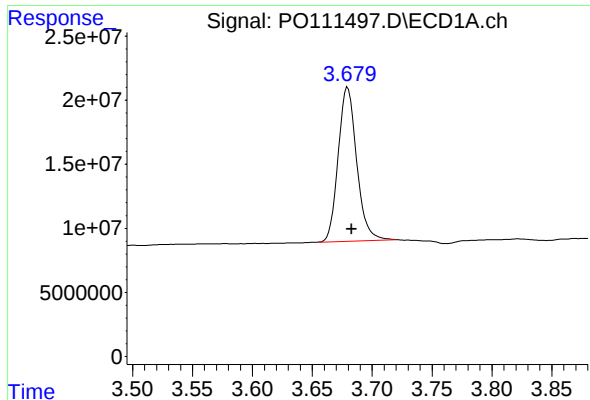


#1 Tetrachloro-m-xylene

R.T.: 3.680 min
Delta R.T.: -0.003 min
Response: 129618762
Conc: 22.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
72-11934


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/06/2025
Supervised By :mohammad ahmed 06/09/2025

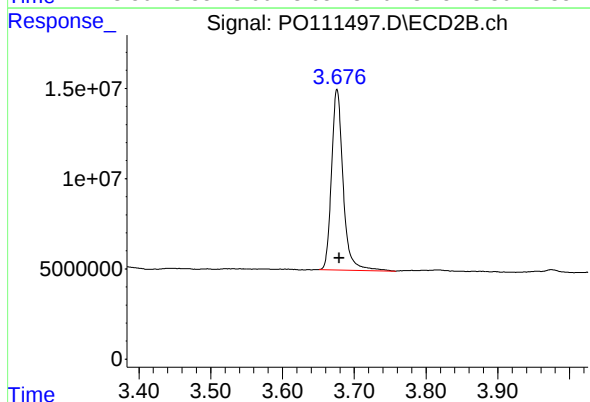


#1 Tetrachloro-m-xylene

R.T.: 3.676 min
Delta R.T.: -0.003 min
Response: 112353974
Conc: 20.61 ng/ml

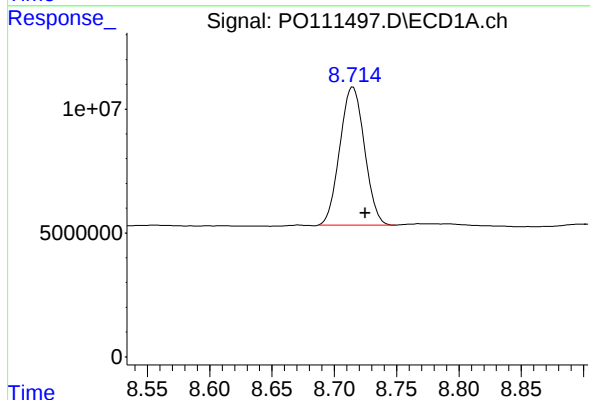

#2 Decachlorobiphenyl

R.T.: 8.715 min
Delta R.T.: -0.010 min
Response: 76916252
Conc: 14.90 ng/ml

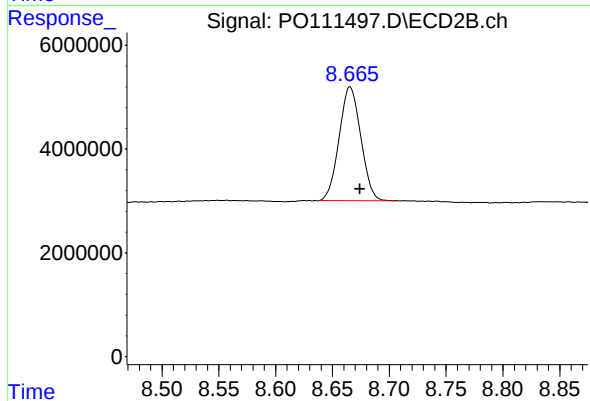

#2 Decachlorobiphenyl

R.T.: 8.665 min
Delta R.T.: -0.009 min
Response: 29225888
Conc: 15.80 ng/ml m