

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060622\
 Data File : P0086920.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2022 10:26
 Operator : YP\AJ
 Sample : N3122-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TB-TRANS-0531

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:16:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.514	3.663	1341120	657434	23.450	20.568
2) SA Decachlor...	10.387	8.686	1247242	498035	27.324	22.211m
Target Compounds						
16) L4 AR-1242-1	5.698	4.756	161660	70094	101.132	89.226
17) L4 AR-1242-2	5.722	4.775	202655	83788	88.954	77.518
18) L4 AR-1242-3	5.784	4.951	143843	51274	101.279	86.846
19) L4 AR-1242-4	5.884	5.036	107806	63471	95.122	110.920
20) L4 AR-1242-5	6.627	5.559	170420	93260	144.924	138.865

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060622\
Data File : PO086920.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2022 10:26
Operator : YP\AJ
Sample : N3122-02
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
TB-TRANS-0531


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:16:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

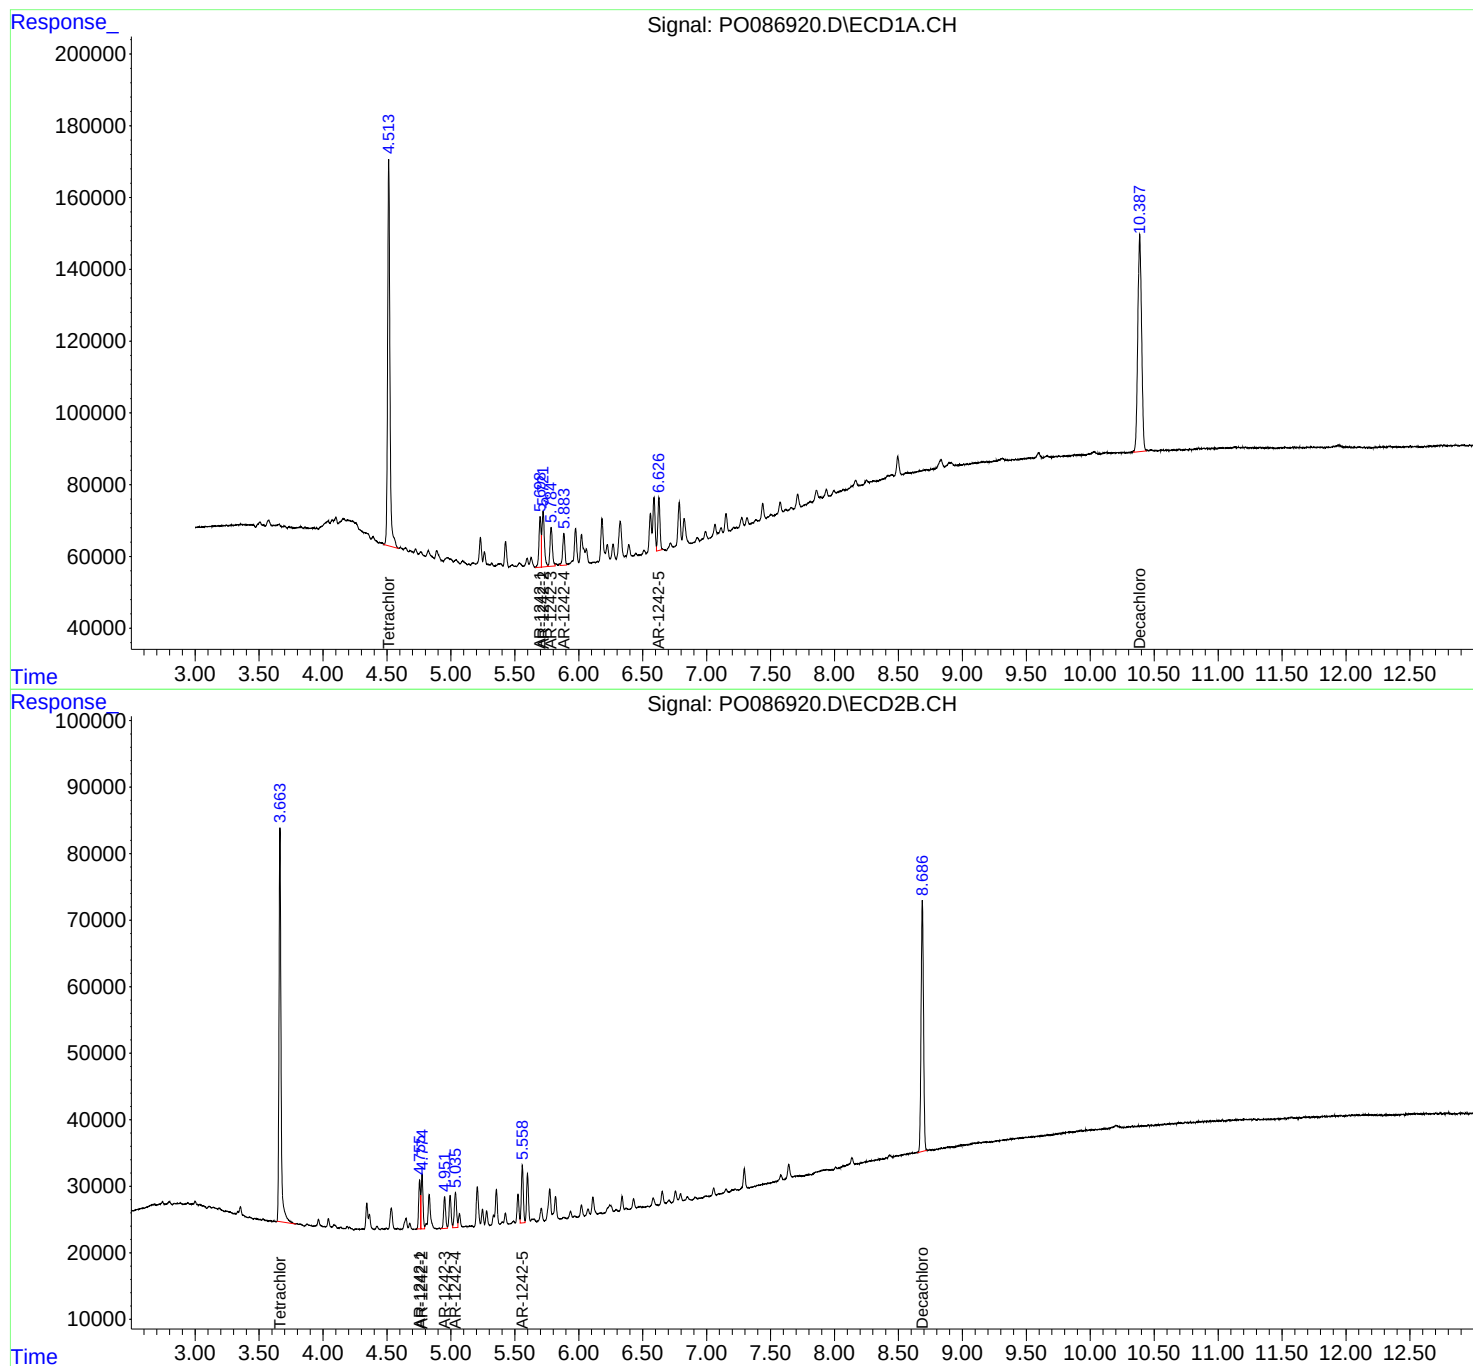

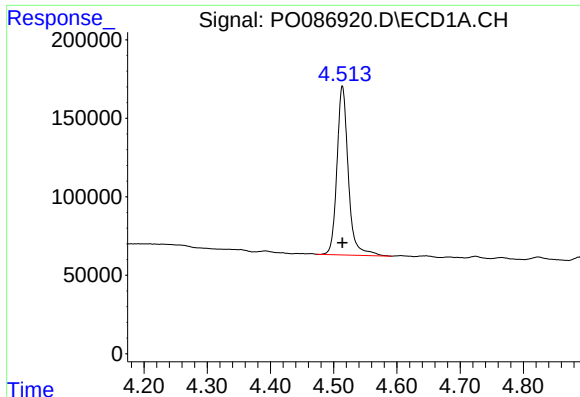


#1 Tetrachloro-m-xylene

R.T.: 4.514 min
Delta R.T.: 0.000 min
Response: 1341120
Conc: 23.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
TB-TRANS-0531


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

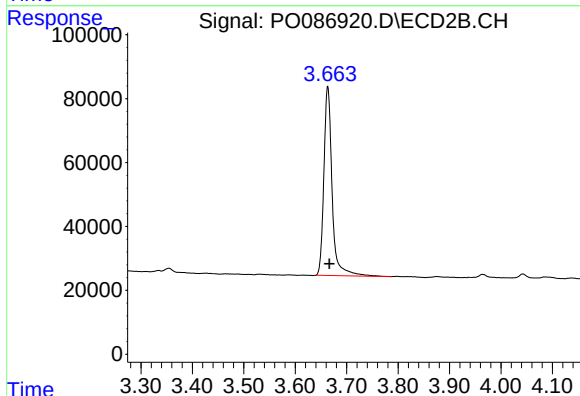


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.003 min
Response: 657434
Conc: 20.57 ng/ml

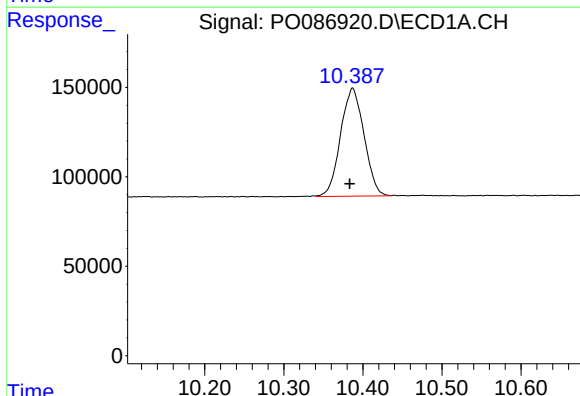


#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.004 min
Response: 1247242
Conc: 27.32 ng/ml

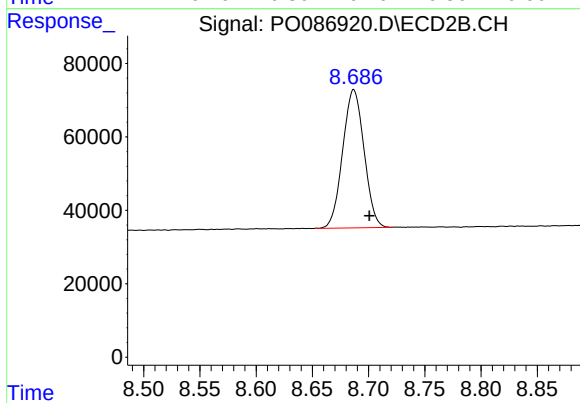

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.014 min
Response: 498035
Conc: 22.21 ng/ml m

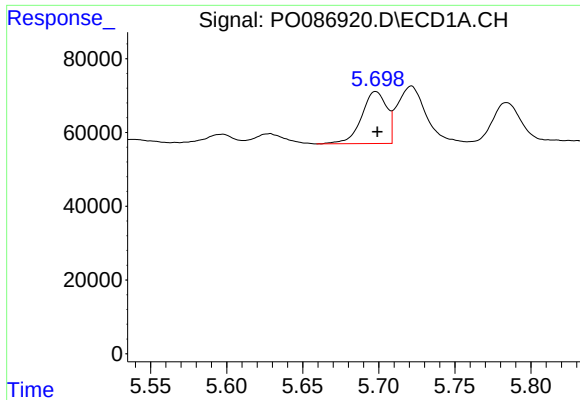


#16 AR-1242-1

R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 161660
Conc: 101.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
TB-TRANS-0531


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

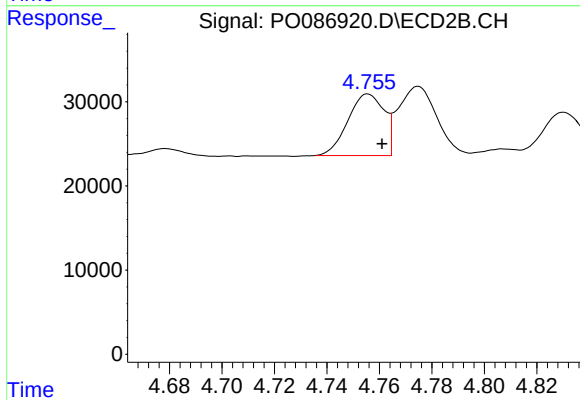


#16 AR-1242-1

R.T.: 4.756 min
Delta R.T.: -0.005 min
Response: 70094
Conc: 89.23 ng/ml

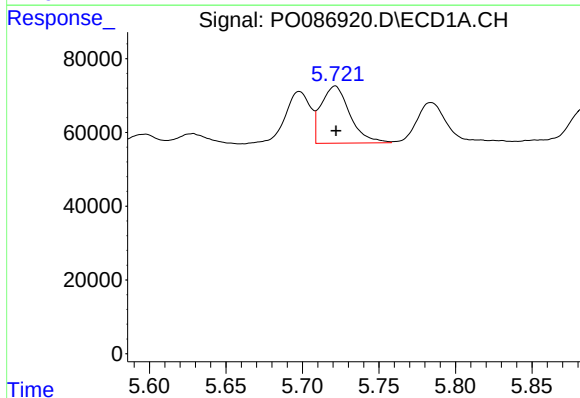


#17 AR-1242-2

R.T.: 5.722 min
Delta R.T.: 0.000 min
Response: 202655
Conc: 88.95 ng/ml

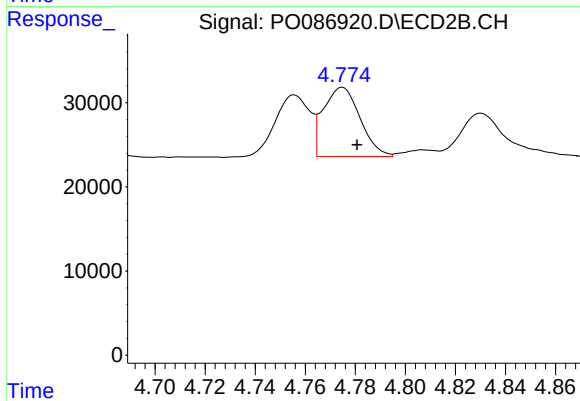

#17 AR-1242-2

R.T.: 4.775 min
Delta R.T.: -0.006 min
Response: 83788
Conc: 77.52 ng/ml

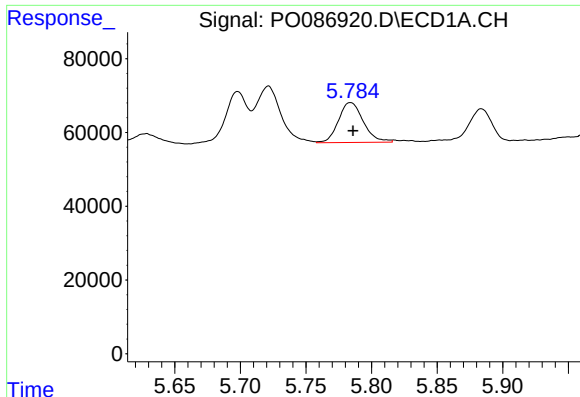


#18 AR-1242-3

R.T.: 5.784 min
Delta R.T.: -0.002 min
Response: 143843
Conc: 101.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
TB-TRANS-0531


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

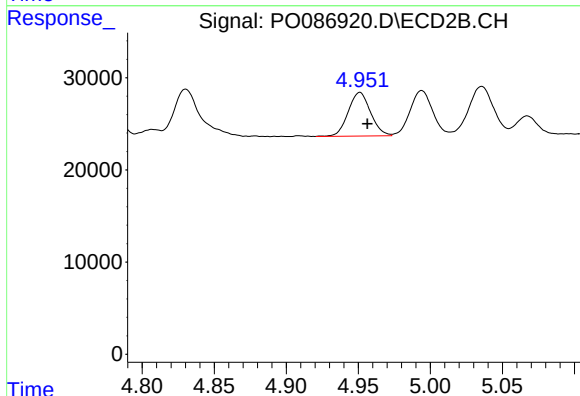


#18 AR-1242-3

R.T.: 4.951 min
Delta R.T.: -0.005 min
Response: 51274
Conc: 86.85 ng/ml

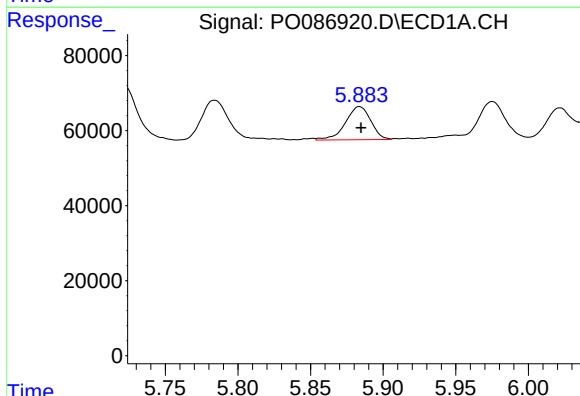


#19 AR-1242-4

R.T.: 5.884 min
Delta R.T.: -0.001 min
Response: 107806
Conc: 95.12 ng/ml

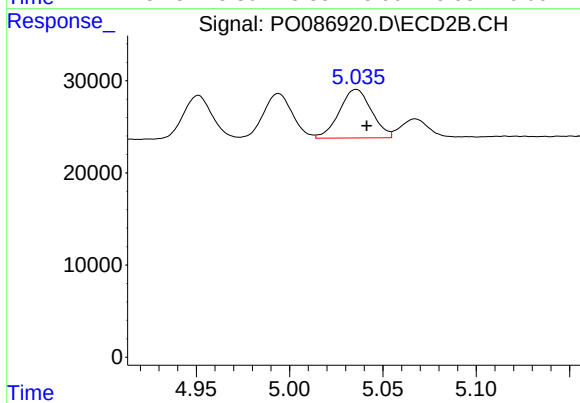

#19 AR-1242-4

R.T.: 5.036 min
Delta R.T.: -0.006 min
Response: 63471
Conc: 110.92 ng/ml

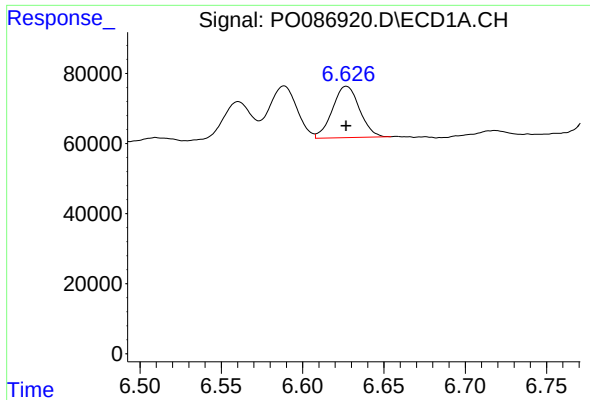


#20 AR-1242-5

R.T.: 6.627 min
Delta R.T.: 0.000 min
Response: 170420
Conc: 144.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
TB-TRANS-0531

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

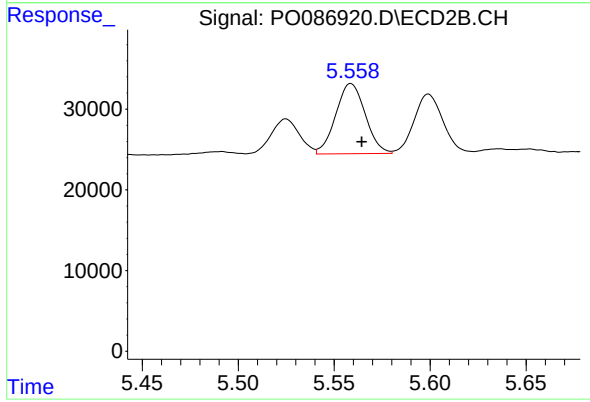

#20 AR-1242-5

R.T.: 5.559 min
Delta R.T.: -0.006 min
Response: 93260
Conc: 138.86 ng/ml