

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060622\
 Data File : P0086955.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jun 2022 23:51
 Operator : YP\AJ
 Sample : PB145349BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB145349BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:36:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.514	3.663	1377210	697344	24.081	21.816
2) SA Decachlor...	10.387	8.686	1226051	494912	26.860	22.072m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060622\
Data File : P0086955.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jun 2022 23:51
Operator : YP\AJ
Sample : PB145349BL
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB145349BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:36:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

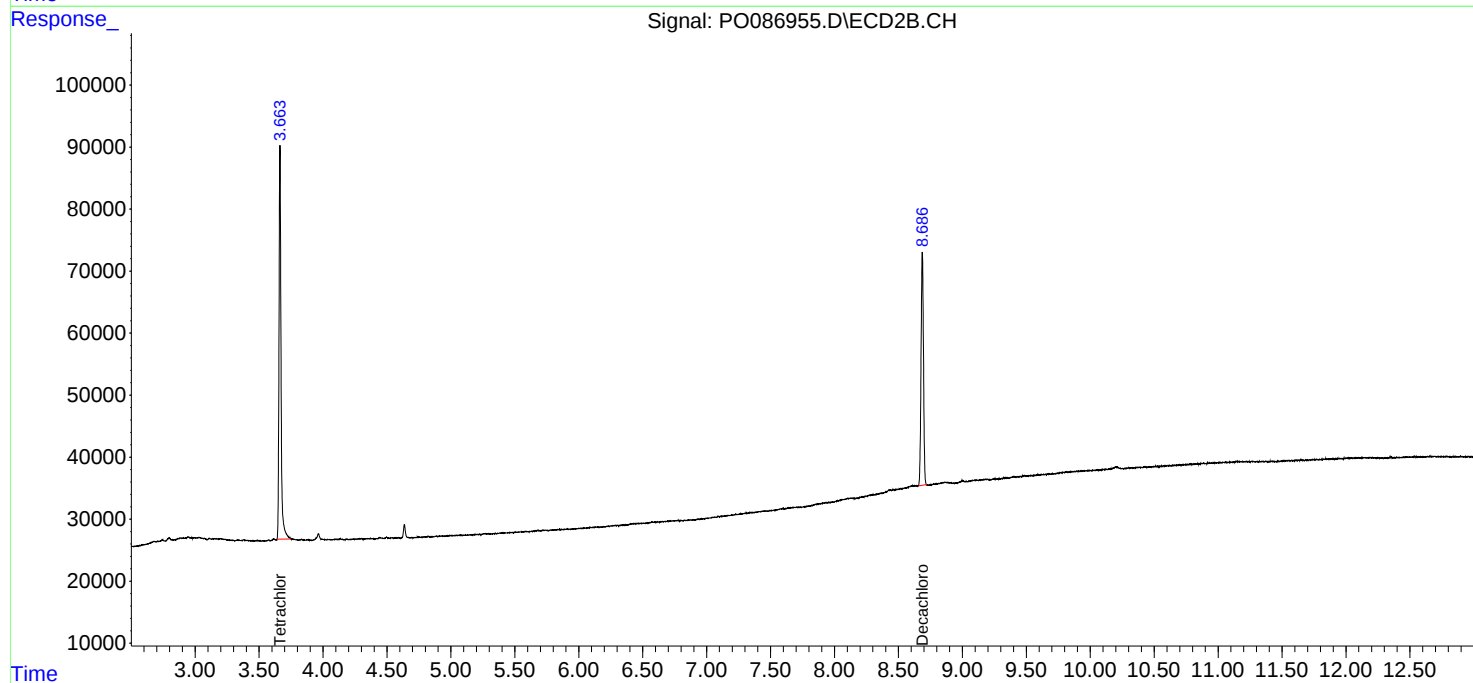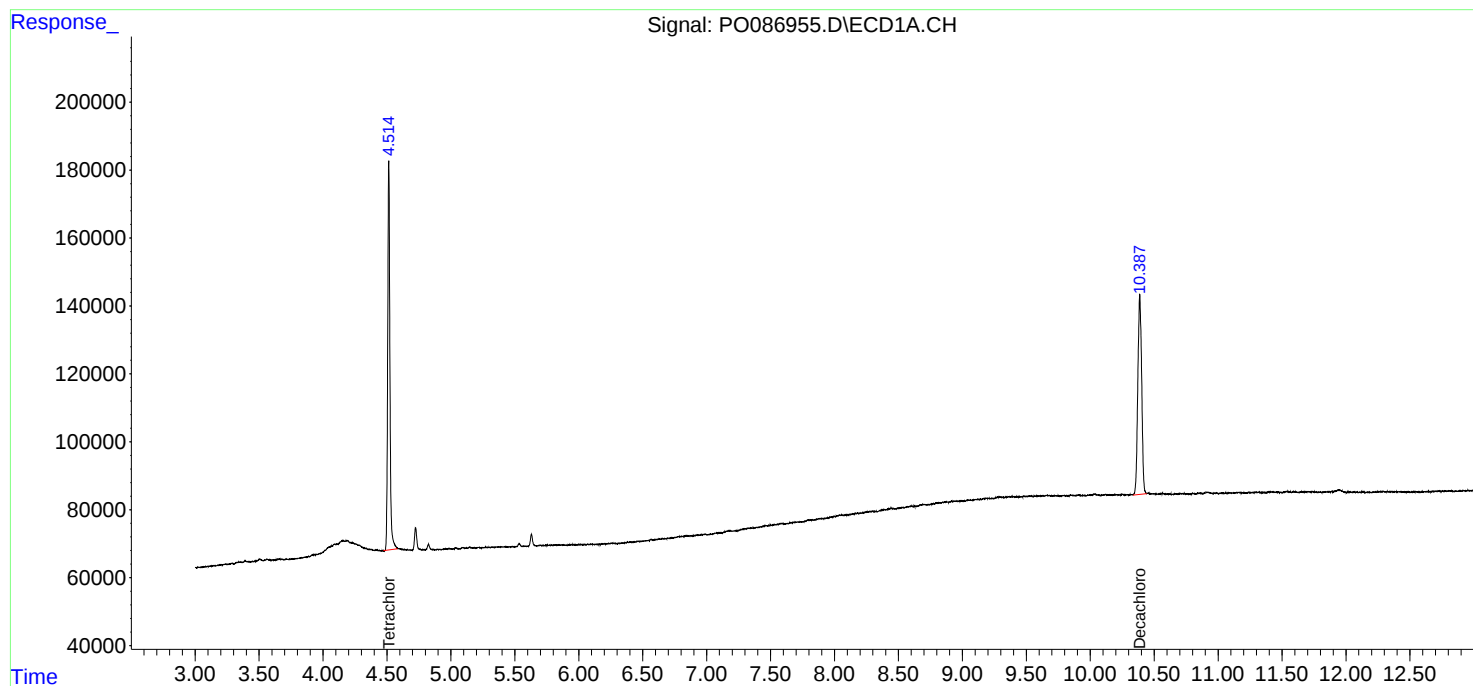

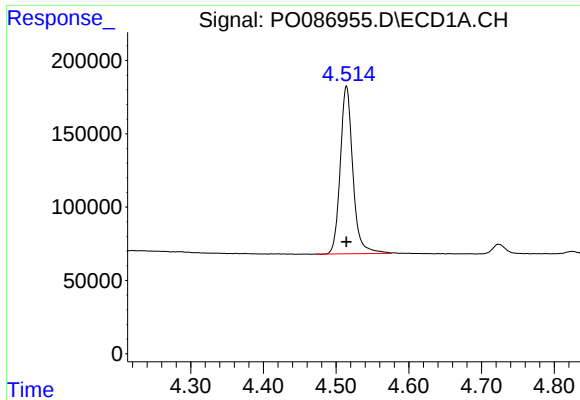


#1 Tetrachloro-m-xylene

R.T.: 4.514 min
Delta R.T.: 0.000 min
Response: 1377210
Conc: 24.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB145349BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

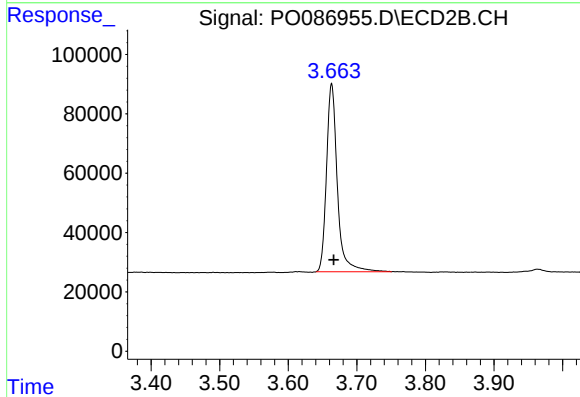


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: -0.003 min
Response: 697344
Conc: 21.82 ng/ml

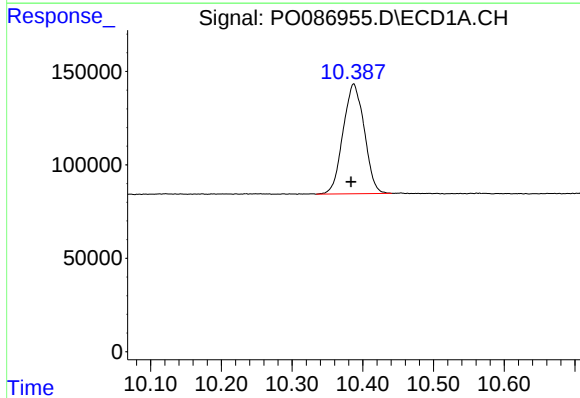

#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.004 min
Response: 1226051
Conc: 26.86 ng/ml

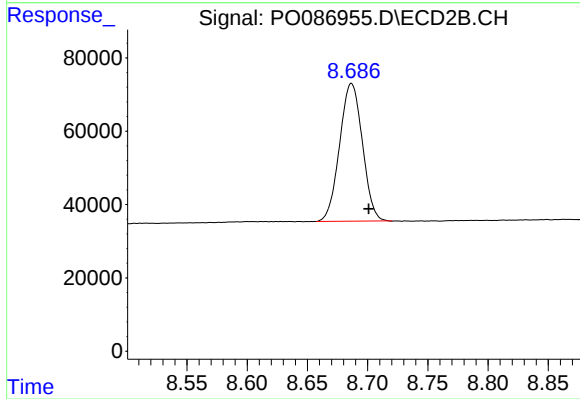

#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.015 min
Response: 494912
Conc: 22.07 ng/ml m