

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060622\
 Data File : P0086960.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2022 1:13
 Operator : YP\AJ
 Sample : N3178-03 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 2342

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 07 02:39:23 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.515	3.664	50384	26231	0.881m	0.821
2) SA Decachlor...	10.385	8.687	113598	18714	2.489	0.835 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060622\
Data File : P0086960.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2022 1:13
Operator : YP\AJ
Sample : N3178-03 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
2342


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 07 02:39:23 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

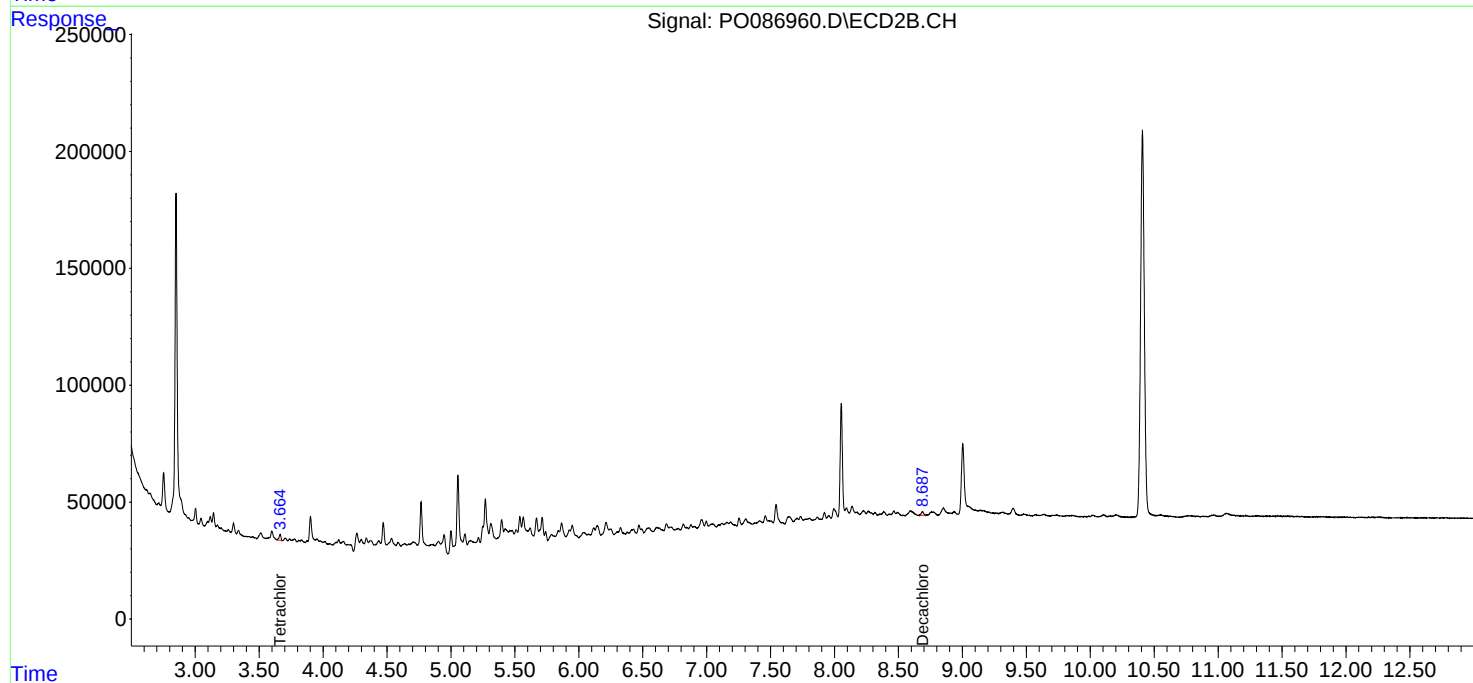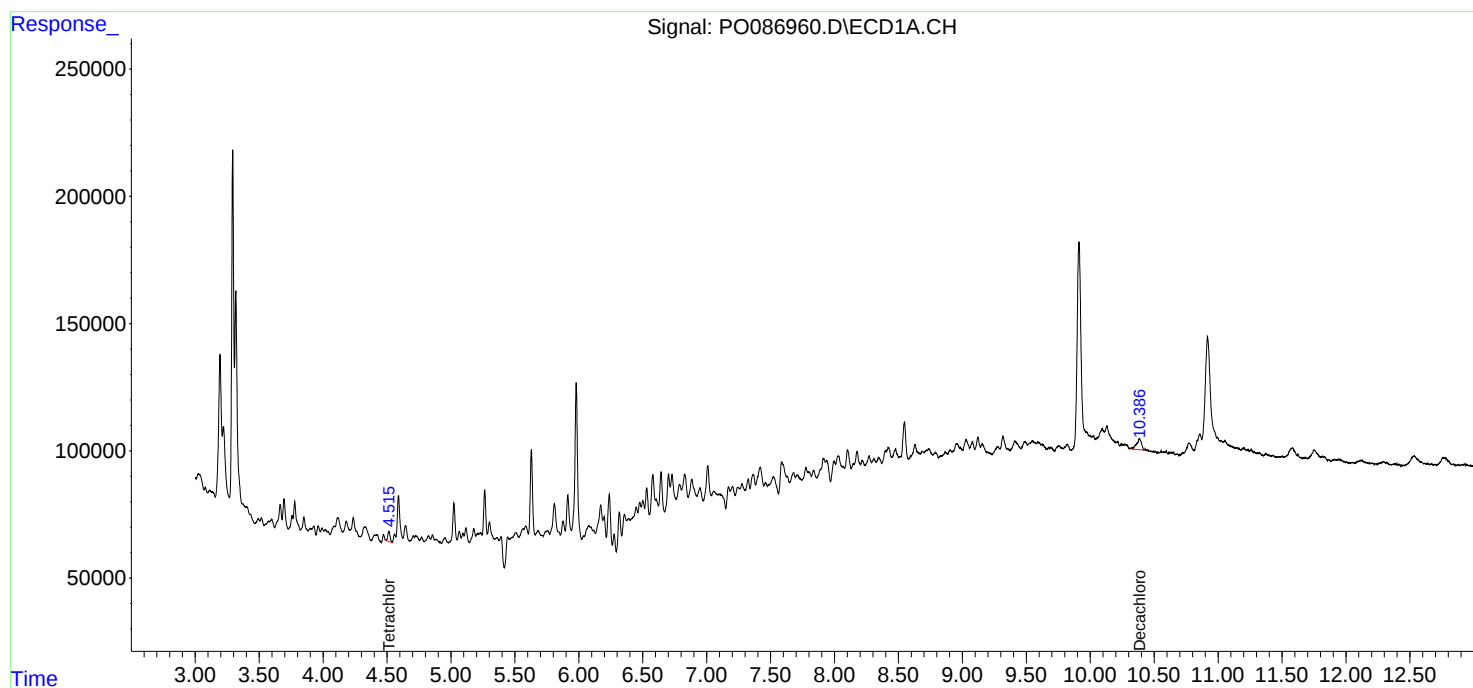

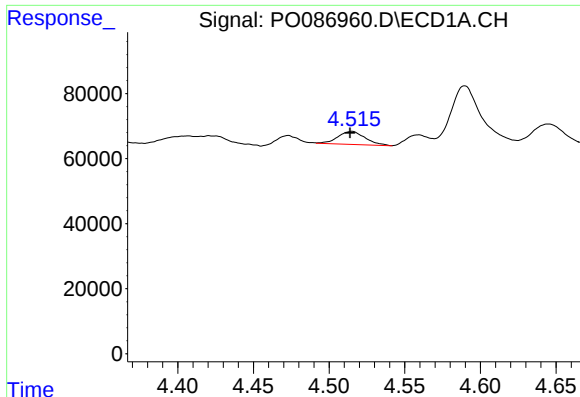


#1 Tetrachloro-m-xylene

R.T.: 4.515 min
Delta R.T.: 0.000 min
Response: 50384
Conc: 0.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
2342


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

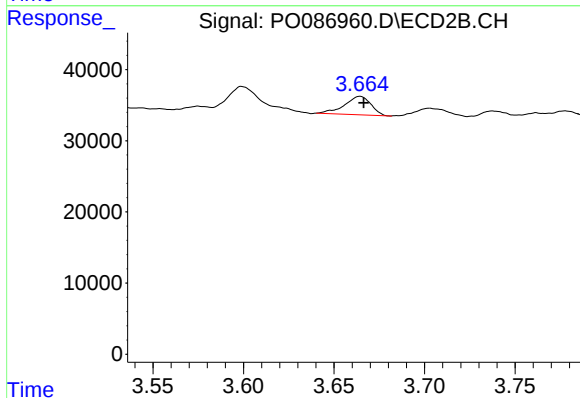


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: -0.002 min
Response: 26231
Conc: 0.82 ng/ml

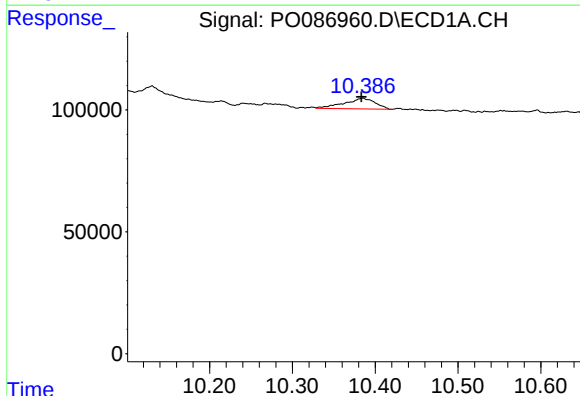

#2 Decachlorobiphenyl

R.T.: 10.385 min
Delta R.T.: 0.002 min
Response: 113598
Conc: 2.49 ng/ml

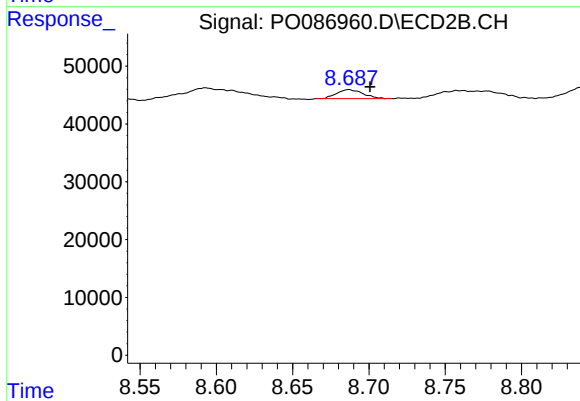

#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: -0.014 min
Response: 18714
Conc: 0.83 ng/ml