

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060623\
 Data File : P0095524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jun 2023 16:20
 Operator : YP/AJ
 Sample : 03043-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MR-PIPE-H

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2023
 Supervised By :Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 06 21:16:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 02 06:53:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.439	3.656	96206750	44393167	26.104	28.303
2)	SA Decachlor...	10.292	8.716	69282435	34142965	25.599	26.392
Target Compounds							
16)	L4 AR-1242-1	5.621	4.750	4135804	6698528	44.685m	150.157 #
17)	L4 AR-1242-2	5.644	4.769	6853942	3477929	53.775m	59.861
18)	L4 AR-1242-3	5.706	4.946	6765814	2585744	83.139m	82.114
19)	L4 AR-1242-4	5.812	5.032	14149808	6745113	219.505	199.962
20)	L4 AR-1242-5	6.551	5.559	25247028	10954095	365.704	255.481 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO060623\
Data File : PO095524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jun 2023 16:20
Operator : YP/AJ
Sample : 03043-08
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MR-PIPE-H


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 06 21:16:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO060123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 02 06:53:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

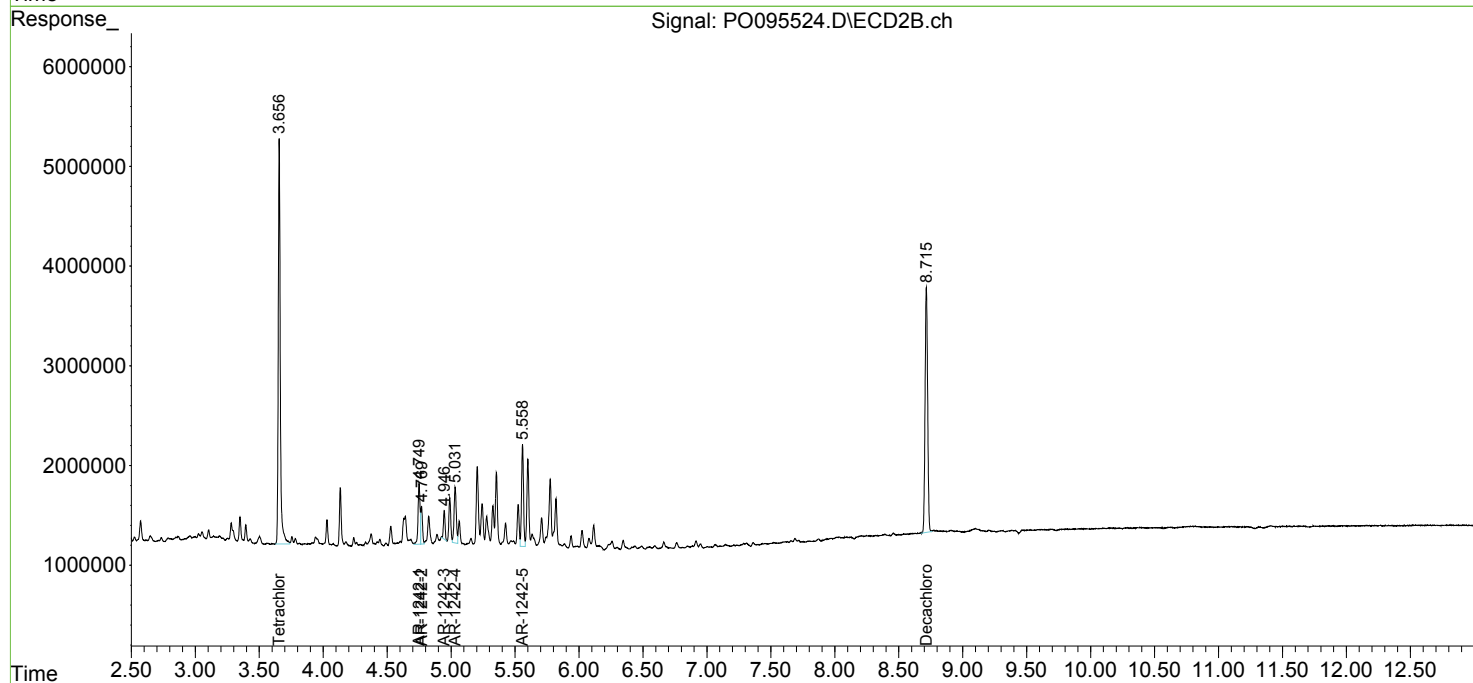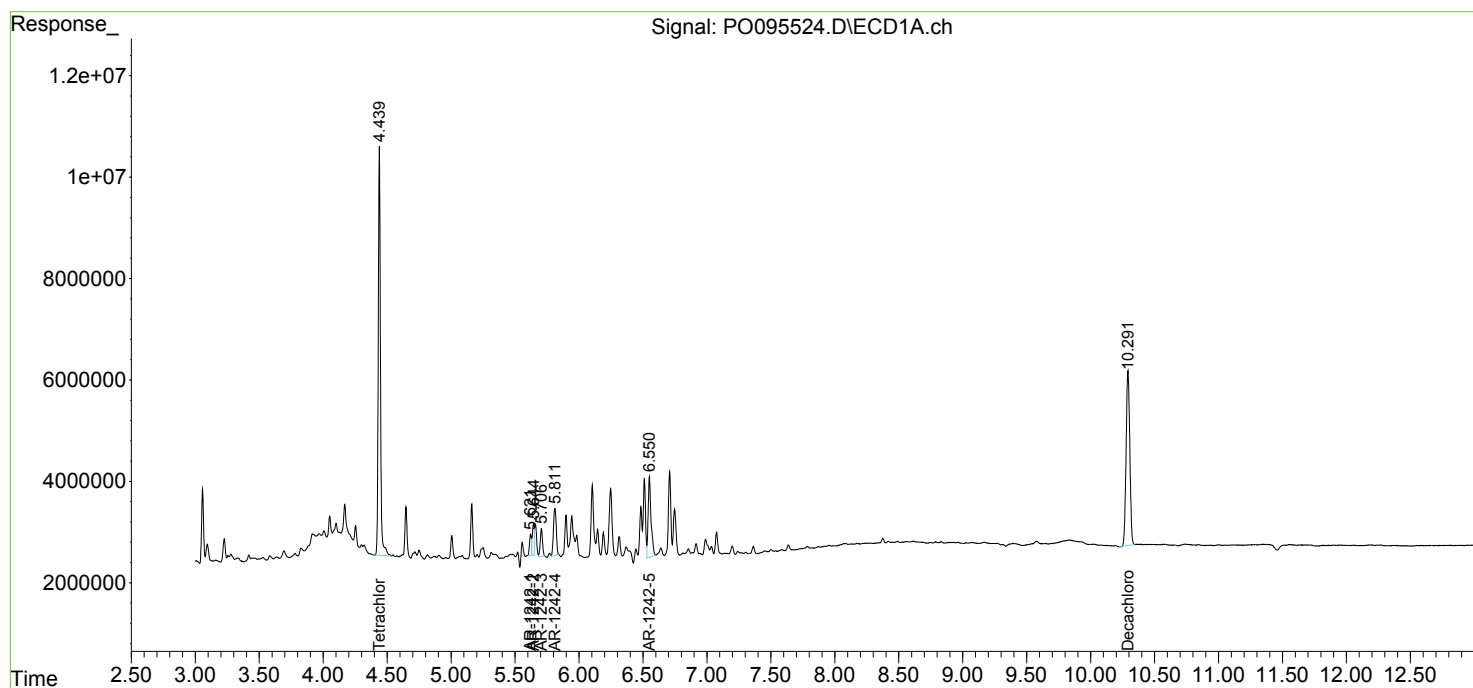

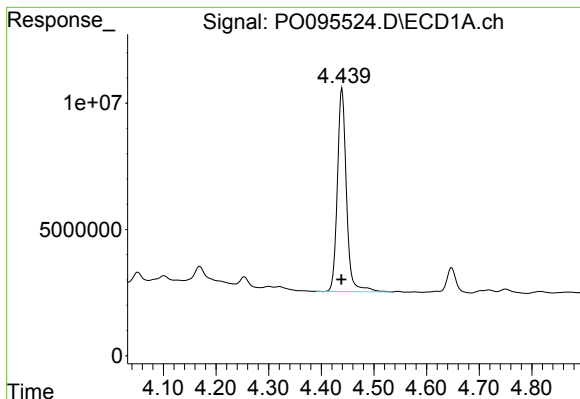


#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: 0.001 min
Response: 96206750
Conc: 26.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-PIPE-H


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

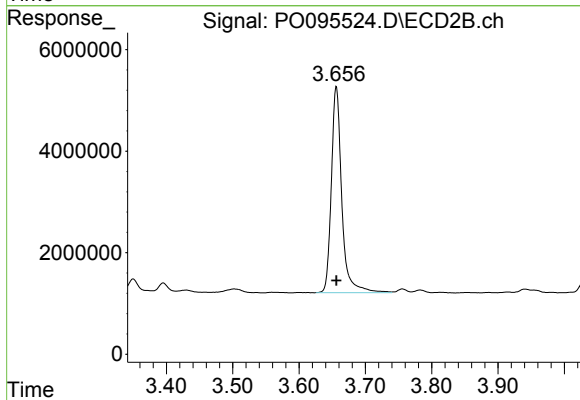


#1 Tetrachloro-m-xylene

R.T.: 3.656 min
Delta R.T.: 0.000 min
Response: 44393167
Conc: 28.30 ng/ml

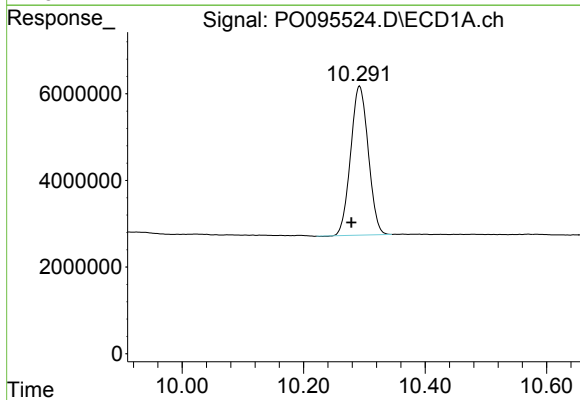


#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: 0.014 min
Response: 69282435
Conc: 25.60 ng/ml

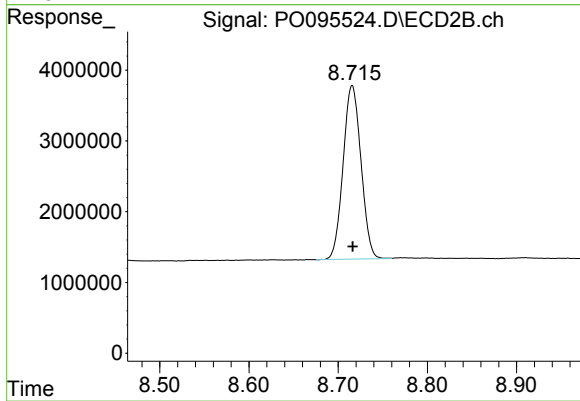

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: 0.000 min
Response: 34142965
Conc: 26.39 ng/ml

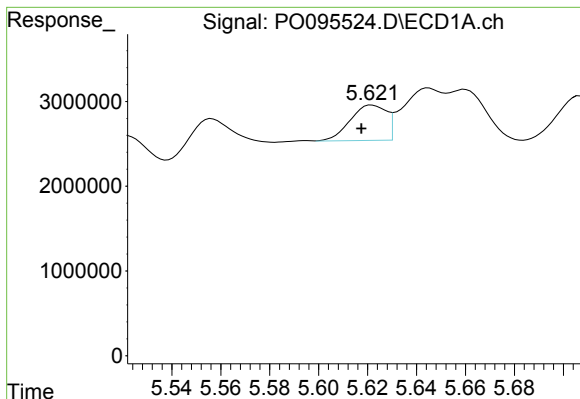


#16 AR-1242-1

R.T.: 5.621 min
Delta R.T.: 0.003 min
Response: 4135804
Conc: 44.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-PIPE-H


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

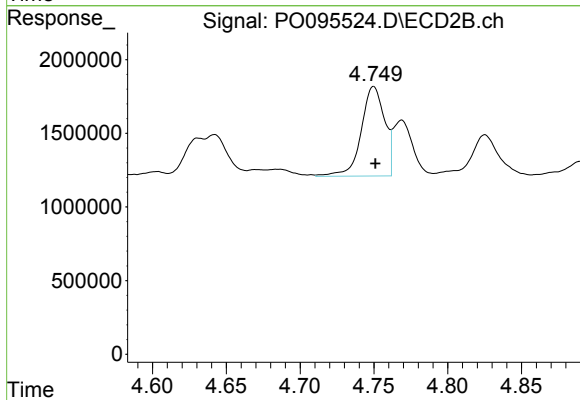


#16 AR-1242-1

R.T.: 4.750 min
Delta R.T.: -0.001 min
Response: 6698528
Conc: 150.16 ng/ml

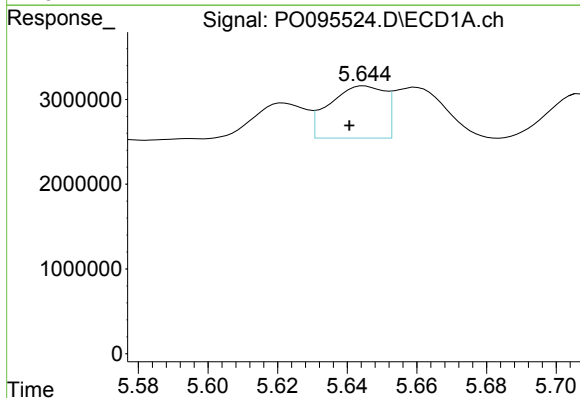


#17 AR-1242-2

R.T.: 5.644 min
Delta R.T.: 0.004 min
Response: 6853942
Conc: 53.78 ng/ml m

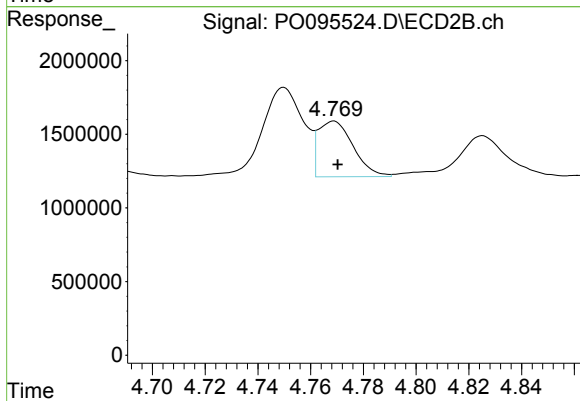

#17 AR-1242-2

R.T.: 4.769 min
Delta R.T.: -0.002 min
Response: 3477929
Conc: 59.86 ng/ml

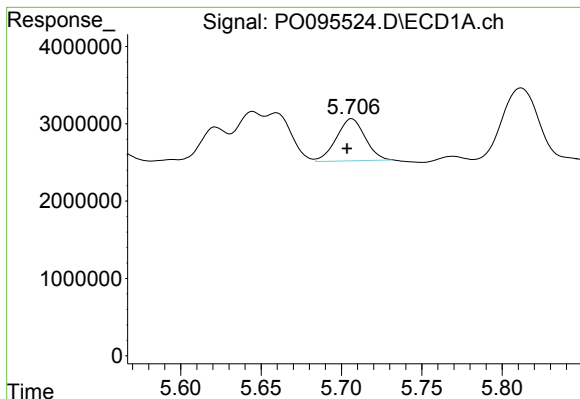


#18 AR-1242-3

R.T.: 5.706 min
Delta R.T.: 0.002 min
Response: 6765814
Conc: 83.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-PIPE-H


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

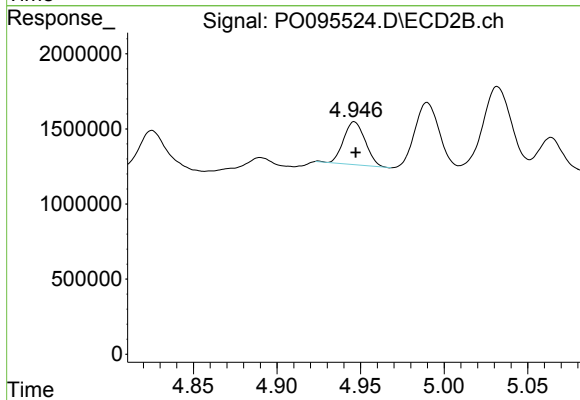


#18 AR-1242-3

R.T.: 4.946 min
Delta R.T.: 0.000 min
Response: 2585744
Conc: 82.11 ng/ml

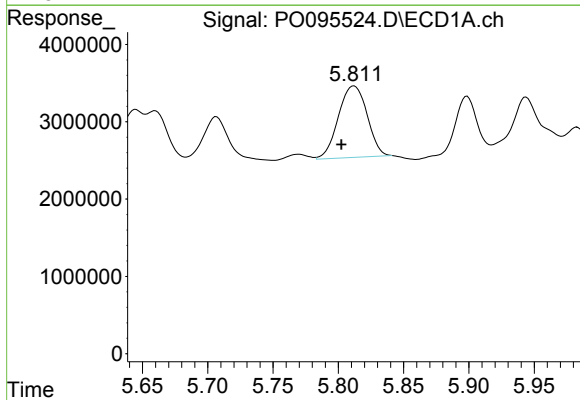


#19 AR-1242-4

R.T.: 5.812 min
Delta R.T.: 0.010 min
Response: 14149808
Conc: 219.51 ng/ml

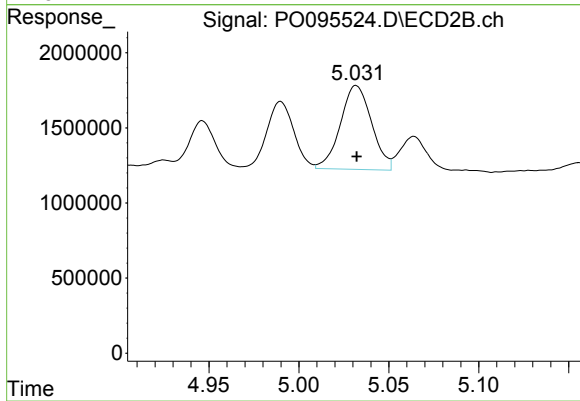

#19 AR-1242-4

R.T.: 5.032 min
Delta R.T.: 0.000 min
Response: 6745113
Conc: 199.96 ng/ml

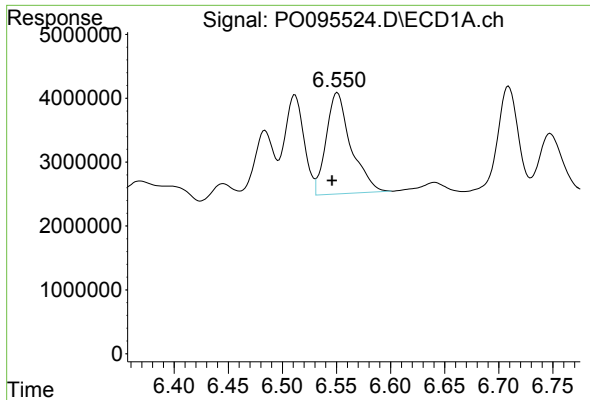


#20 AR-1242-5

R.T.: 6.551 min
Delta R.T.: 0.005 min
Response: 25247028
Conc: 365.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-PIPE-H

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2023
Supervised By :Ankita Jodhani 06/07/2023

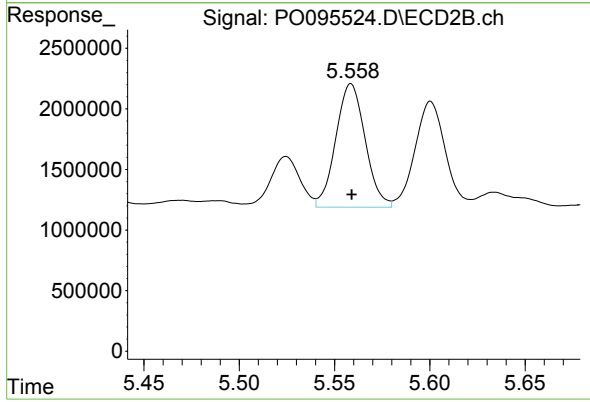

#20 AR-1242-5

R.T.: 5.559 min
Delta R.T.: 0.000 min
Response: 10954095
Conc: 255.48 ng/ml