

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060721\
 Data File : P0078517.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2021 18:40
 Operator : DD\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1242ICC050

Manual Integrations
 APPROVED

Ankita
 6/8/2021 1:16:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 03:40:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 03:38:40 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.613	356549	165982	4.655	4.990
2) SA Decachlor...	9.945	8.799	227712	150052	5.538	5.809
Target Compounds						
16) L4 AR-1242-1	5.633	4.842	93824	46327	51.842m	55.143
17) L4 AR-1242-2	5.655	4.861	133168	66420	49.015	54.042
18) L4 AR-1242-3	5.720	5.048	80755	33321	48.649	51.791
19) L4 AR-1242-4	5.825	5.144	72529	34805	54.755	52.454
20) L4 AR-1242-5	6.595	5.699	68225	42036	50.490	49.982

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060721\
Data File : P0078517.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2021 18:40
Operator : DD\AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Ankita
6/8/2021 1:16:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 03:40:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 03:38:40 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

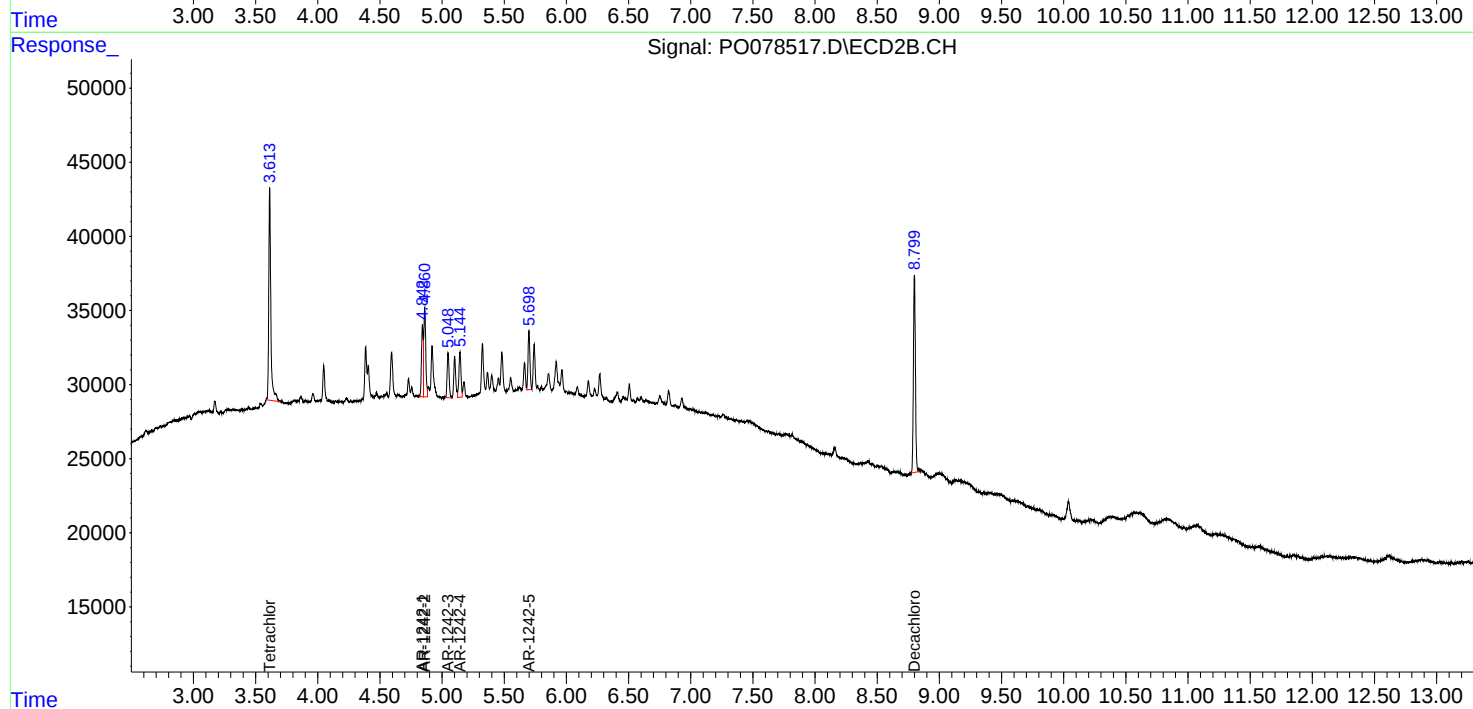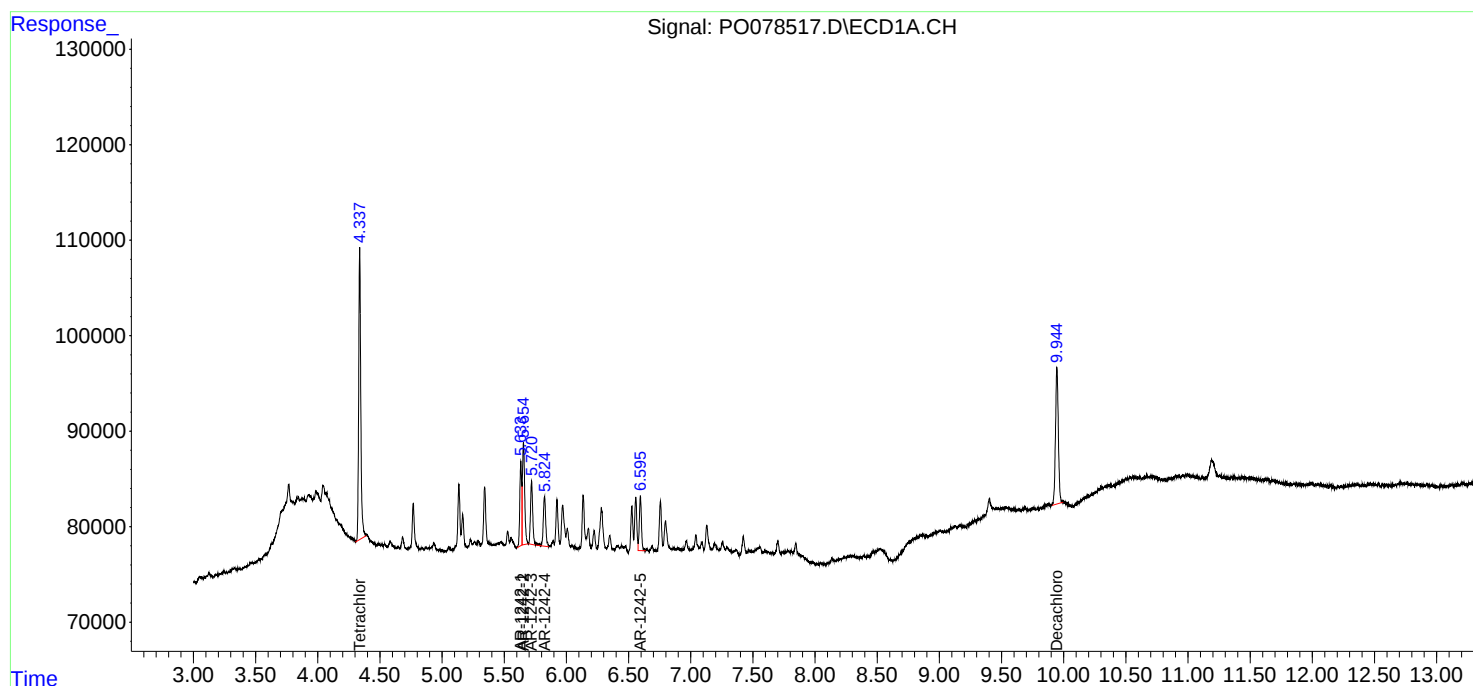

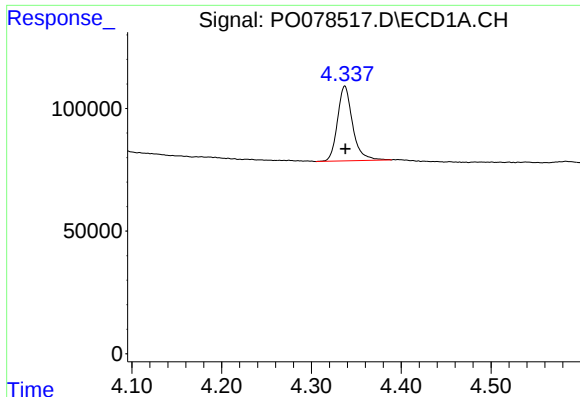


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: 0.000 min
Response: 356549
Conc: 4.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242IC050


Manual Integrations
APPROVED

Ankita
6/8/2021 1:16:26 PM

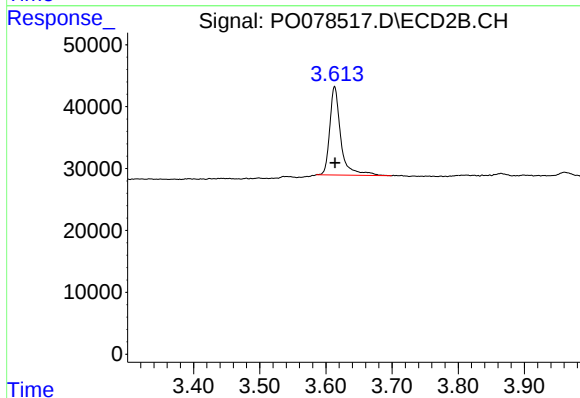


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: 0.000 min
Response: 165982
Conc: 4.99 ng/ml

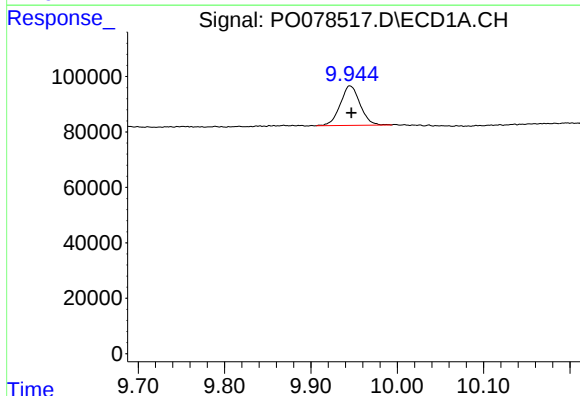


#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: -0.002 min
Response: 227712
Conc: 5.54 ng/ml

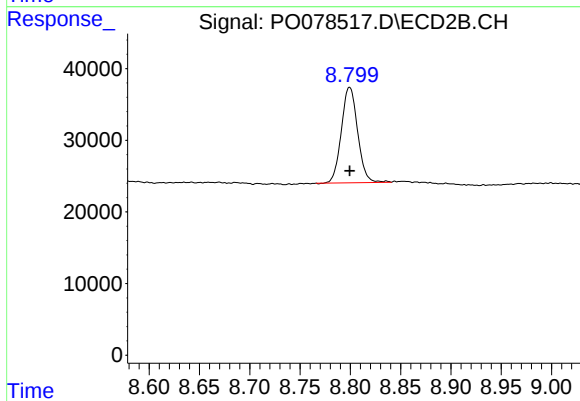

#2 Decachlorobiphenyl

R.T.: 8.799 min
Delta R.T.: 0.000 min
Response: 150052
Conc: 5.81 ng/ml

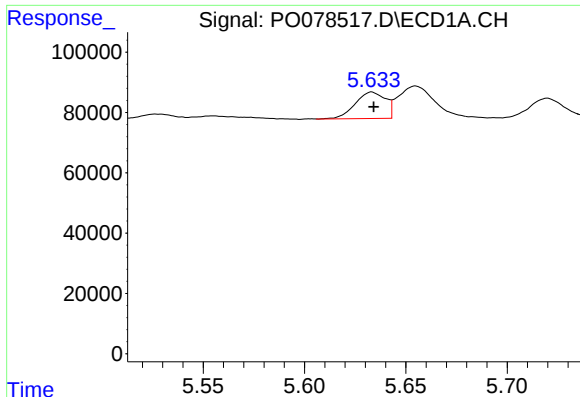


#16 AR-1242-1

R.T.: 5.633 min
Delta R.T.: -0.001 min
Response: 93824
Conc: 51.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Ankita
6/8/2021 1:16:26 PM

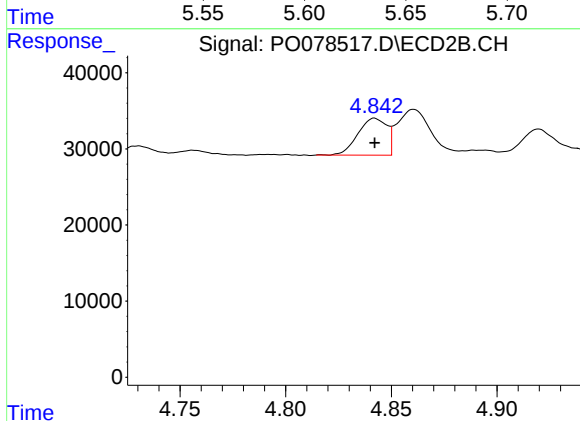


#16 AR-1242-1

R.T.: 4.842 min
Delta R.T.: 0.000 min
Response: 46327
Conc: 55.14 ng/ml

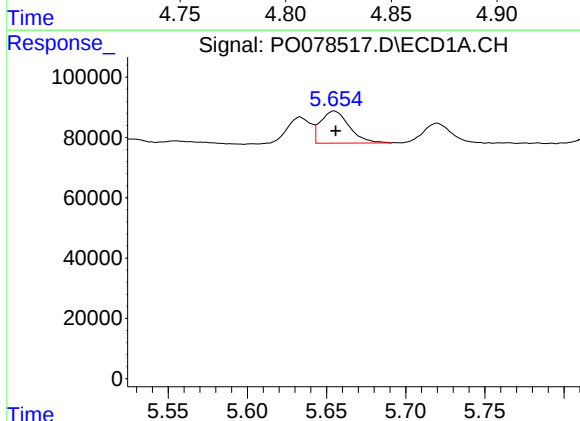


#17 AR-1242-2

R.T.: 5.655 min
Delta R.T.: 0.000 min
Response: 133168
Conc: 49.02 ng/ml

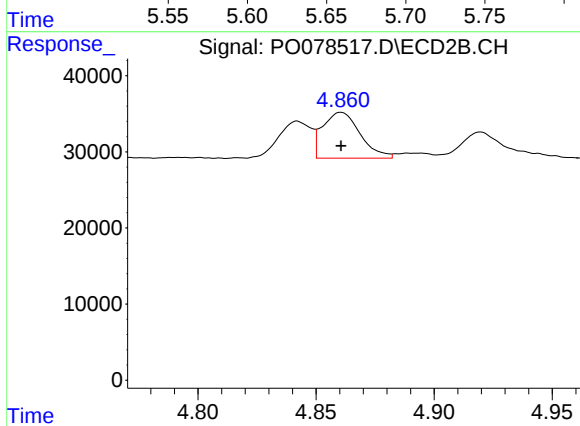

#17 AR-1242-2

R.T.: 4.861 min
Delta R.T.: 0.000 min
Response: 66420
Conc: 54.04 ng/ml

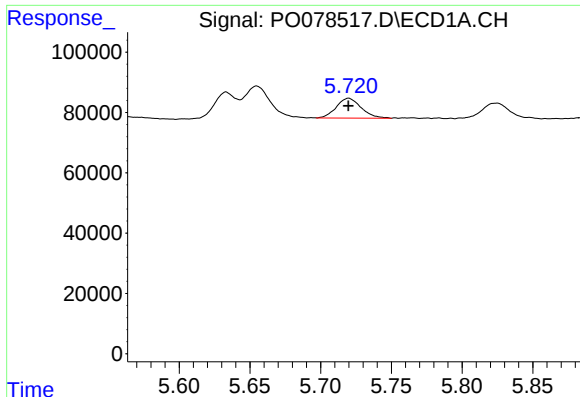


#18 AR-1242-3

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 80755
Conc: 48.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Ankita
6/8/2021 1:16:26 PM

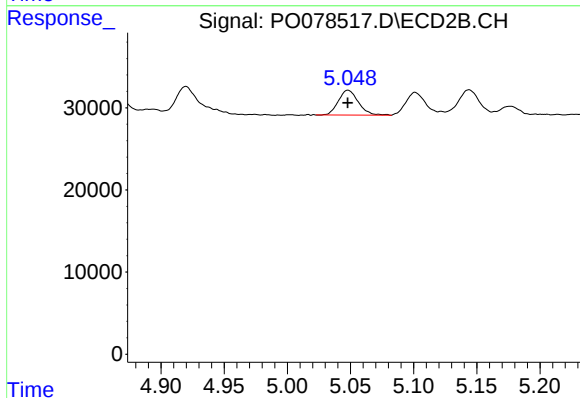


#18 AR-1242-3

R.T.: 5.048 min
Delta R.T.: 0.000 min
Response: 33321
Conc: 51.79 ng/ml

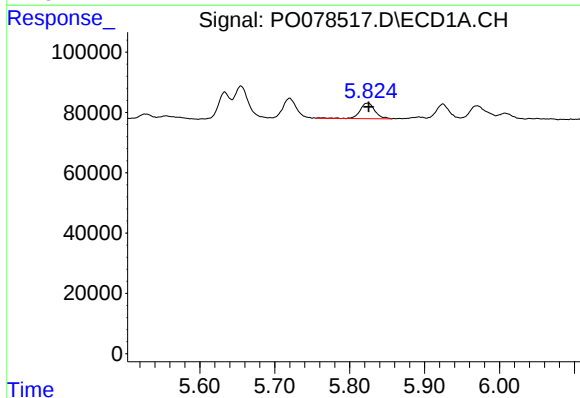


#19 AR-1242-4

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 72529
Conc: 54.76 ng/ml

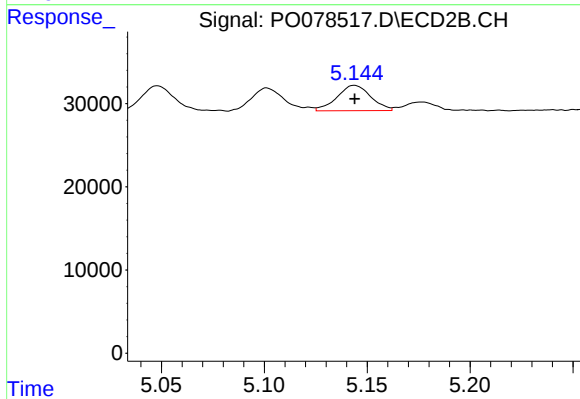

#19 AR-1242-4

R.T.: 5.144 min
Delta R.T.: 0.000 min
Response: 34805
Conc: 52.45 ng/ml

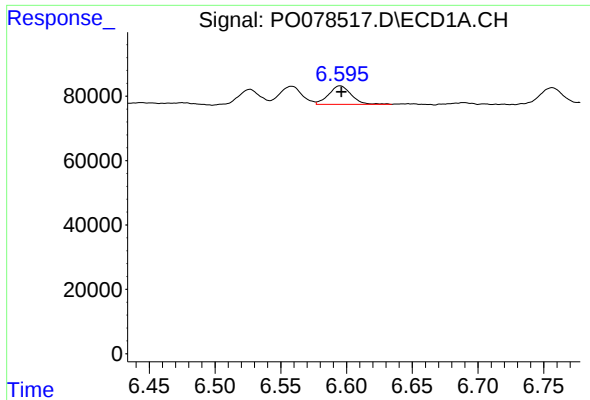


#20 AR-1242-5

R.T.: 6.595 min
Delta R.T.: 0.000 min
Response: 68225
Conc: 50.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Ankita
6/8/2021 1:16:26 PM

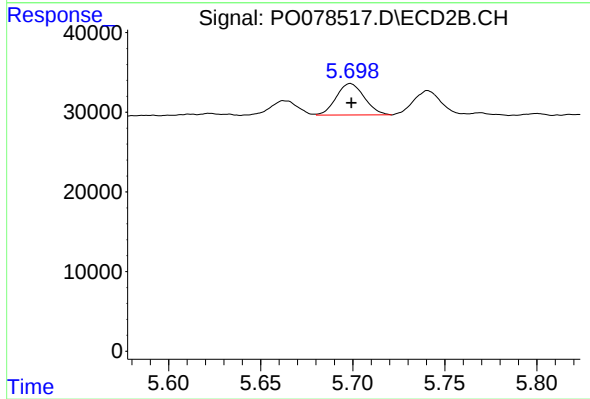

#20 AR-1242-5

R.T.: 5.699 min
Delta R.T.: 0.000 min
Response: 42036
Conc: 49.98 ng/ml