

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060721\
 Data File : P0078546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jun 2021 10:23
 Operator : DD\AJ
 Sample : AR1262ICV500
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPO060721AR1262

Manual Integrations
 APPROVED

Ankita
 6/10/2021 12:55:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 09 02:35:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.613	3614279	1500774	47.319	47.504
2) SA Decachlor...	9.948	8.798	2092203	1352042	51.599	56.229
Target Compounds						
36) L8 AR-1262-1	7.921	6.927	1802932	548365	460.900	459.029
37) L8 AR-1262-2	8.460	7.475	2937727	1783757	459.183	454.829
38) L8 AR-1262-3	8.732	7.756	1993088	759144	477.214	461.175
39) L8 AR-1262-4	8.809	7.819	1489188	1400936	480.548m	465.729
40) L8 AR-1262-5	9.356	8.314	923329	641497	487.293	472.684

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060721\
Data File : P0078546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jun 2021 10:23
Operator : DD\AJ
Sample : AR1262ICV500
Misc :
ALS Vial : 49 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ICVPO060721AR1262


Manual Integrations
APPROVED

Ankita
6/10/2021 12:55:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 09 02:35:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

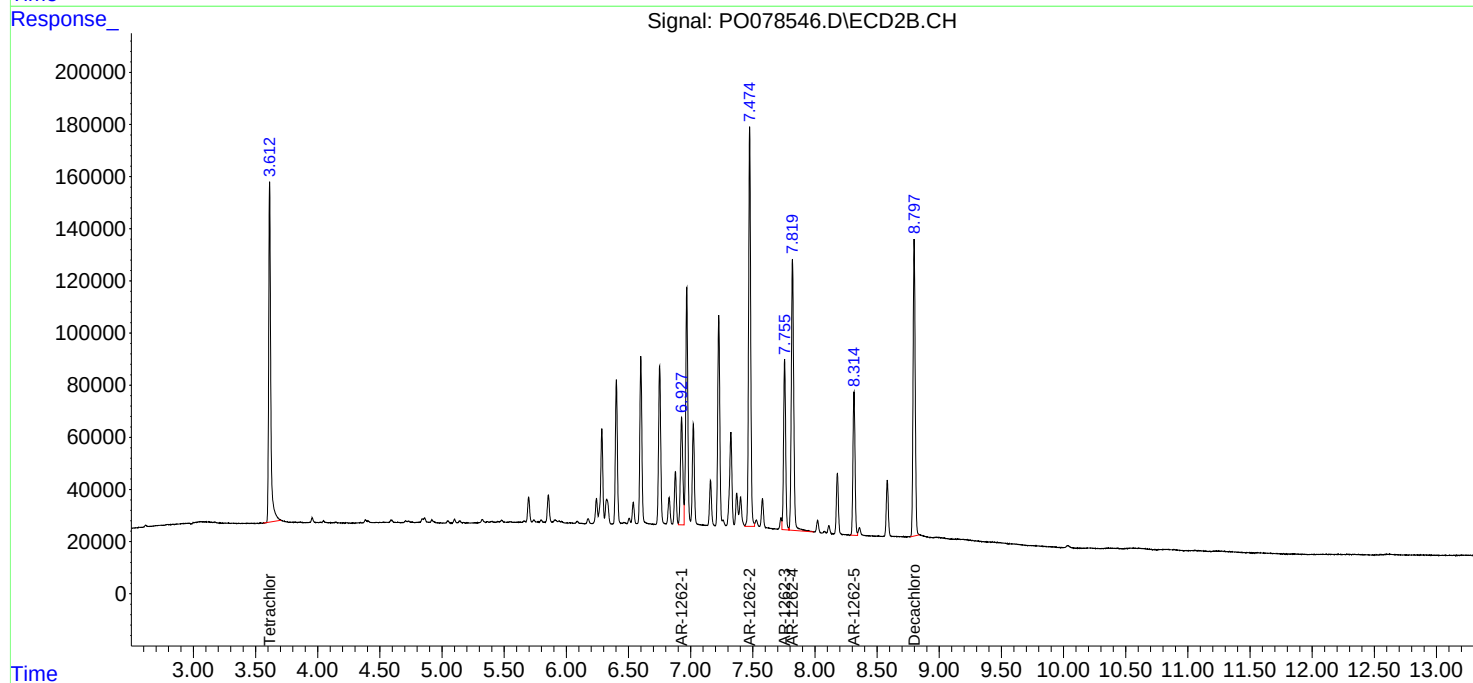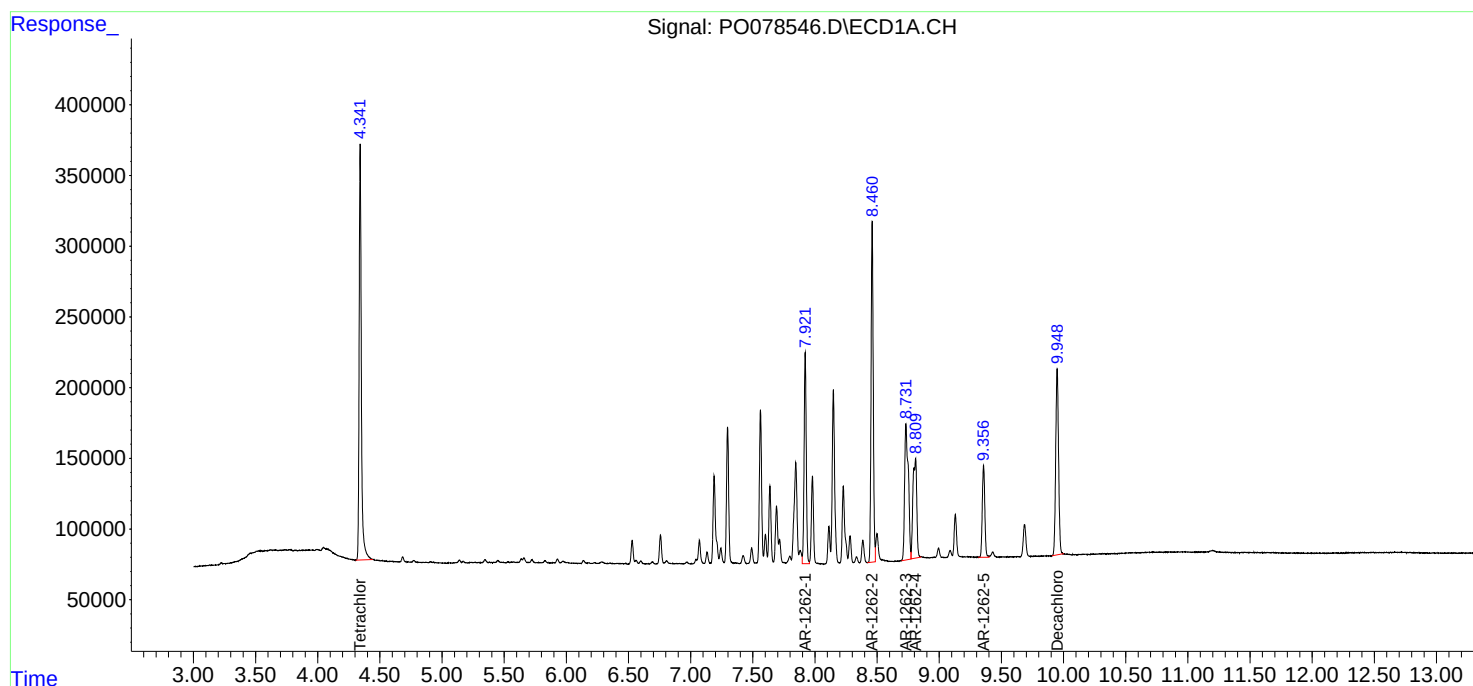

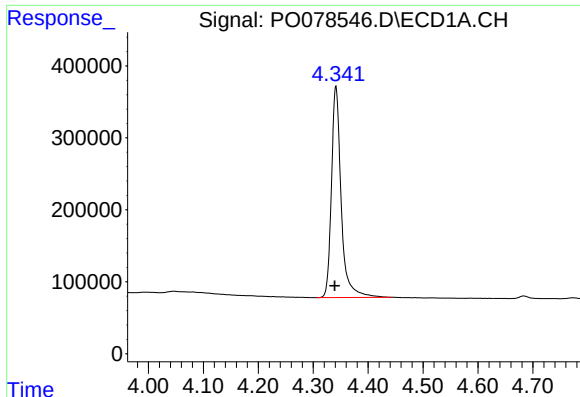


#1 Tetrachloro-m-xylene

R.T.: 4.341 min
Delta R.T.: 0.002 min
Response: 3614279
Conc: 47.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO060721AR1262


Manual Integrations
APPROVED

Ankita
6/10/2021 12:55:55 PM

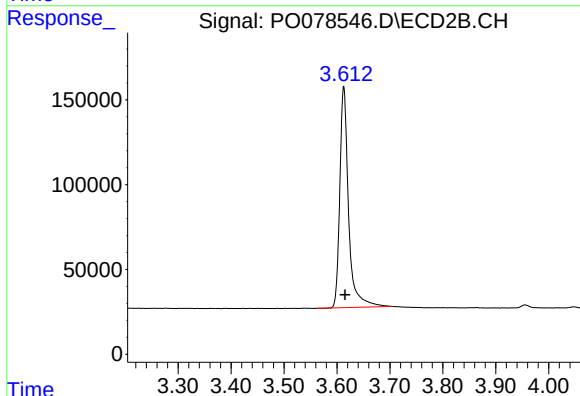


#1 Tetrachloro-m-xylene

R.T.: 3.613 min
Delta R.T.: -0.002 min
Response: 1500774
Conc: 47.50 ng/ml

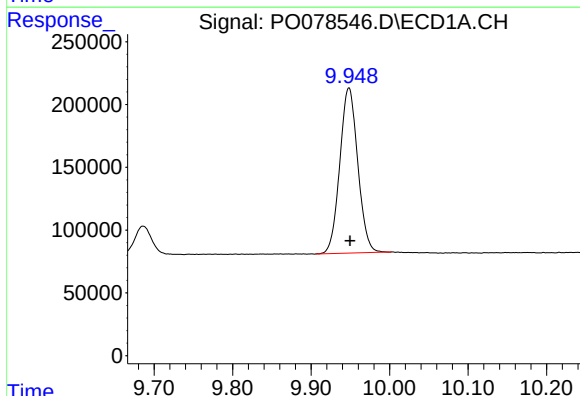


#2 Decachlorobiphenyl

R.T.: 9.948 min
Delta R.T.: -0.002 min
Response: 2092203
Conc: 51.60 ng/ml

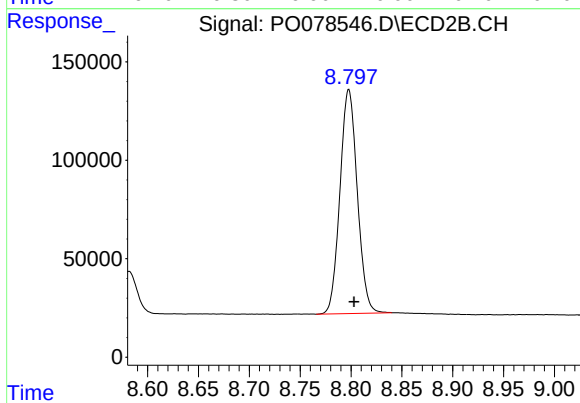

#2 Decachlorobiphenyl

R.T.: 8.798 min
Delta R.T.: -0.005 min
Response: 1352042
Conc: 56.23 ng/ml

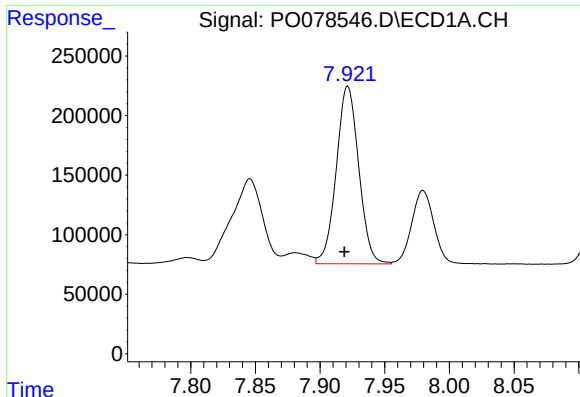


#36 AR-1262-1

R.T.: 7.921 min
Delta R.T.: 0.003 min
Response: 1802932
Conc: 460.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO060721AR1262


Manual Integrations
APPROVED

Ankita
6/10/2021 12:55:55 PM

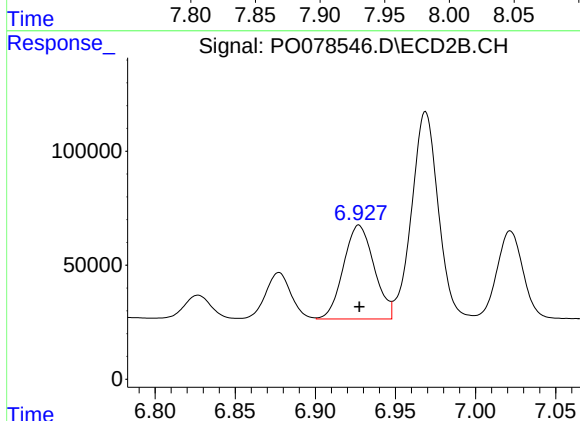


#36 AR-1262-1

R.T.: 6.927 min
Delta R.T.: 0.000 min
Response: 548365
Conc: 459.03 ng/ml

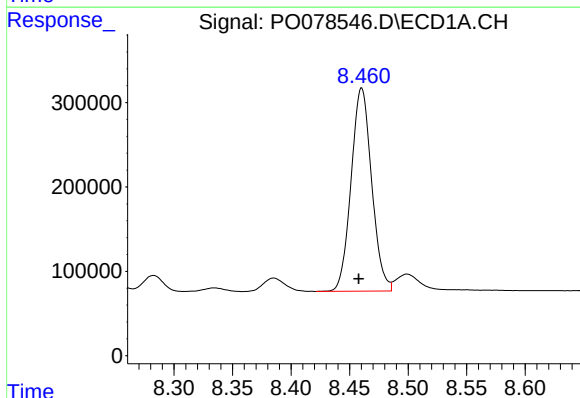


#37 AR-1262-2

R.T.: 8.460 min
Delta R.T.: 0.003 min
Response: 2937727
Conc: 459.18 ng/ml

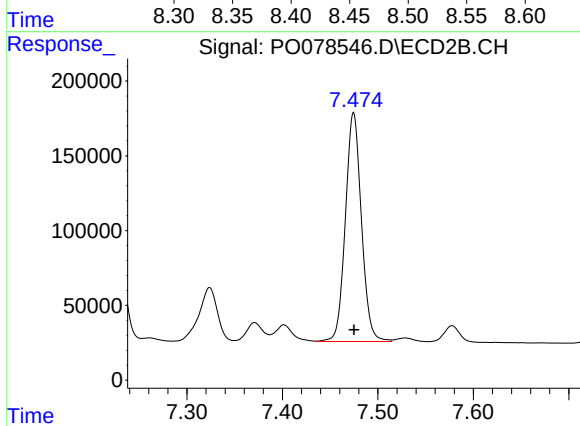

#37 AR-1262-2

R.T.: 7.475 min
Delta R.T.: 0.000 min
Response: 1783757
Conc: 454.83 ng/ml

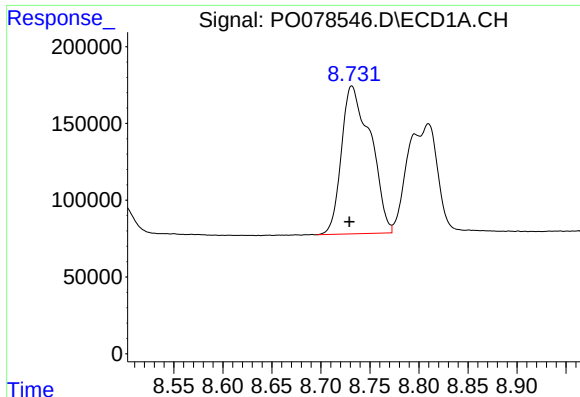


#38 AR-1262-3

R.T.: 8.732 min
Delta R.T.: 0.002 min
Response: 1993088
Conc: 477.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO060721AR1262


Manual Integrations
APPROVED

Ankita
6/10/2021 12:55:55 PM

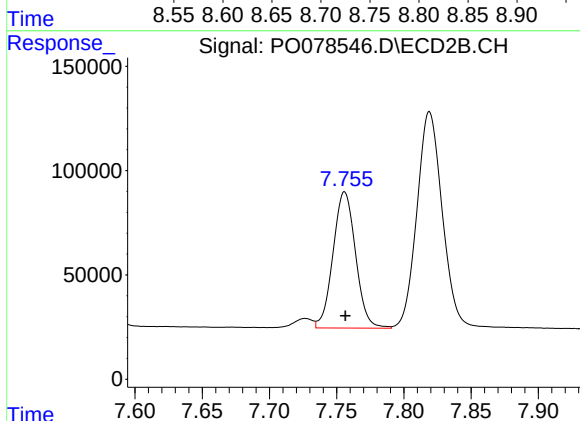


#38 AR-1262-3

R.T.: 7.756 min
Delta R.T.: 0.000 min
Response: 759144
Conc: 461.17 ng/ml

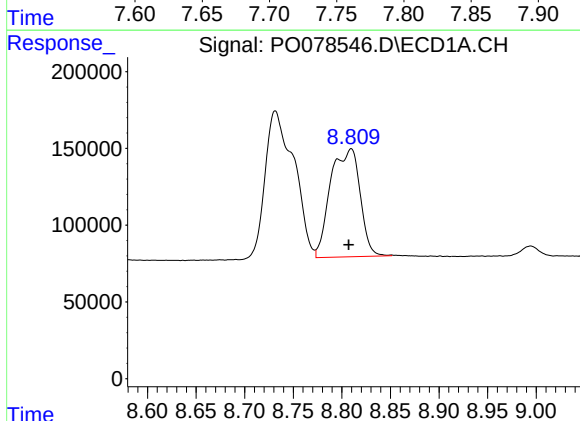


#39 AR-1262-4

R.T.: 8.809 min
Delta R.T.: 0.002 min
Response: 1489188
Conc: 480.55 ng/ml m

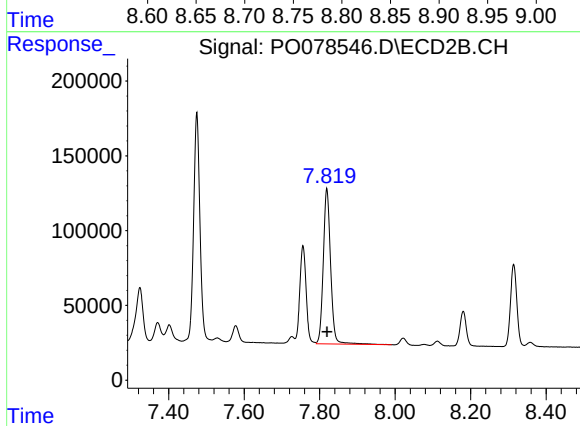

#39 AR-1262-4

R.T.: 7.819 min
Delta R.T.: 0.000 min
Response: 1400936
Conc: 465.73 ng/ml

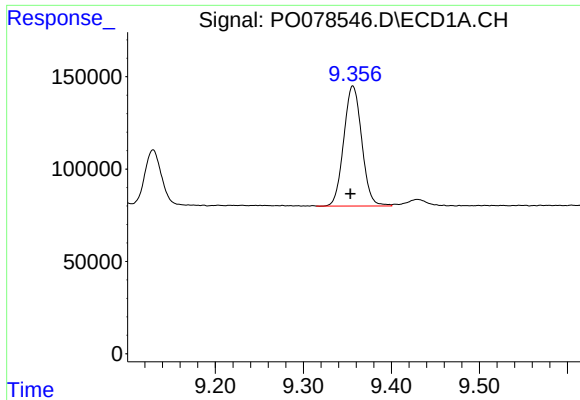


#40 AR-1262-5

R.T.: 9.356 min
Delta R.T.: 0.003 min
Response: 923329
Conc: 487.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPO060721AR1262

Manual Integrations
APPROVED

Ankita
6/10/2021 12:55:55 PM

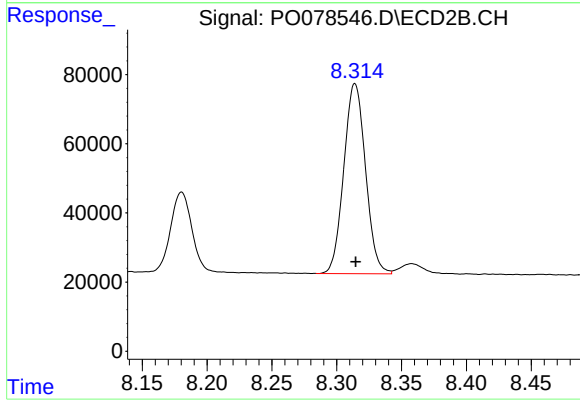

#40 AR-1262-5

R.T.: 8.314 min
Delta R.T.: 0.000 min
Response: 641497
Conc: 472.68 ng/ml