

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060722\
 Data File : P0086989.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2022 18:02
 Operator : YP\AJ
 Sample : N3143-05MS
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220425-SPLP-AMENDED-COMP-EMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:32:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.513	3.660	1803567	847246	31.536	26.506
2)	SA Decachlor...	10.387	8.683	1026740	438100	22.494	19.538
Target Compounds							
3)	L1 AR-1016-1	5.698	4.751	1525086	929717	768.053	941.857
4)	L1 AR-1016-2	5.721	4.772	2146967	827496	757.655	606.744
5)	L1 AR-1016-3	5.784	4.947	1361988	452398	779.053	613.702
6)	L1 AR-1016-4	5.883	4.991	1080771	348313	773.770	596.338
7)	L1 AR-1016-5	6.181	5.204	1014842	446092	738.577	612.668
31)	L7 AR-1260-1	7.317	6.239	1668879	802899	672.447	620.007
32)	L7 AR-1260-2	7.574	6.426	1974398	940637	582.386	608.990
33)	L7 AR-1260-3	7.937	6.579	1206877	928195	558.540	534.100
34)	L7 AR-1260-4	8.166	7.052	1472250	600734	572.937	527.796
35)	L7 AR-1260-5	8.495	7.293	2618446	1364558	551.032	513.801



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060722\
Data File : P0086989.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2022 18:02
Operator : YP\AJ
Sample : N3143-05MS
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:32:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

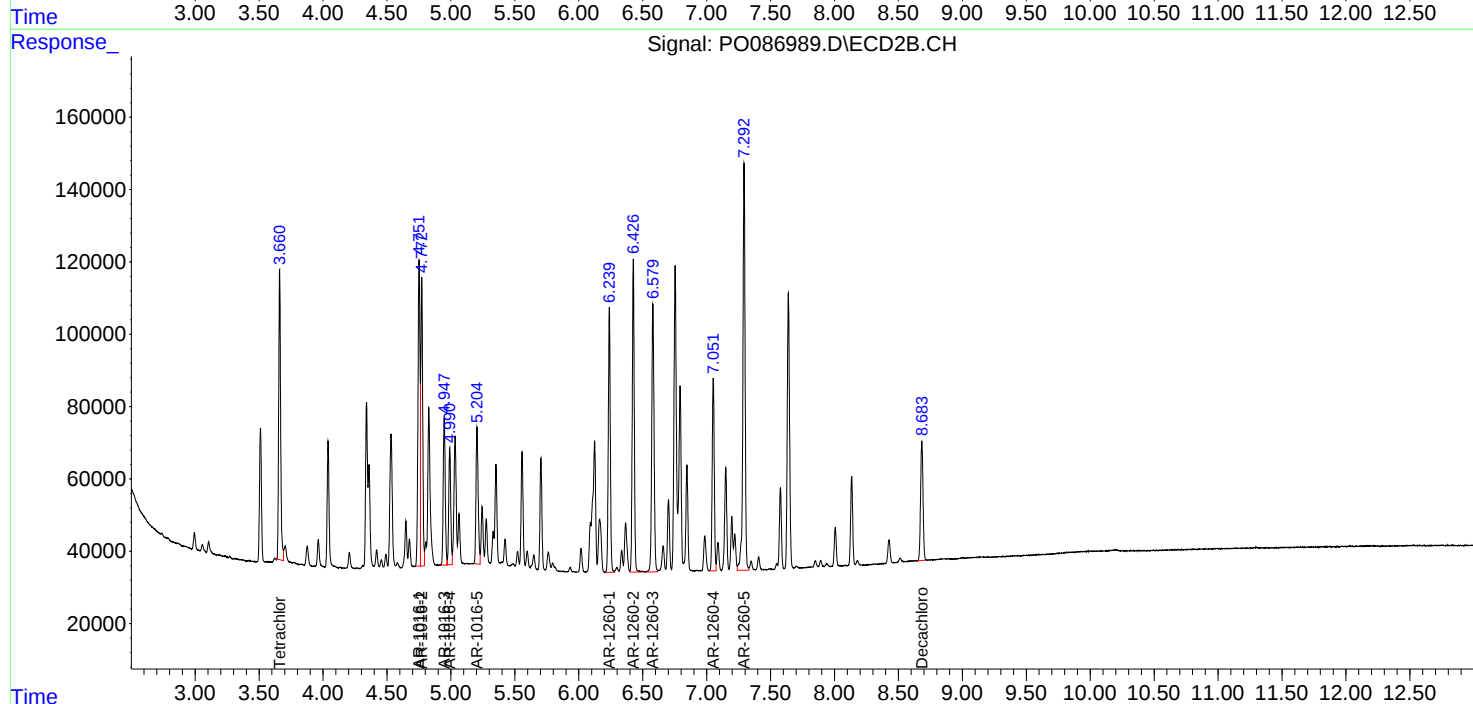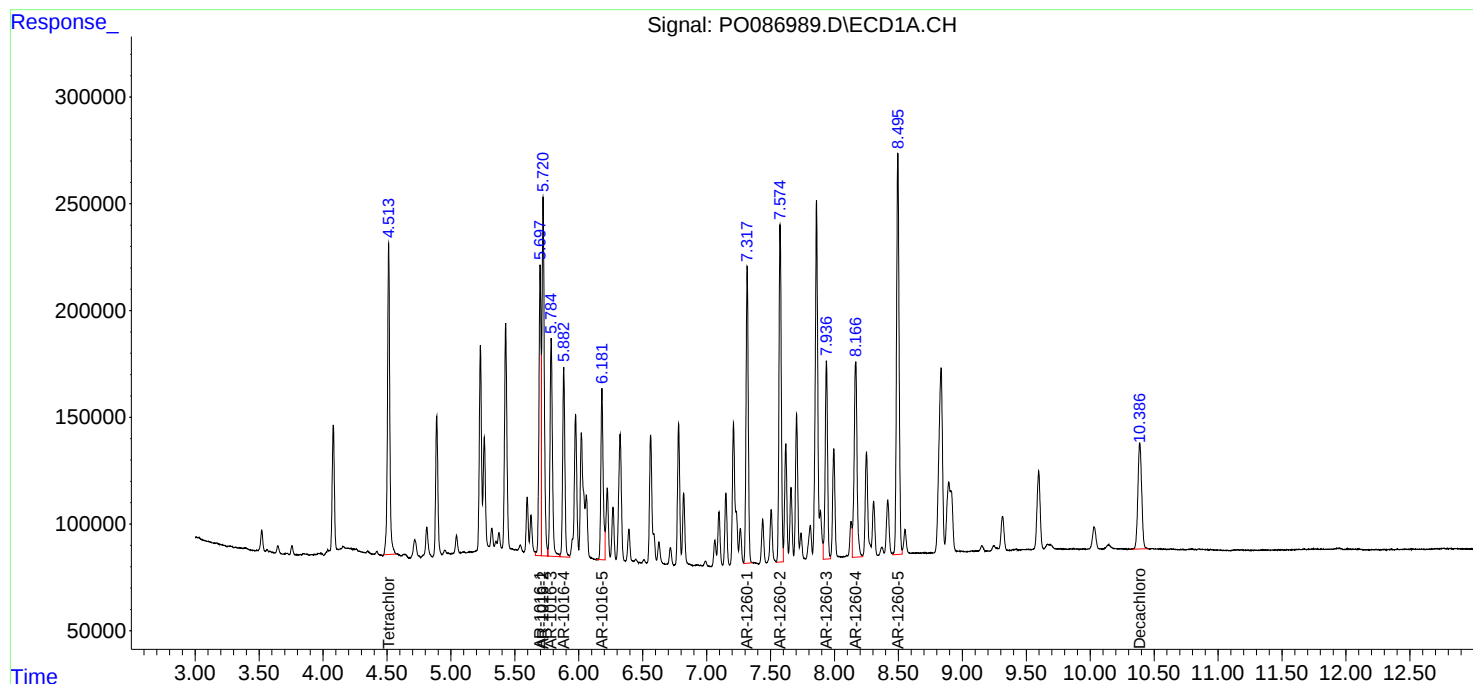


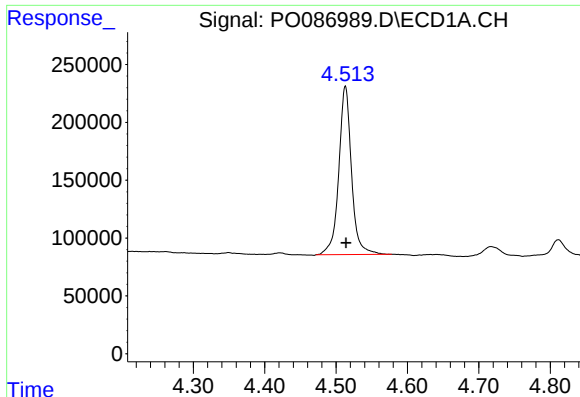

#1 Tetrachloro-m-xylene


R.T.: 4.513 min
Delta R.T.: 0.000 min
Response: 1803567
Conc: 31.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

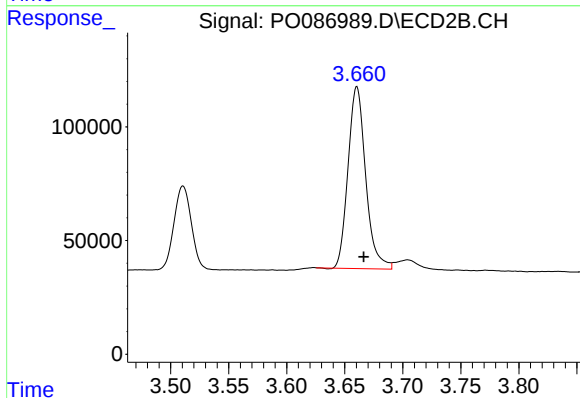


#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: -0.006 min
Response: 847246
Conc: 26.51 ng/ml

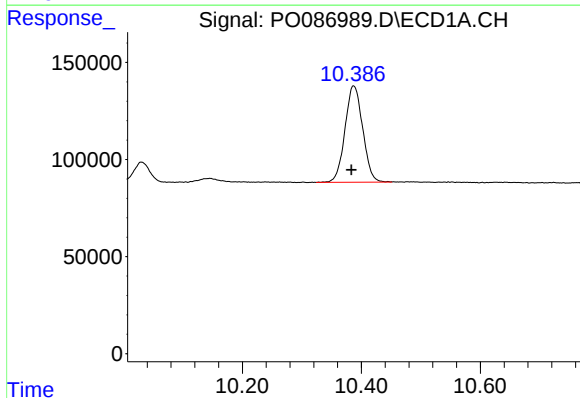


#2 Decachlorobiphenyl

R.T.: 10.387 min
Delta R.T.: 0.003 min
Response: 1026740
Conc: 22.49 ng/ml

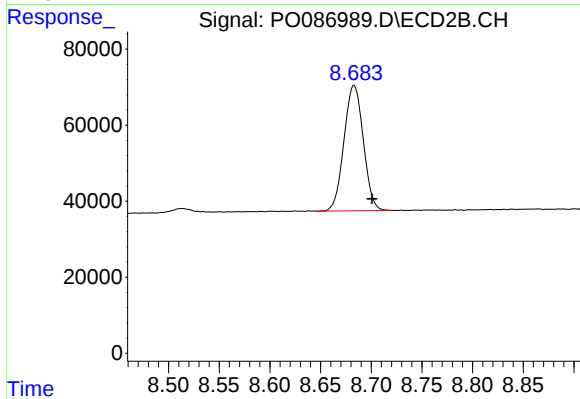

#2 Decachlorobiphenyl


R.T.: 8.683 min
Delta R.T.: -0.018 min
Response: 438100
Conc: 19.54 ng/ml

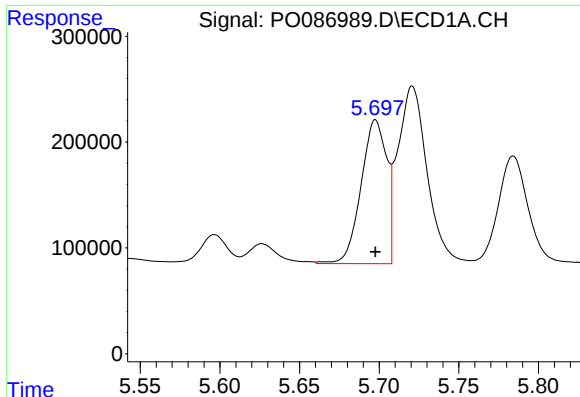

#3 AR-1016-1


R.T.: 5.698 min
Delta R.T.: 0.000 min
Response: 1525086
Conc: 768.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

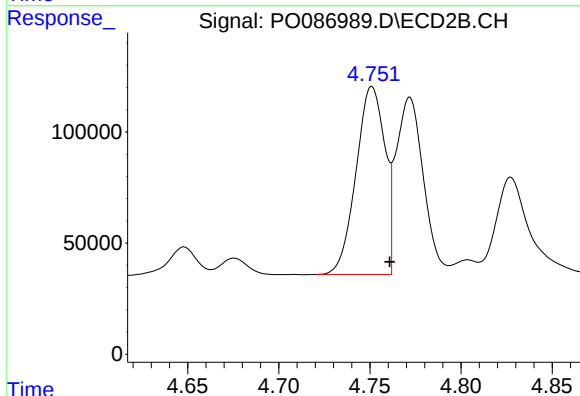


#3 AR-1016-1

R.T.: 4.751 min
Delta R.T.: -0.010 min
Response: 929717
Conc: 941.86 ng/ml

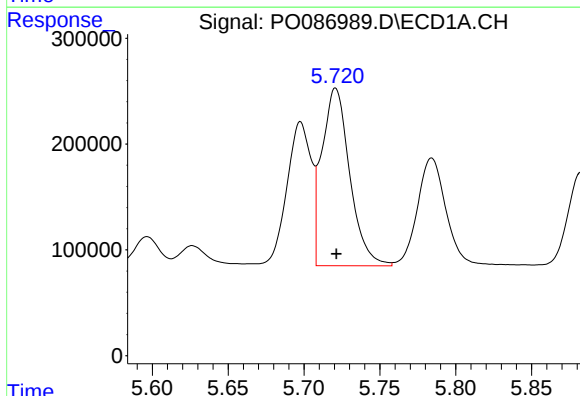


#4 AR-1016-2

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 2146967
Conc: 757.66 ng/ml

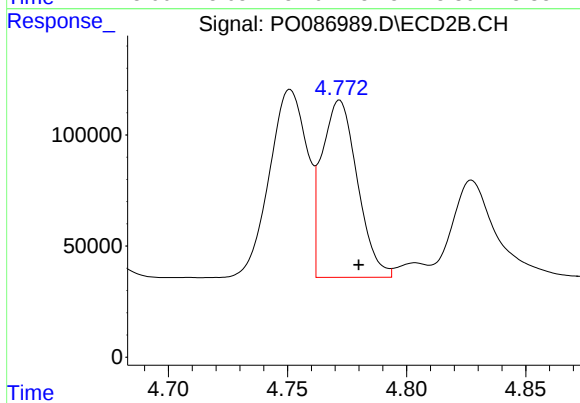

#4 AR-1016-2


R.T.: 4.772 min
Delta R.T.: -0.008 min
Response: 827496
Conc: 606.74 ng/ml

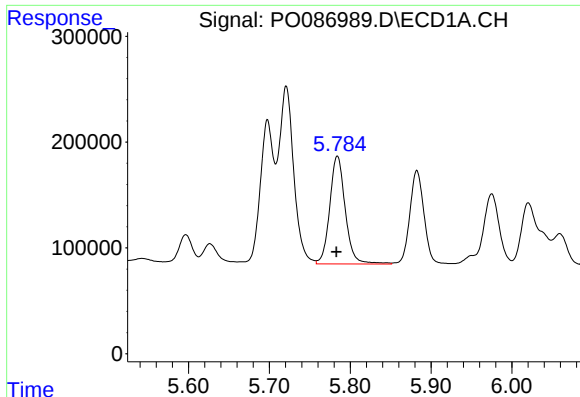

#5 AR-1016-3


R.T.: 5.784 min
Delta R.T.: 0.001 min
Response: 1361988
Conc: 779.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

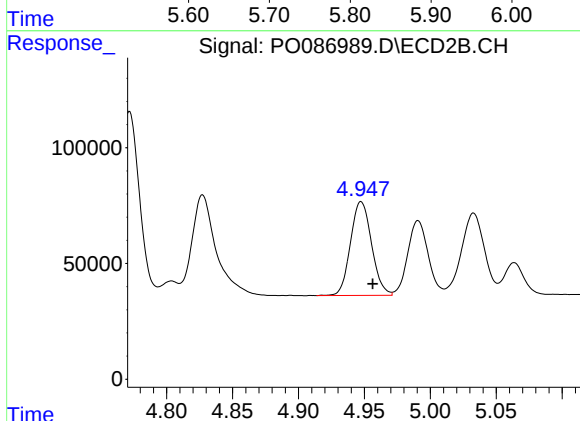


#5 AR-1016-3

R.T.: 4.947 min
Delta R.T.: -0.009 min
Response: 452398
Conc: 613.70 ng/ml

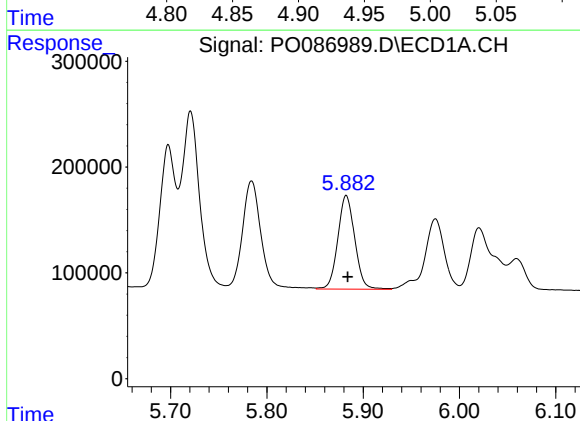


#6 AR-1016-4

R.T.: 5.883 min
Delta R.T.: -0.001 min
Response: 1080771
Conc: 773.77 ng/ml

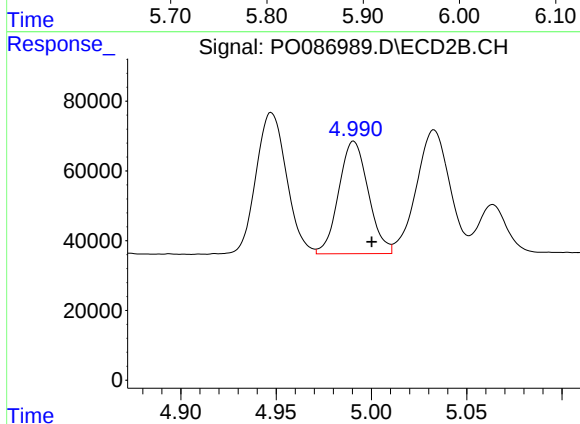

#6 AR-1016-4


R.T.: 4.991 min
Delta R.T.: -0.009 min
Response: 348313
Conc: 596.34 ng/ml

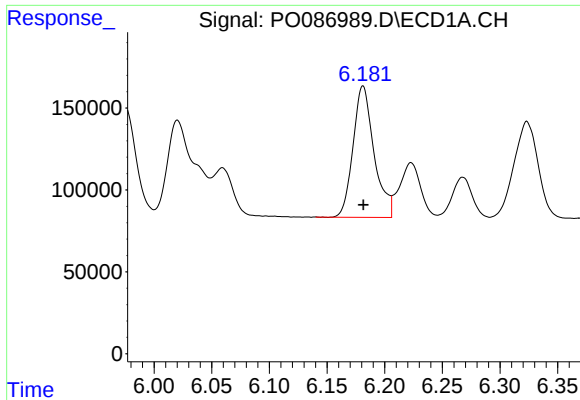

#7 AR-1016-5


R.T.: 6.181 min
Delta R.T.: 0.000 min
Response: 1014842
Conc: 738.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

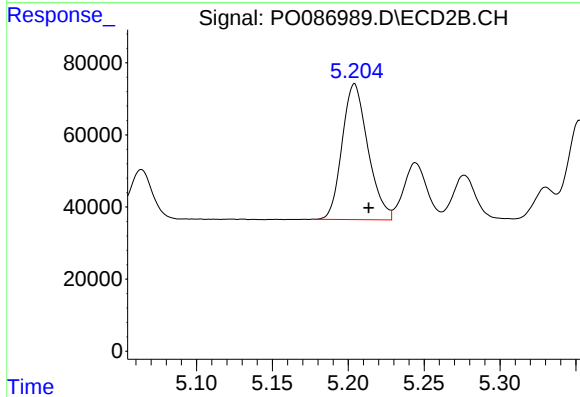


#7 AR-1016-5

R.T.: 5.204 min
Delta R.T.: -0.009 min
Response: 446092
Conc: 612.67 ng/ml

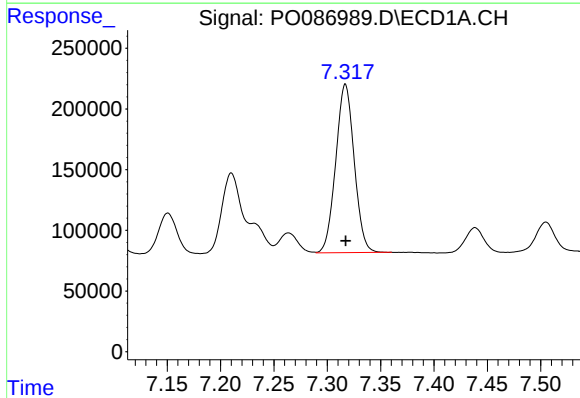


#31 AR-1260-1

R.T.: 7.317 min
Delta R.T.: 0.000 min
Response: 1668879
Conc: 672.45 ng/ml

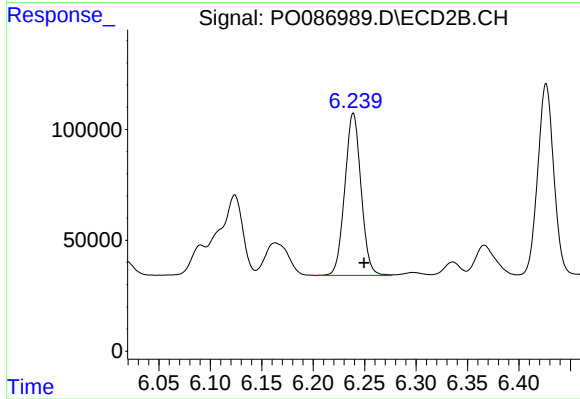

#31 AR-1260-1


R.T.: 6.239 min
Delta R.T.: -0.010 min
Response: 802899
Conc: 620.01 ng/ml

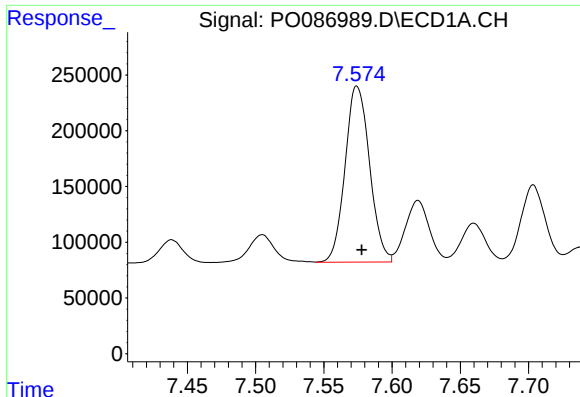

#32 AR-1260-2


R.T.: 7.574 min
Delta R.T.: -0.004 min
Response: 1974398
Conc: 582.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

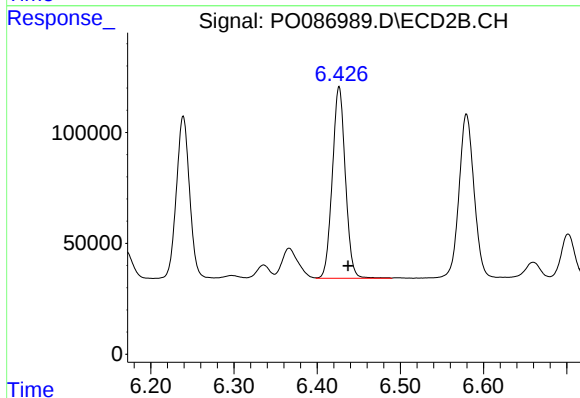


#32 AR-1260-2

R.T.: 6.426 min
Delta R.T.: -0.011 min
Response: 940637
Conc: 608.99 ng/ml

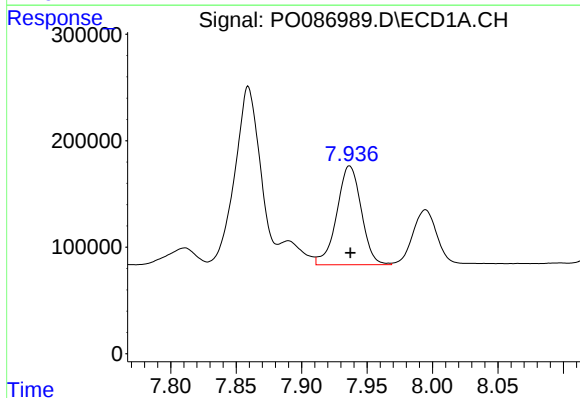


#33 AR-1260-3

R.T.: 7.937 min
Delta R.T.: 0.000 min
Response: 1206877
Conc: 558.54 ng/ml

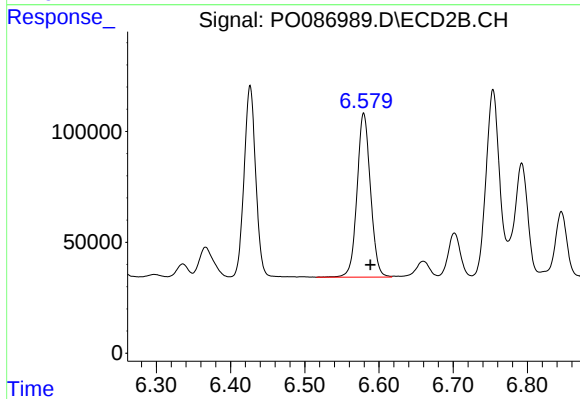

#33 AR-1260-3


R.T.: 6.579 min
Delta R.T.: -0.009 min
Response: 928195
Conc: 534.10 ng/ml

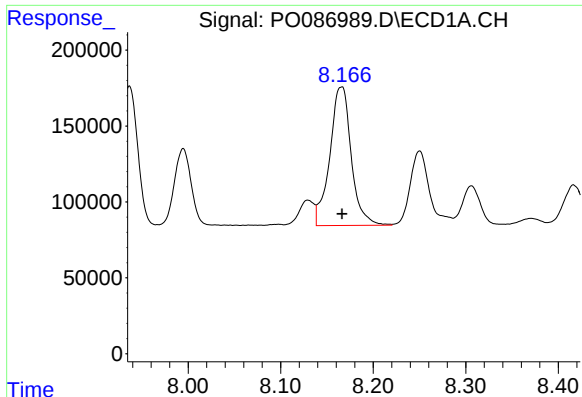

#34 AR-1260-4


R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 1472250
Conc: 572.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220425-SPLP-AMENDED-COMP-EMS

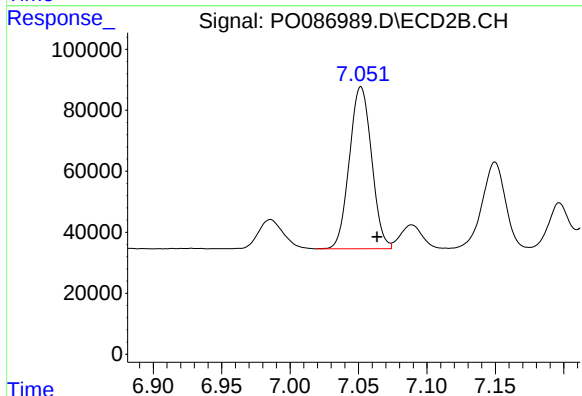


#34 AR-1260-4

R.T.: 7.052 min
Delta R.T.: -0.012 min
Response: 600734
Conc: 527.80 ng/ml

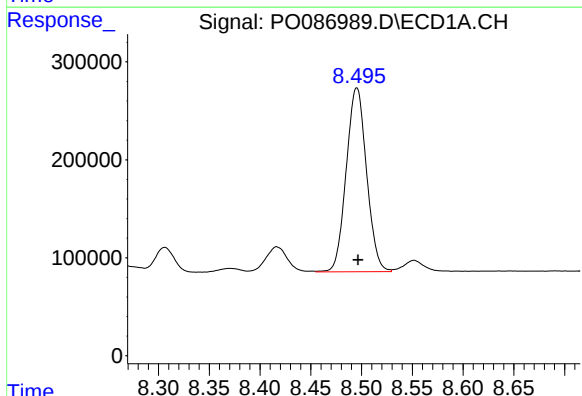

#35 AR-1260-5

R.T.: 8.495 min
Delta R.T.: -0.001 min
Response: 2618446
Conc: 551.03 ng/ml

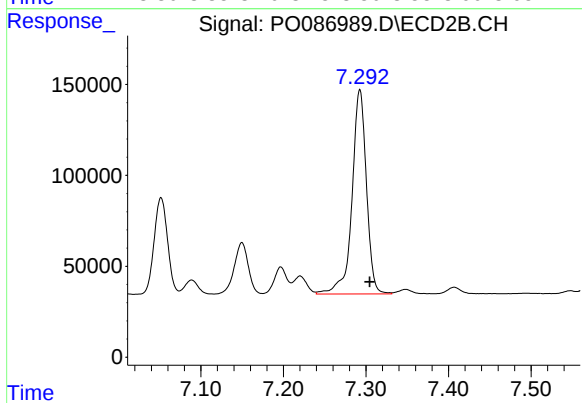

#35 AR-1260-5

R.T.: 7.293 min
Delta R.T.: -0.012 min
Response: 1364558
Conc: 513.80 ng/ml