

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060722\
 Data File : P0086993.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jun 2022 19:07
 Operator : YP\AJ
 Sample : N3170-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220424-SPLP-AMENDED-COMPOSITE-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 01:35:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jun 01 17:55:39 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.514	3.662	1449594	711416	25.346	22.256
2) SA Decachlor...	10.391	8.683	1118163	473773	24.497	21.129

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060722\
Data File : P0086993.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jun 2022 19:07
Operator : YP\AJ
Sample : N3170-06
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220424-SPLP-AMENDED-COMPOSITE-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 01:35:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jun 01 17:55:39 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

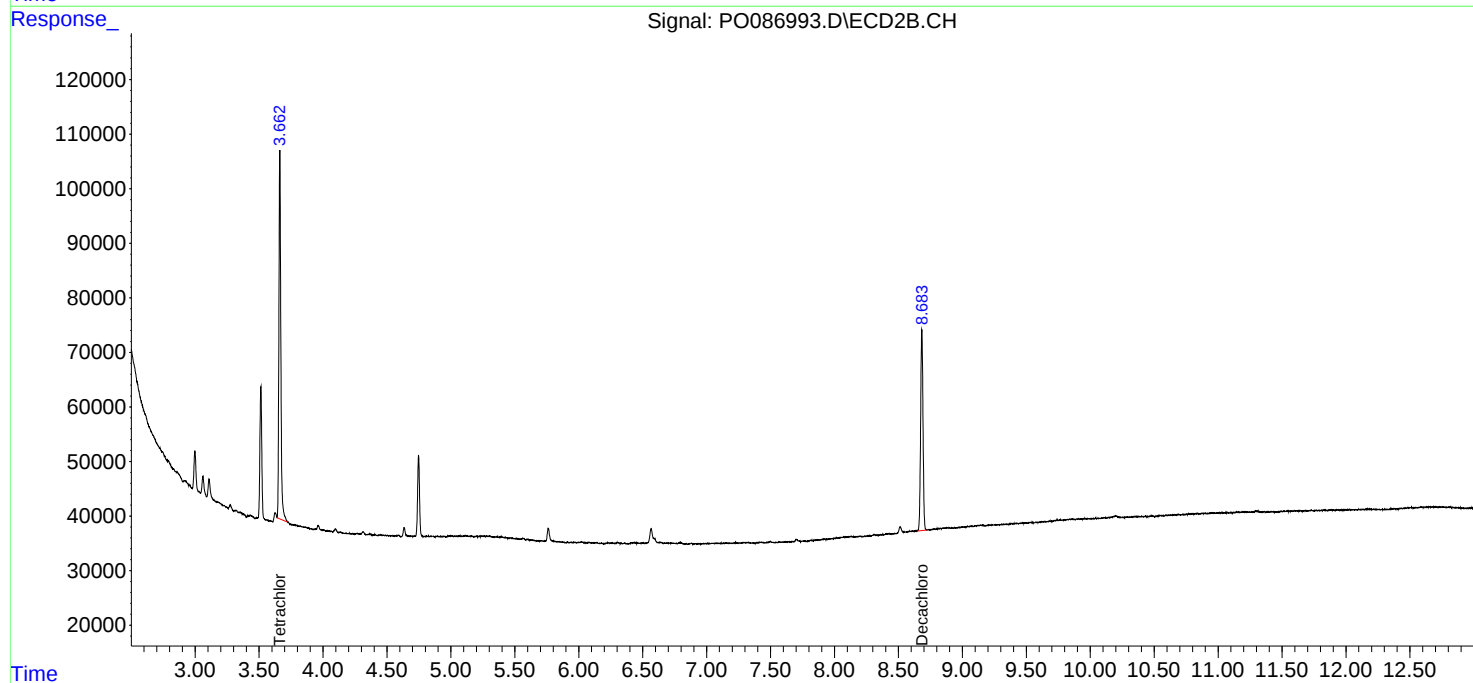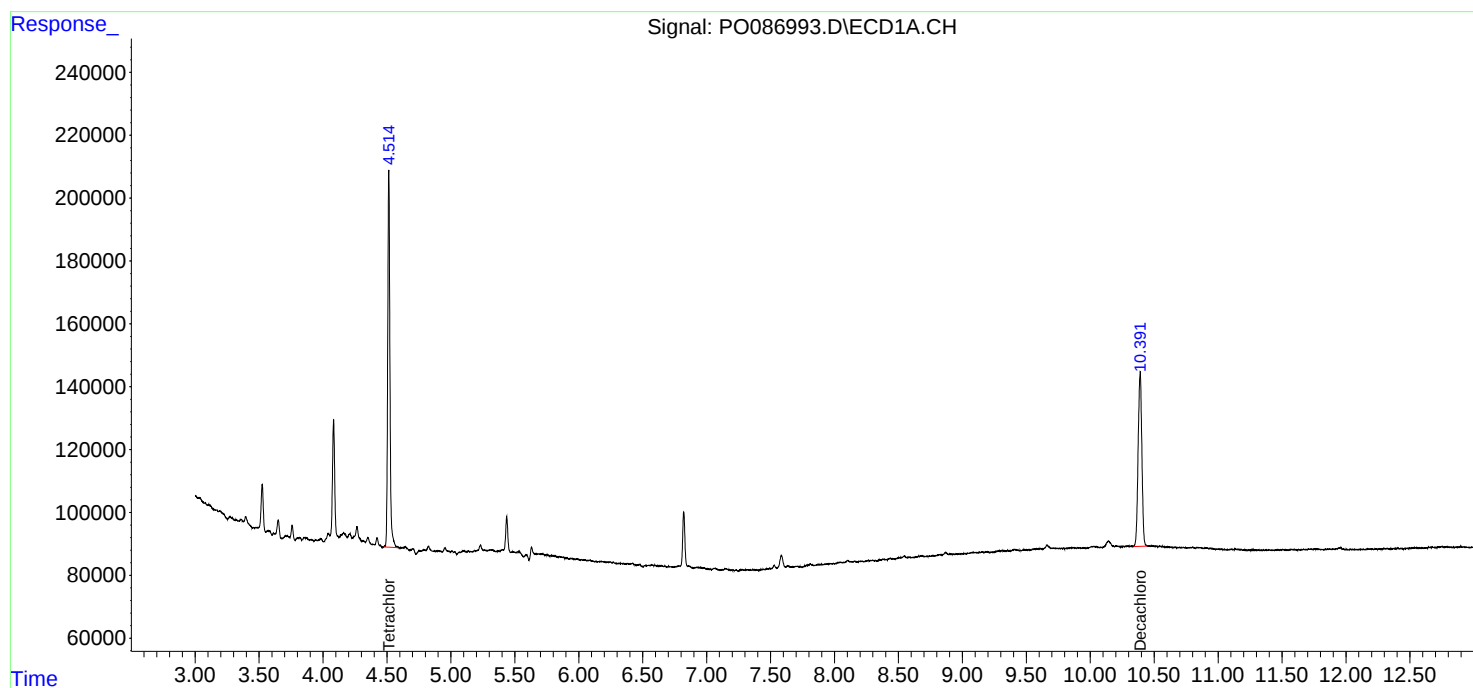

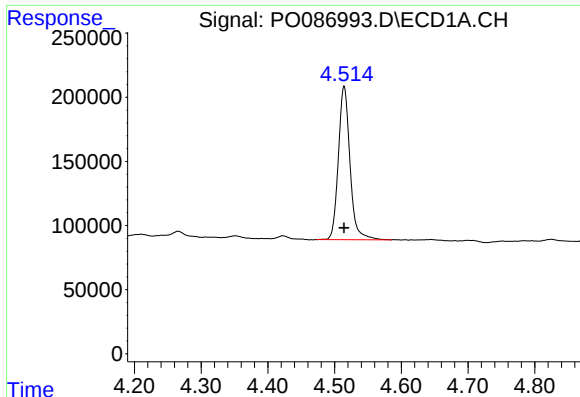

#1 Tetrachloro-m-xylene


R.T.: 4.514 min
Delta R.T.: 0.000 min
Response: 1449594
Conc: 25.35 ng/ml

Instrument :

ECD_O


ClientSampleId :

20220424-SPLP-AMENDED-COMPOSITE-D

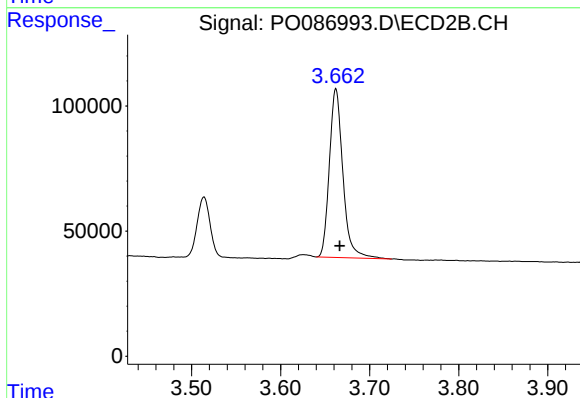


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.004 min
Response: 711416
Conc: 22.26 ng/ml

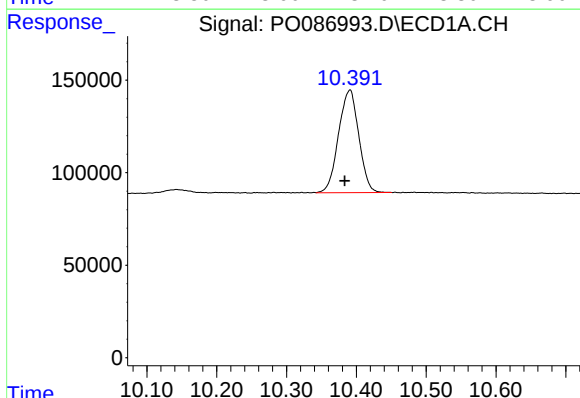

#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.008 min
Response: 1118163
Conc: 24.50 ng/ml

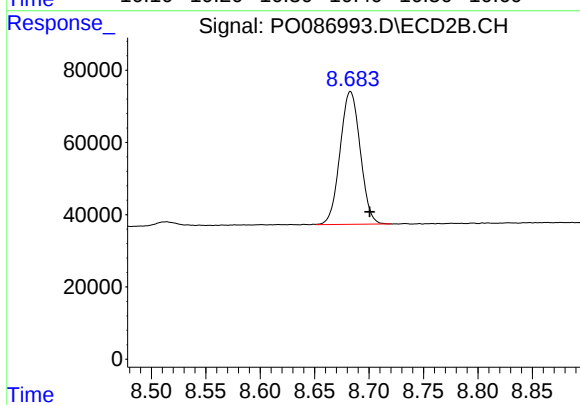

#2 Decachlorobiphenyl

R.T.: 8.683 min
Delta R.T.: -0.018 min
Response: 473773
Conc: 21.13 ng/ml