

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060723\
 Data File : P0095545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jun 2023 10:51
 Operator : YP/AJ
 Sample : 03043-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MR-PIPE-A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/08/2023
 Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 08 05:45:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jun 02 06:53:15 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.439	3.655	108.8E6	49456088	29.512	31.531
2) SA Decachlor...	10.292	8.716	72126588	33252684	26.650	25.704

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0060723\
Data File : P0095545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jun 2023 10:51
Operator : YP/AJ
Sample : 03043-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MR-PIPE-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 08 05:45:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060123.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jun 02 06:53:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

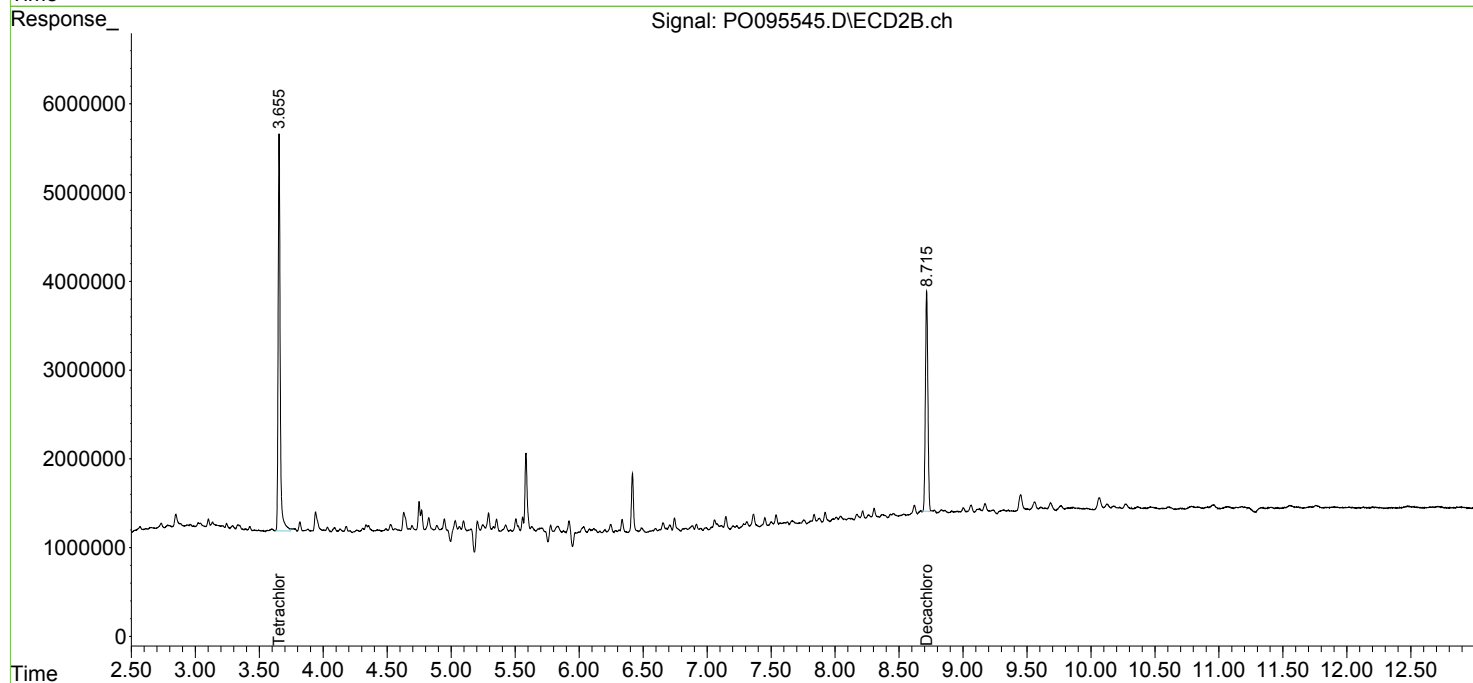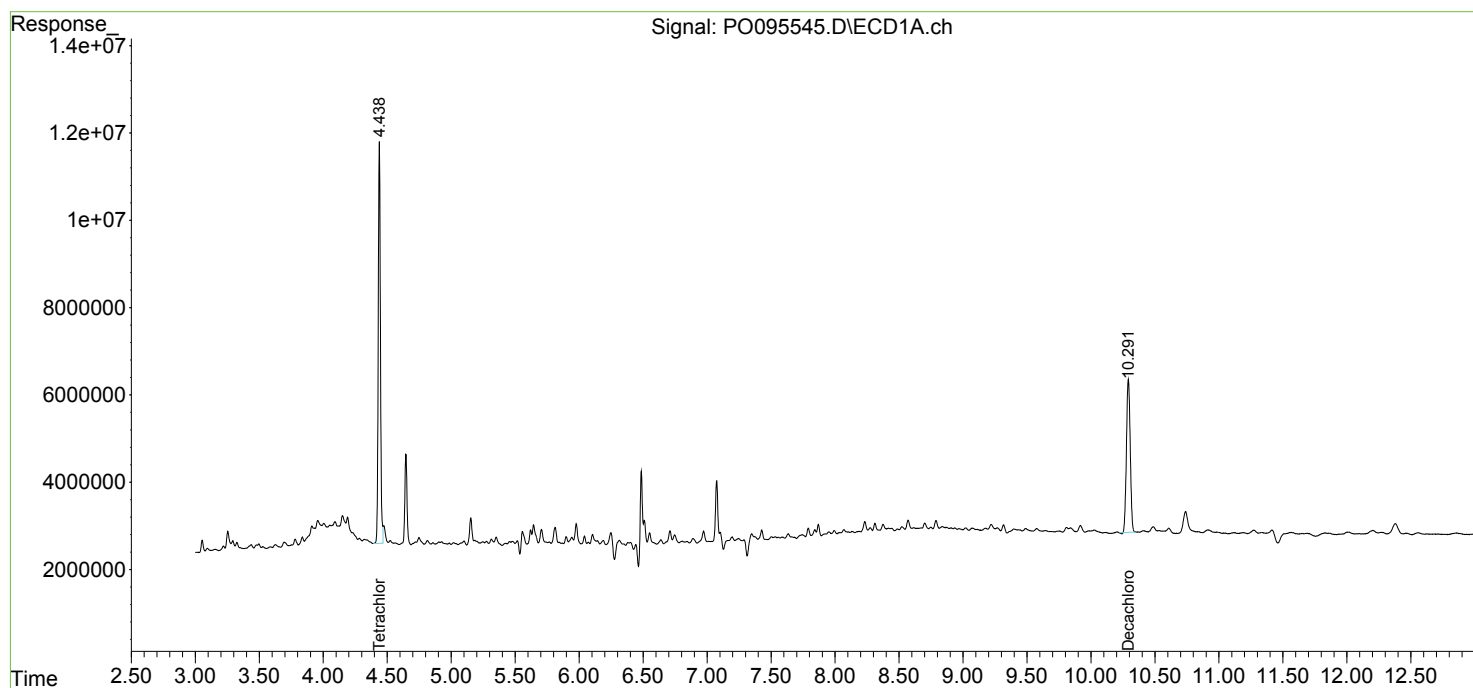

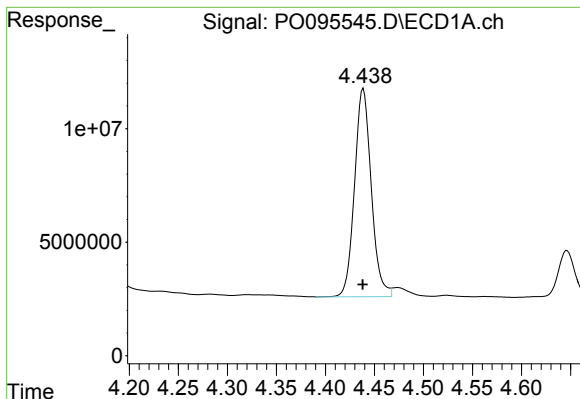


#1 Tetrachloro-m-xylene

R.T.: 4.439 min
Delta R.T.: 0.000 min
Response: 108766323
Conc: 29.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MR-PIPE-A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/08/2023
Supervised By :Ankita Jodhani 06/08/2023

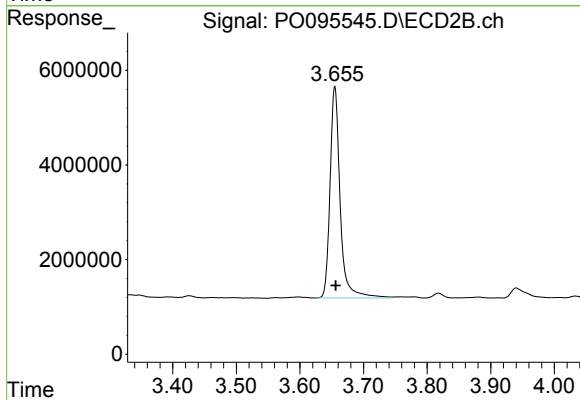


#1 Tetrachloro-m-xylene

R.T.: 3.655 min
Delta R.T.: -0.002 min
Response: 49456088
Conc: 31.53 ng/ml

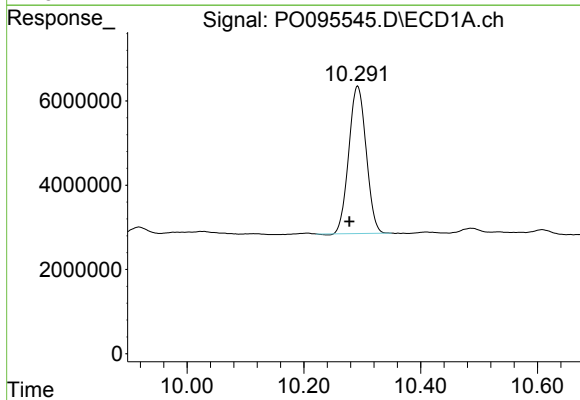

#2 Decachlorobiphenyl

R.T.: 10.292 min
Delta R.T.: 0.014 min
Response: 72126588
Conc: 26.65 ng/ml

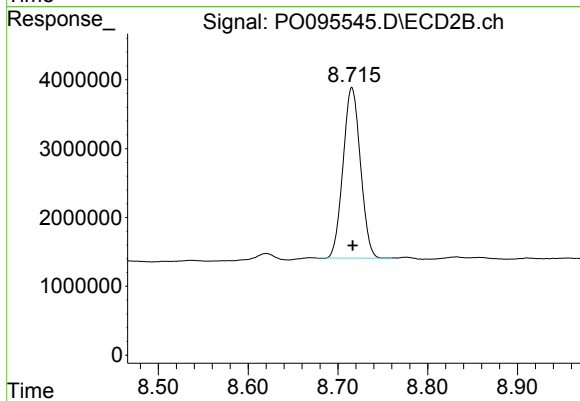

#2 Decachlorobiphenyl

R.T.: 8.716 min
Delta R.T.: 0.000 min
Response: 33252684
Conc: 25.70 ng/ml