

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
 Data File : P0057028.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2019 11:31
 Operator : SM/SJ
 Sample : K3246-01RE
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-PS-01-047RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 12:40:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.243	3.563	664873	568962	17.367	17.253
2)	SA Decachlor...	9.807	8.491	567816	363092	11.568	10.183
Target Compounds							
8)	L2 AR-1221-1	0.000	3.725	0	61229	N.D.	120.732 #
9)	L2 AR-1221-2	0.000	3.930	0	83545	N.D.	221.682 #
10)	L2 AR-1221-3	0.000	3.930	0	83545	N.D.	69.792 #
11)	L3 AR-1232-1	0.000	3.930	0	83545	N.D.	92.997 #
20)	L4 AR-1242-5	0.000	5.446	0	1385282	N.D.	1171.713 #
25)	L5 AR-1248-5	0.000	5.446	0	1385282	N.D.	836.992 #
26)	L6 AR-1254-1	0.000	5.446	0	1385282	N.D.	523.790 #
27)	L6 AR-1254-2	0.000	5.635	0	153828	N.D.	71.355 #
28)	L6 AR-1254-3	6.847	0.000	852427	0	206.730	N.D. #
29)	L6 AR-1254-4	0.000	6.275	0	637969	N.D.	290.391 #
32)	L7 AR-1260-2	0.000	6.315	0	56358	N.D.	22.864 #
33)	L7 AR-1260-3	0.000	6.434	0	45121	N.D.	20.114 #
38)	L8 AR-1262-3	0.000	7.463	0	2342126	N.D.	793.019 #
39)	L8 AR-1262-4	0.000	7.463	0	2342126	N.D.	449.492 #
41)	L9 AR-1268-1	0.000	7.463	0	2342126	N.D.	313.743 #
42)	L9 AR-1268-2	0.000	7.463	0	2342126	N.D.	335.400 #
43)	L9 AR-1268-3	0.000	7.754	0	16964	N.D.	2.858 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061019\
Data File : PO057028.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2019 11:31
Operator : SM/SJ
Sample : K3246-01RE
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 12:40:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

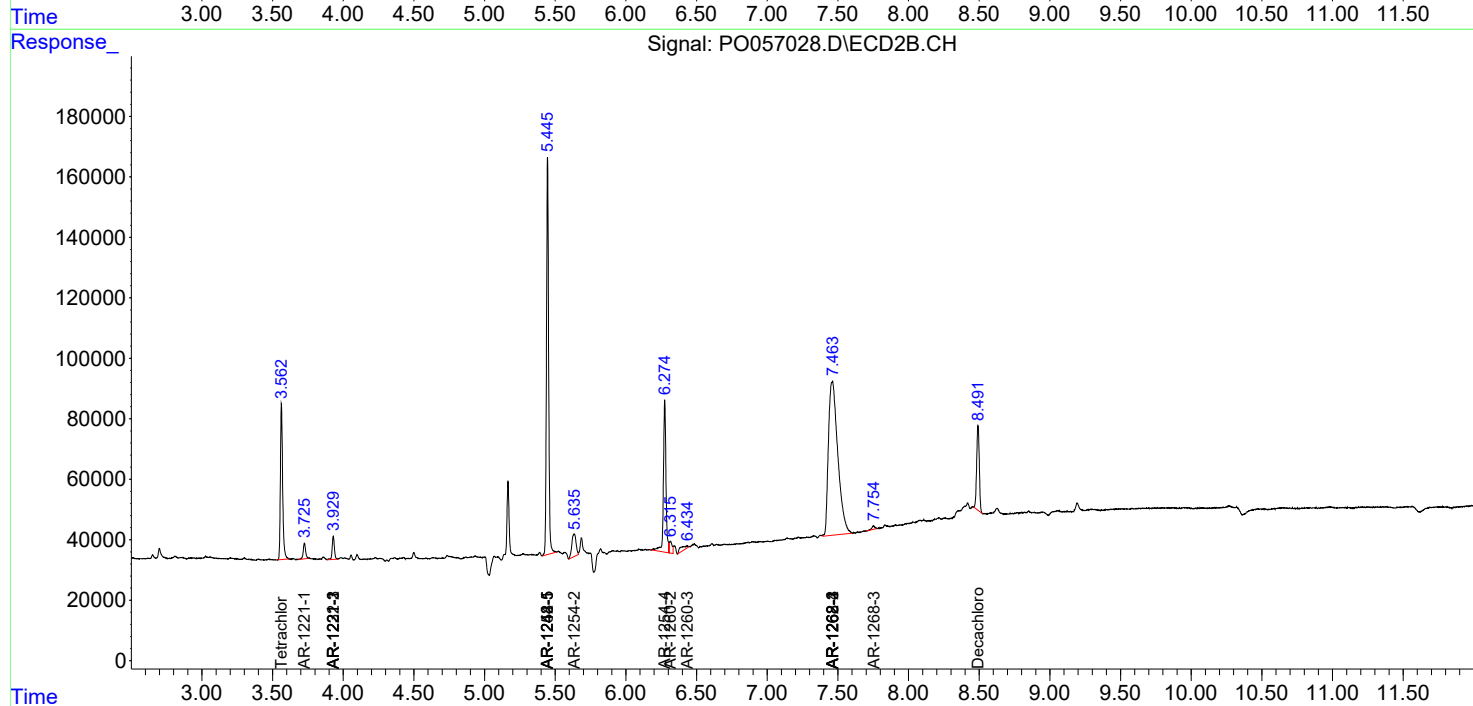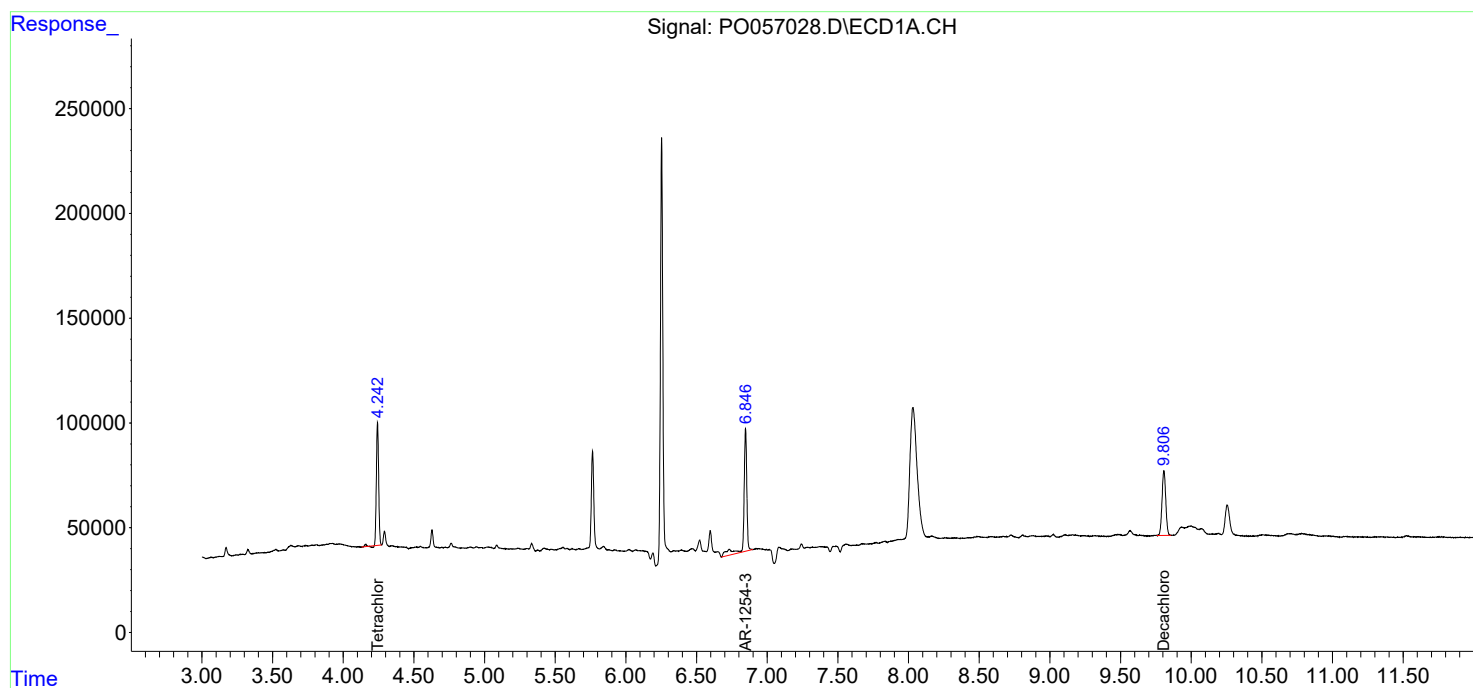


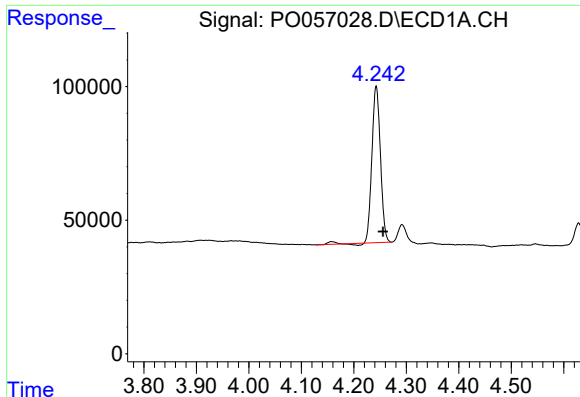

#1 Tetrachloro-m-xylene


R.T.: 4.243 min
Delta R.T.: -0.013 min
Response: 664873
Conc: 17.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

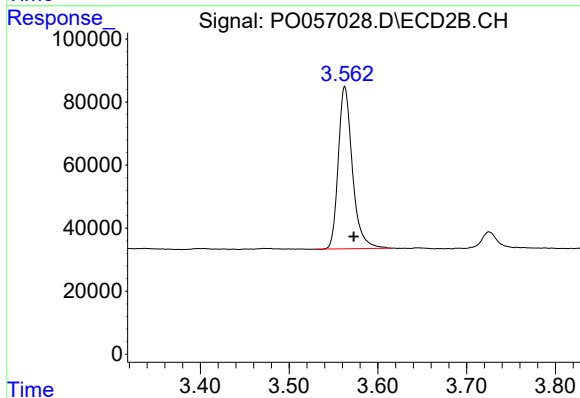


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 568962
Conc: 17.25 ng/ml

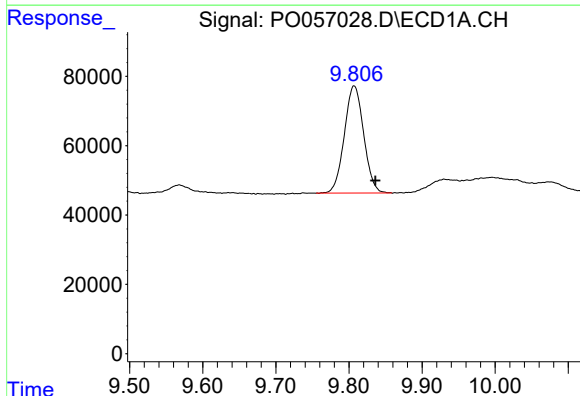


#2 Decachlorobiphenyl

R.T.: 9.807 min
Delta R.T.: -0.029 min
Response: 567816
Conc: 11.57 ng/ml

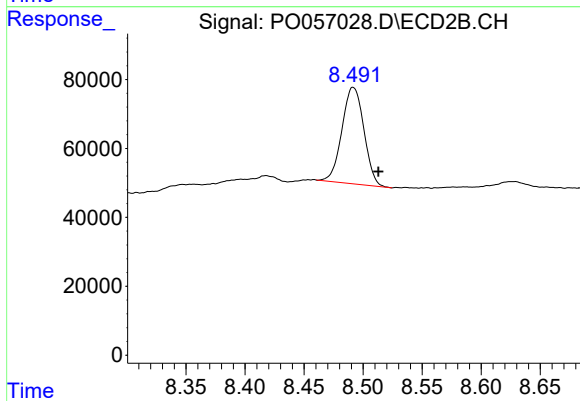

#2 Decachlorobiphenyl


R.T.: 8.491 min
Delta R.T.: -0.022 min
Response: 363092
Conc: 10.18 ng/ml

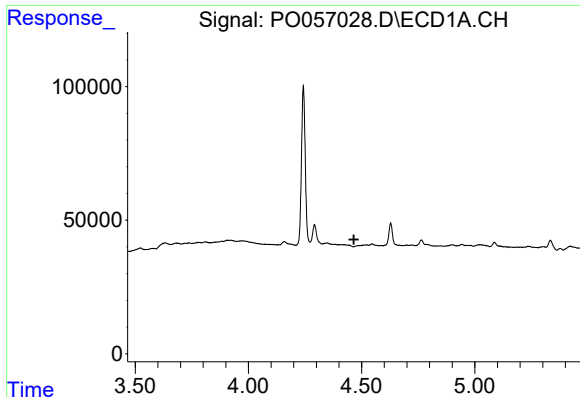

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.466 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

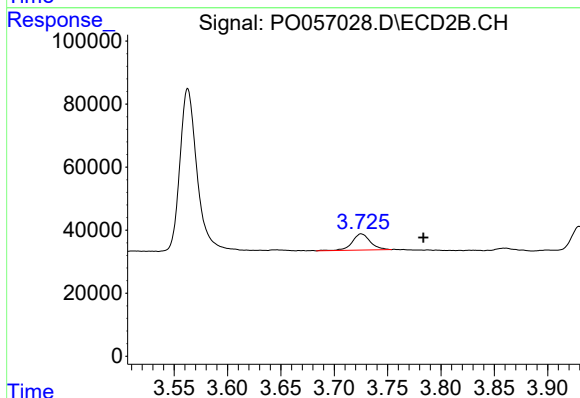


#8 AR-1221-1

R.T.: 3.725 min
Delta R.T.: -0.058 min
Response: 61229
Conc: 120.73 ng/ml

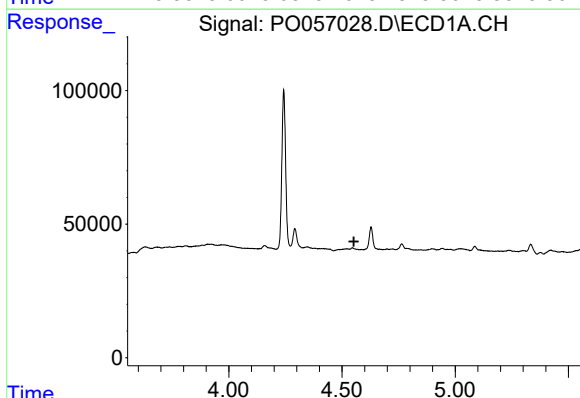


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.553 min
Response: 0
Conc: N.D.

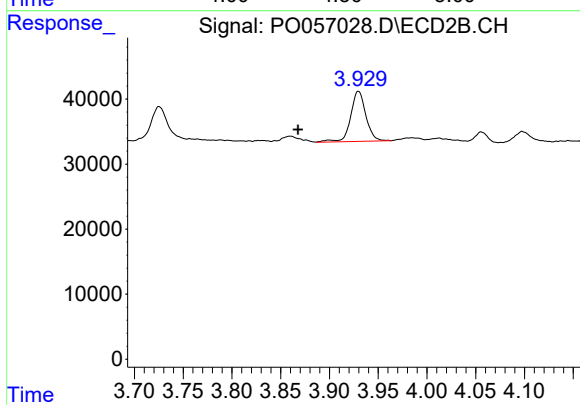

#9 AR-1221-2


R.T.: 3.930 min
Delta R.T.: 0.062 min
Response: 83545
Conc: 221.68 ng/ml

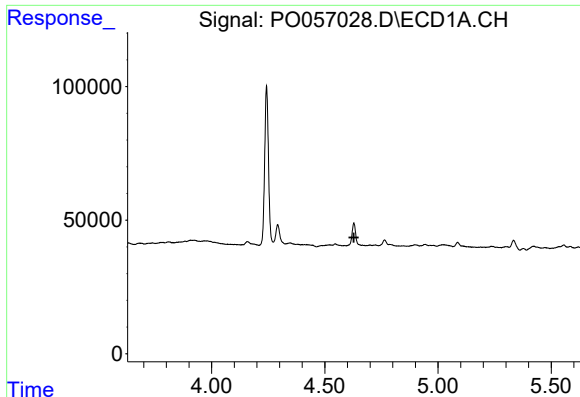

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 4.628 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

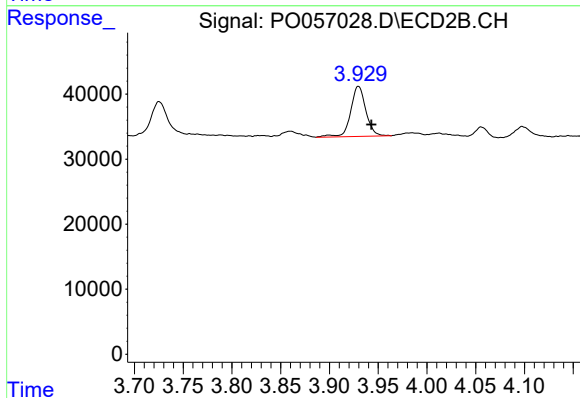


#10 AR-1221-3

R.T.: 3.930 min
Delta R.T.: -0.013 min
Response: 83545
Conc: 69.79 ng/ml

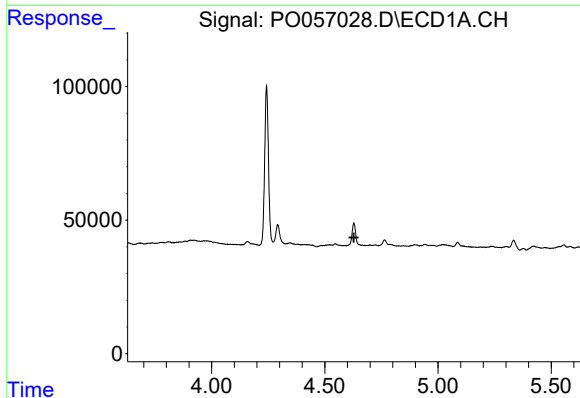


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 4.629 min
Response: 0
Conc: N.D.

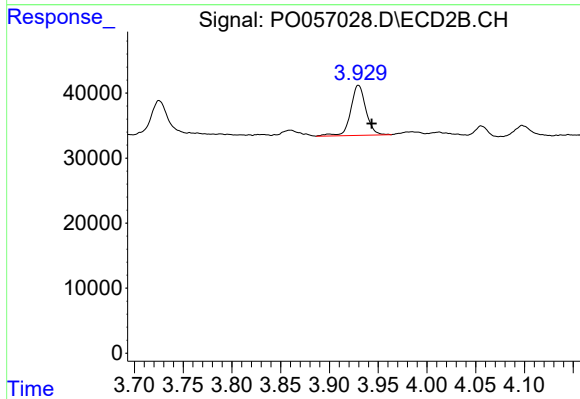

#11 AR-1232-1


R.T.: 3.930 min
Delta R.T.: -0.014 min
Response: 83545
Conc: 93.00 ng/ml

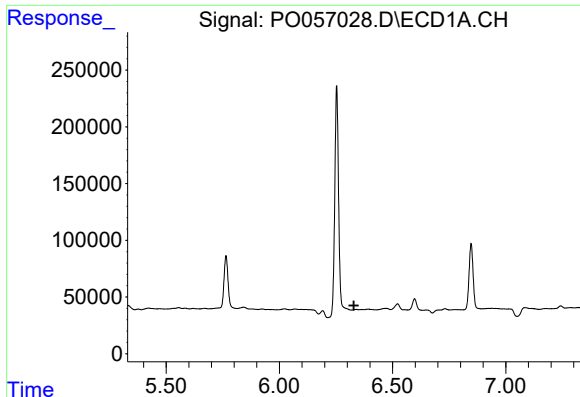

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

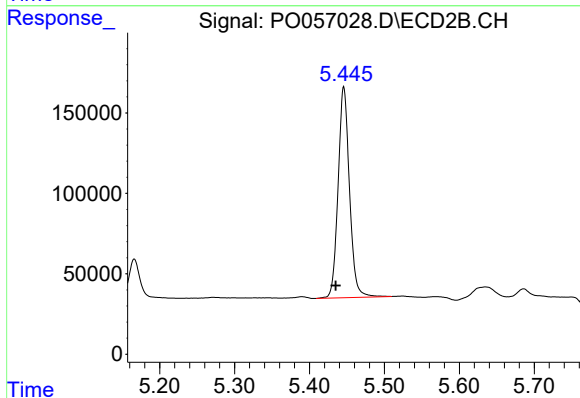


#20 AR-1242-5

R.T.: 5.446 min
Delta R.T.: 0.011 min
Response: 1385282
Conc: 1171.71 ng/ml

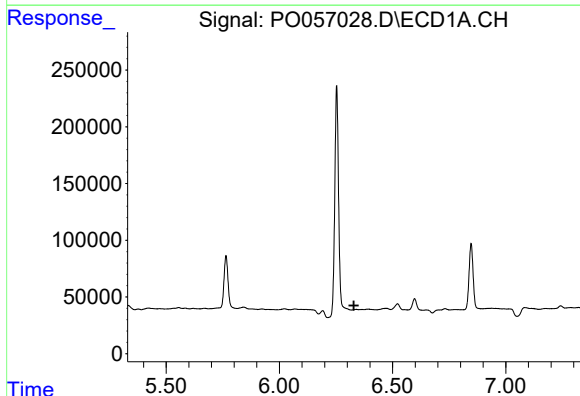


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 6.329 min
Response: 0
Conc: N.D.

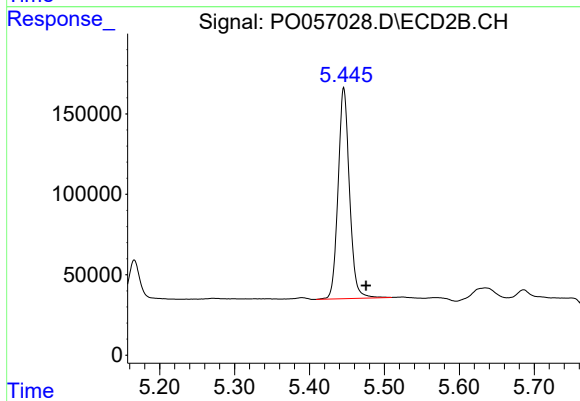

#25 AR-1248-5


R.T.: 5.446 min
Delta R.T.: -0.030 min
Response: 1385282
Conc: 836.99 ng/ml

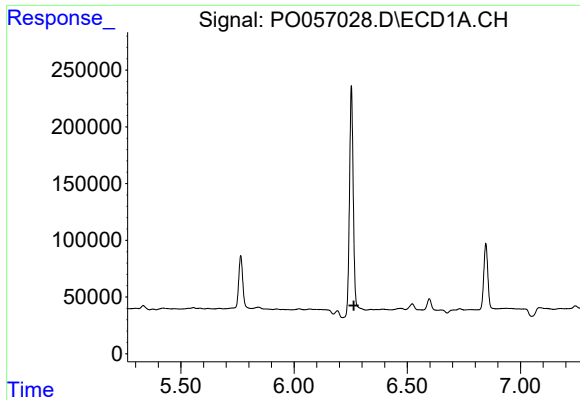

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T.: 6.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

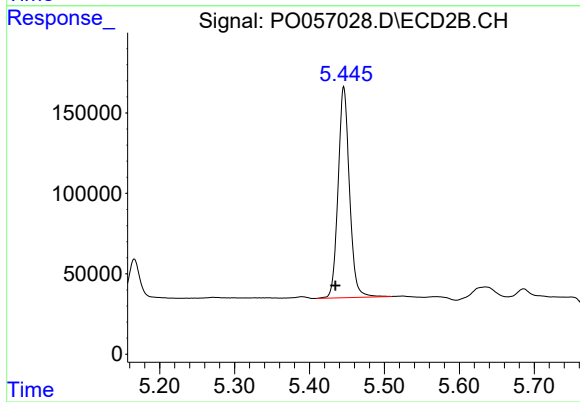


#26 AR-1254-1

R.T.: 5.446 min
Delta R.T.: 0.011 min
Response: 1385282
Conc: 523.79 ng/ml

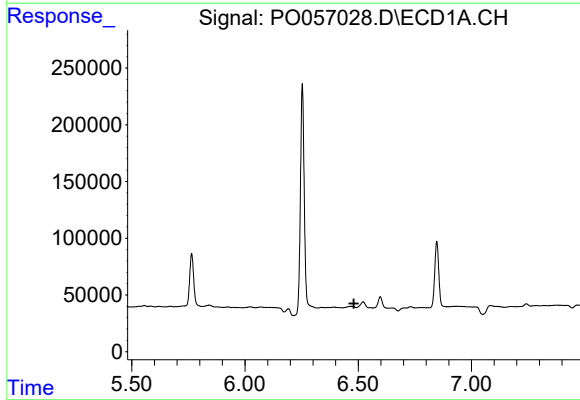


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.481 min
Response: 0
Conc: N.D.

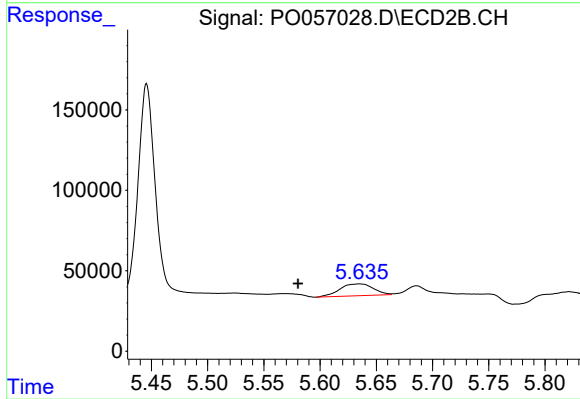

#27 AR-1254-2


R.T.: 5.635 min
Delta R.T.: 0.054 min
Response: 153828
Conc: 71.36 ng/ml

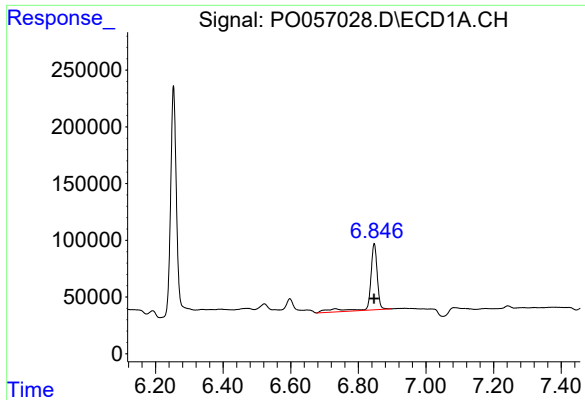

#28 AR-1254-3


R.T.: 6.847 min
Delta R.T.: 0.000 min
Response: 852427
Conc: 206.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

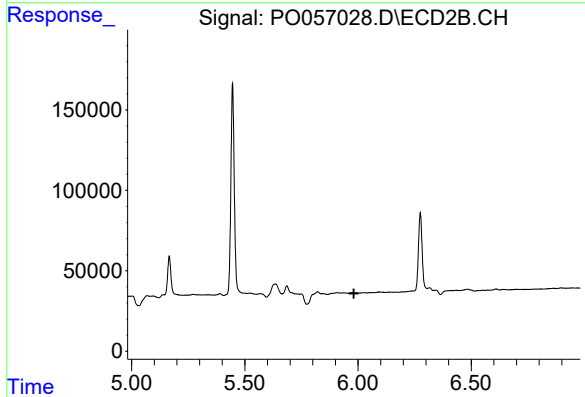


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 5.982 min
Response: 0
Conc: N.D.

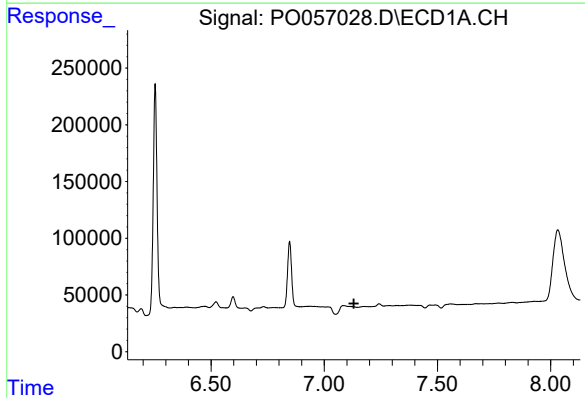


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.131 min
Response: 0
Conc: N.D.

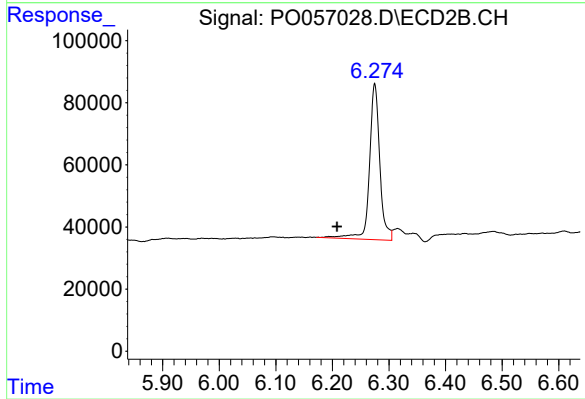

#29 AR-1254-4


R.T.: 6.275 min
Delta R.T.: 0.067 min
Response: 637969
Conc: 290.39 ng/ml

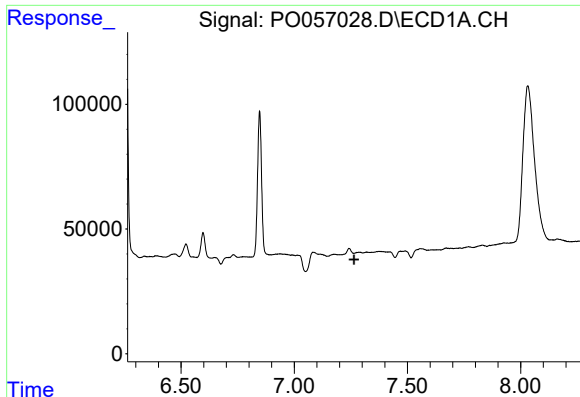

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 7.264 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

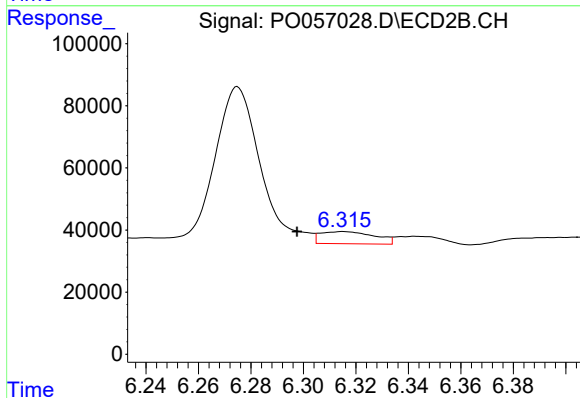


#32 AR-1260-2

R.T.: 6.315 min
Delta R.T.: 0.018 min
Response: 56358
Conc: 22.86 ng/ml

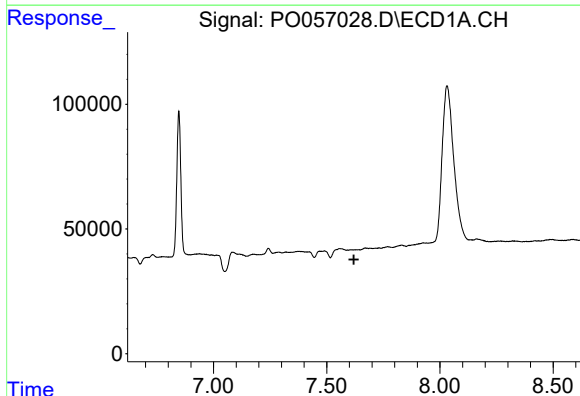


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

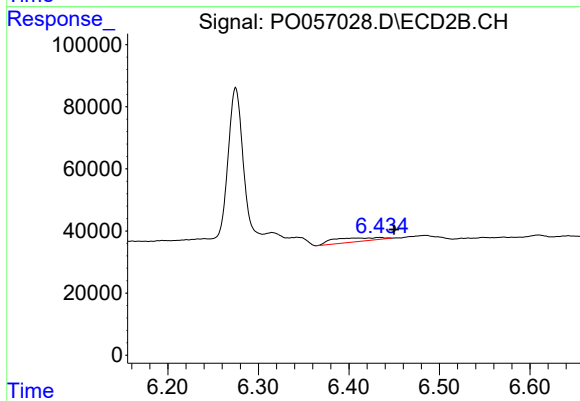

#33 AR-1260-3


R.T.: 6.434 min
Delta R.T.: -0.015 min
Response: 45121
Conc: 20.11 ng/ml

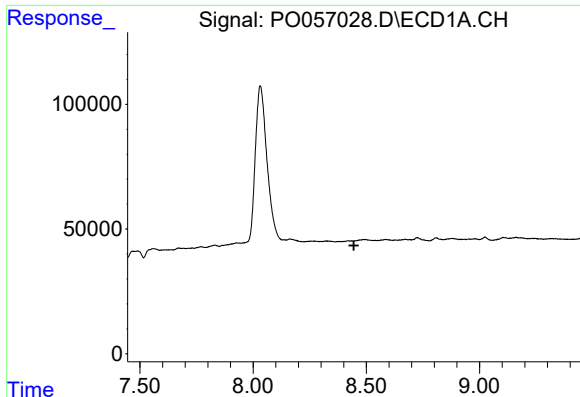

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.445 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

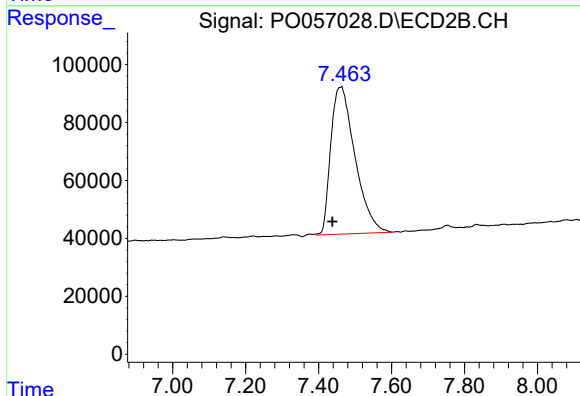


#38 AR-1262-3

R.T.: 7.463 min
Delta R.T.: 0.025 min
Response: 2342126
Conc: 793.02 ng/ml

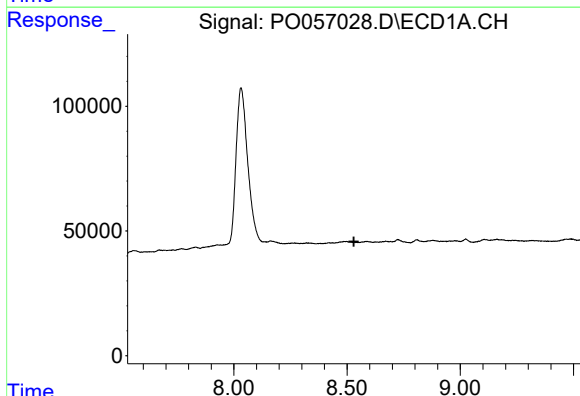


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T.: 8.530 min
Response: 0
Conc: N.D.

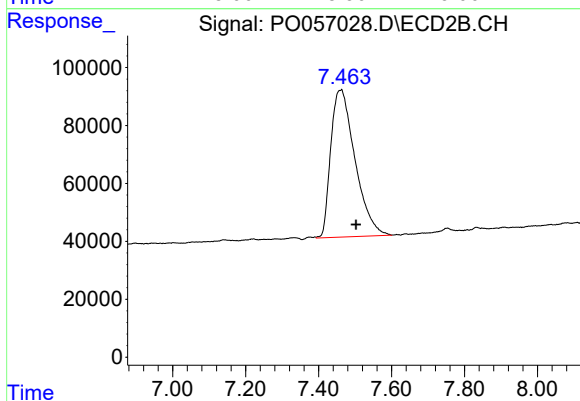

#39 AR-1262-4


R.T.: 7.463 min
Delta R.T.: -0.040 min
Response: 2342126
Conc: 449.49 ng/ml

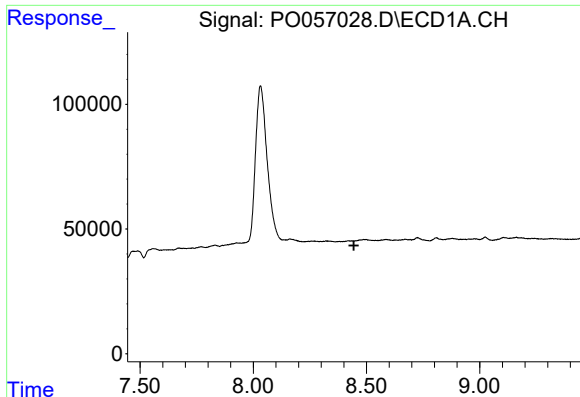

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

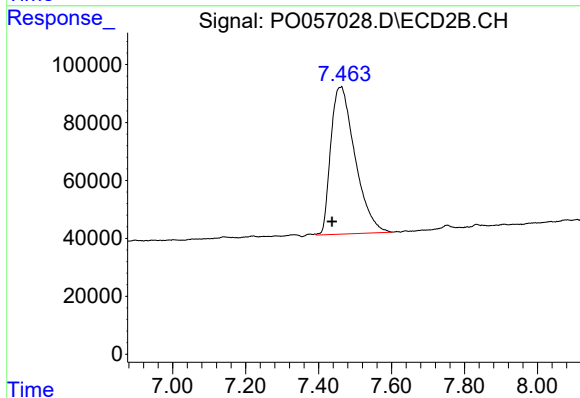


#41 AR-1268-1

R.T.: 7.463 min
Delta R.T.: 0.026 min
Response: 2342126
Conc: 313.74 ng/ml

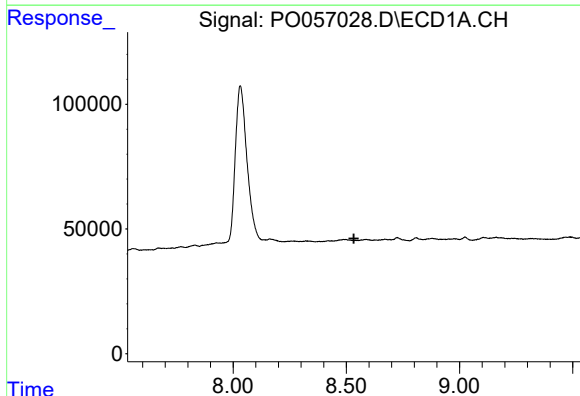


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.534 min
Response: 0
Conc: N.D.

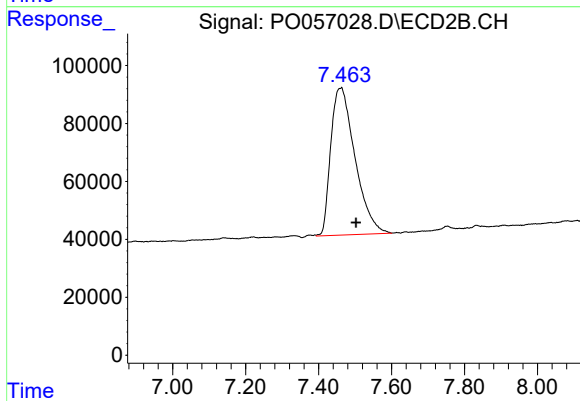

#42 AR-1268-2


R.T.: 7.463 min
Delta R.T.: -0.039 min
Response: 2342126
Conc: 335.40 ng/ml

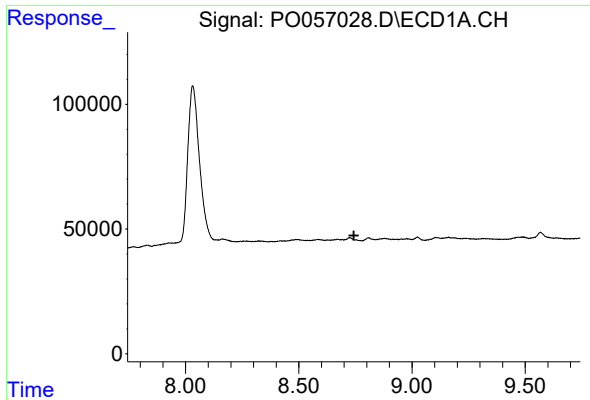

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 8.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
FK-PS-01-047RE

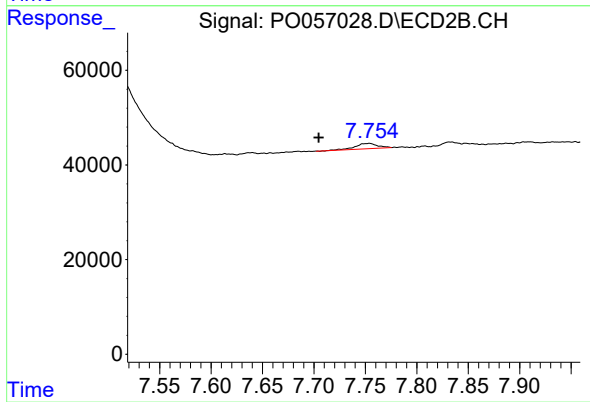

#43 AR-1268-3

R.T.: 7.754 min
Delta R.T.: 0.049 min
Response: 16964
Conc: 2.86 ng/ml