

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
 Data File : P0057019.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2019 8:59
 Operator : SM/SJ
 Sample : K3241-19RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Q115-7ARE

Manual Integrations
 APPROVED

Ankita
 6/11/2019 2:43:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 12:32:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.244	3.562	697445	571947	18.218	17.343
2)	SA Decachlor...	9.809	8.492	451624	284650	9.201m	7.983

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061019\
Data File : PO057019.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2019 8:59
Operator : SM/SJ
Sample : K3241-19RE
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Q115-7ARE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:43:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 12:32:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

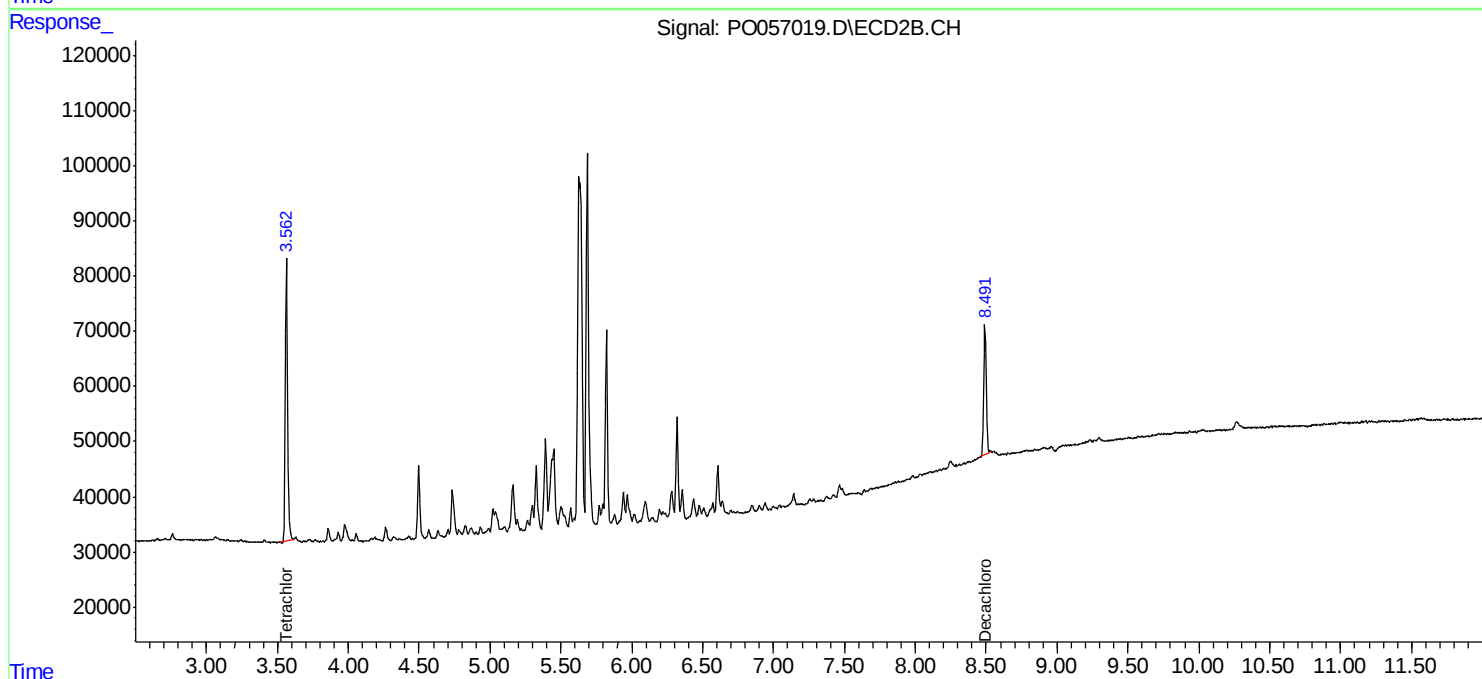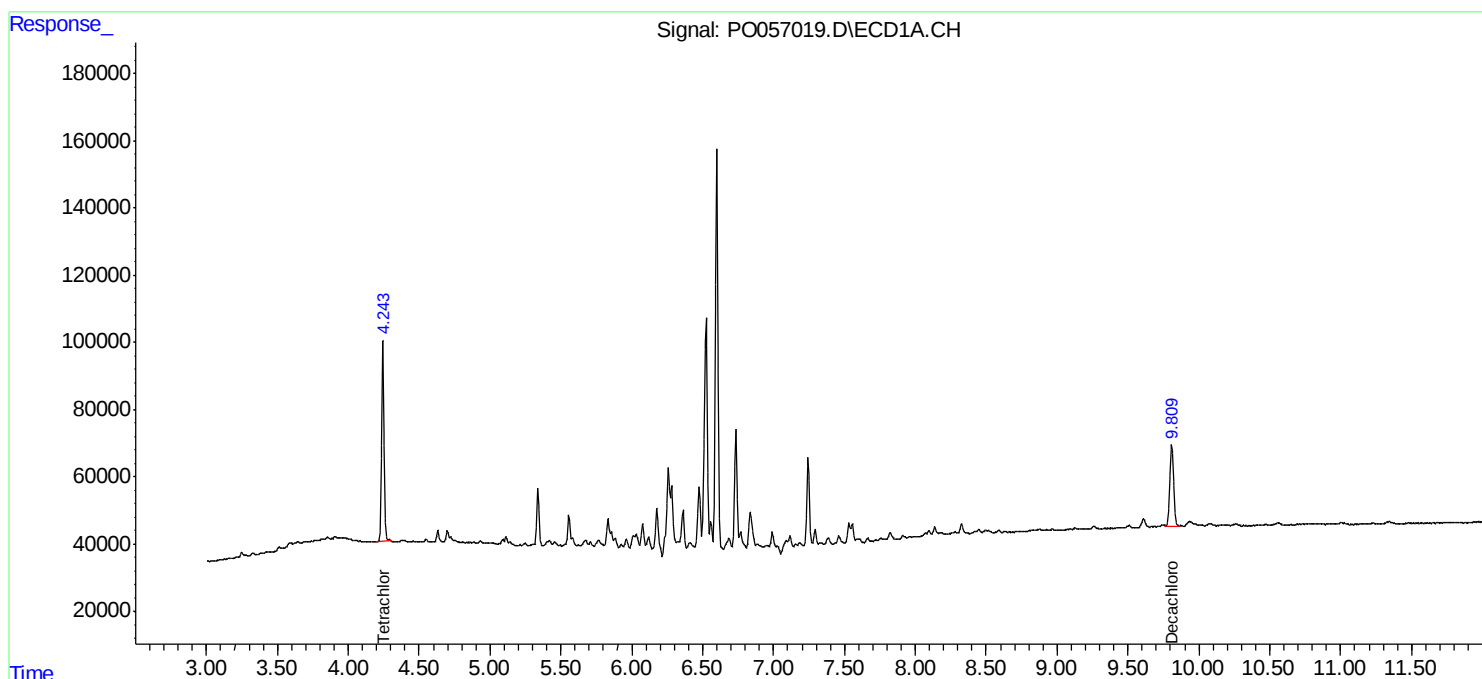

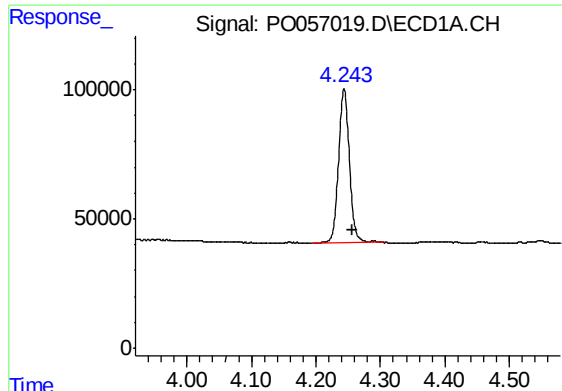


#1 Tetrachloro-m-xylene

R.T.: 4.244 min
Delta R.T.: -0.012 min
Response: 697445
Conc: 18.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
Q115-7ARE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:43:56 PM

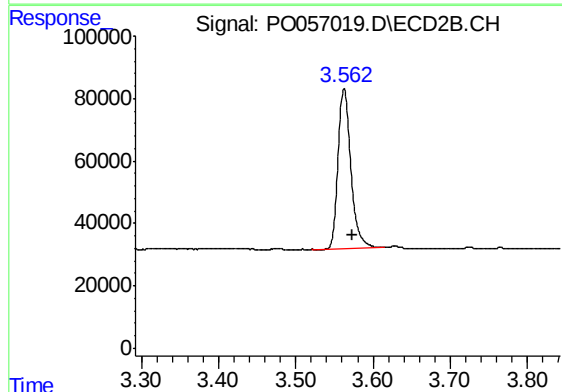


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: -0.011 min
Response: 571947
Conc: 17.34 ng/ml

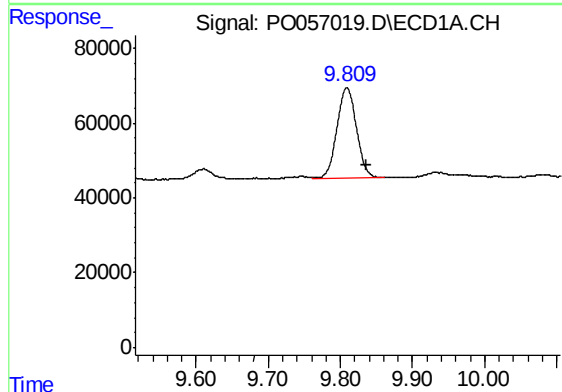

#2 Decachlorobiphenyl

R.T.: 9.809 min
Delta R.T.: -0.027 min
Response: 451624
Conc: 9.20 ng/ml m

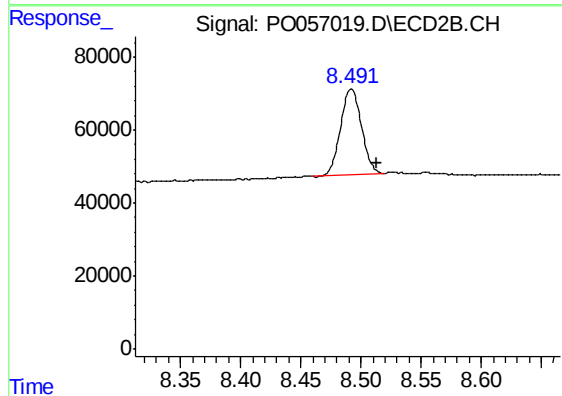

#2 Decachlorobiphenyl

R.T.: 8.492 min
Delta R.T.: -0.021 min
Response: 284650
Conc: 7.98 ng/ml