

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
 Data File : P0057029.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2019 11:48
 Operator : SM/SJ
 Sample : K3204-02RE
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-2RE

Manual Integrations
 APPROVED

Ankita
 6/11/2019 2:44:11 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 10 12:40:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.242	3.564	278399	245207	7.272m	7.435
2)	SA Decachlor...	9.809	8.491	184834	115133	3.766m	3.229

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061019\
Data File : PO057029.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2019 11:48
Operator : SM/SJ
Sample : K3204-02RE
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-2RE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:11 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 10 12:40:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

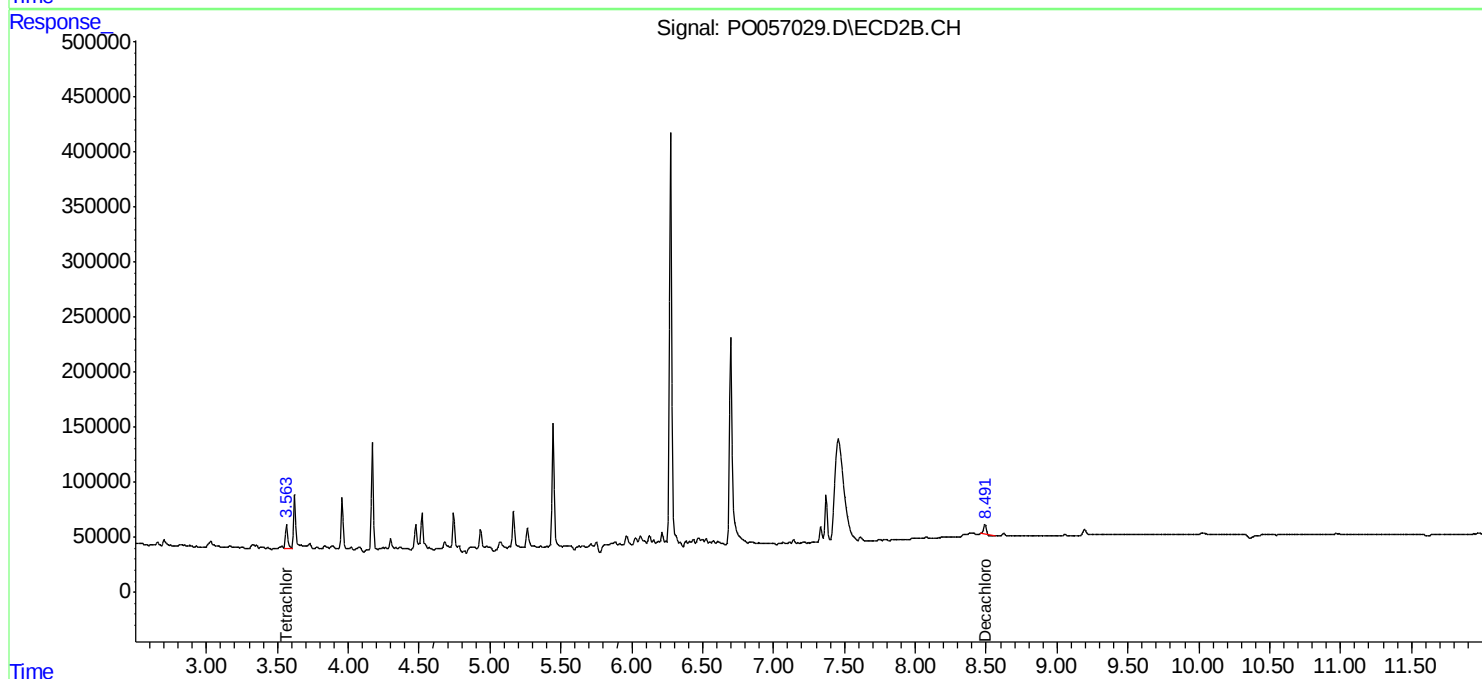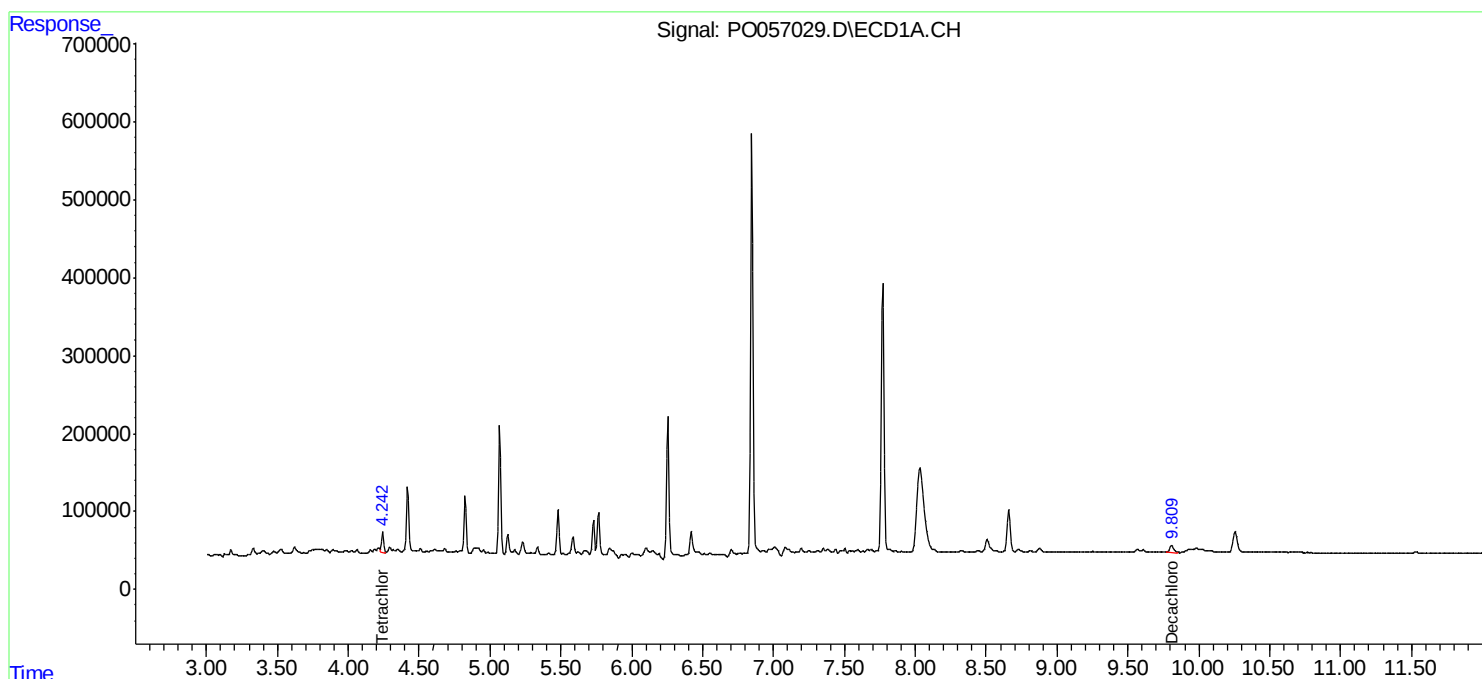

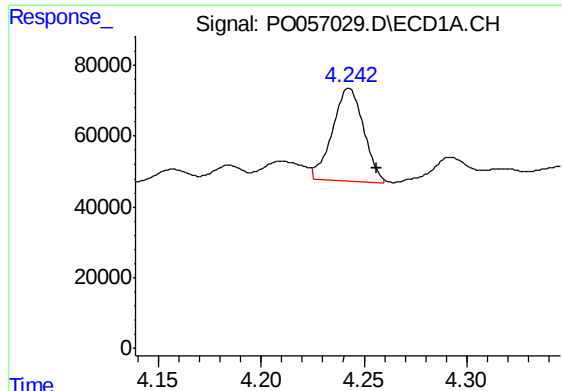


#1 Tetrachloro-m-xylene

R.T.: 4.242 min
Delta R.T.: -0.014 min
Response: 278399
Conc: 7.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-2RE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:11 PM

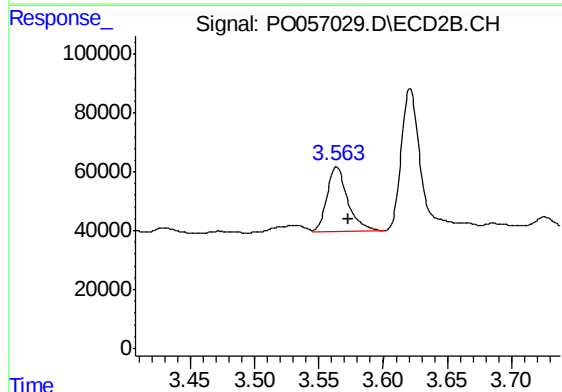


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.009 min
Response: 245207
Conc: 7.44 ng/ml

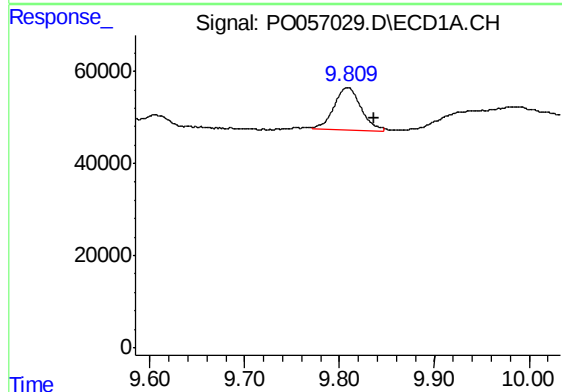

#2 Decachlorobiphenyl

R.T.: 9.809 min
Delta R.T.: -0.027 min
Response: 184834
Conc: 3.77 ng/ml m

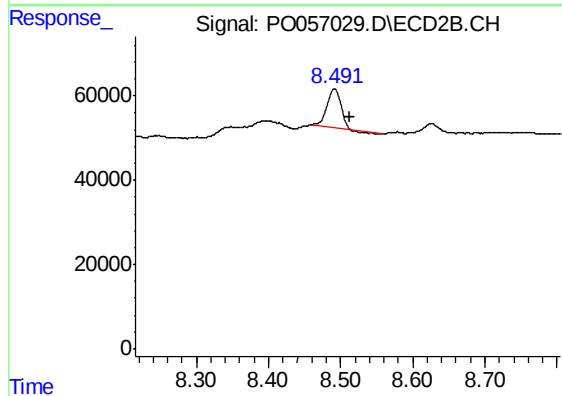

#2 Decachlorobiphenyl

R.T.: 8.491 min
Delta R.T.: -0.022 min
Response: 115133
Conc: 3.23 ng/ml