

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
 Data File : P0057036.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2019 14:03
 Operator : SM/SJ
 Sample : K3241-10RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Q115-4ARE

Manual Integrations
 APPROVED

Ankita
 6/11/2019 2:44:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:48:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.244	3.563	712576	566637	18.613	17.182
2) SA Decachlor...	9.809	8.492	412047	291937	8.395m	8.187m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
Data File : P0057036.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2019 14:03
Operator : SM/SJ
Sample : K3241-10RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Q115-4ARE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:48:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

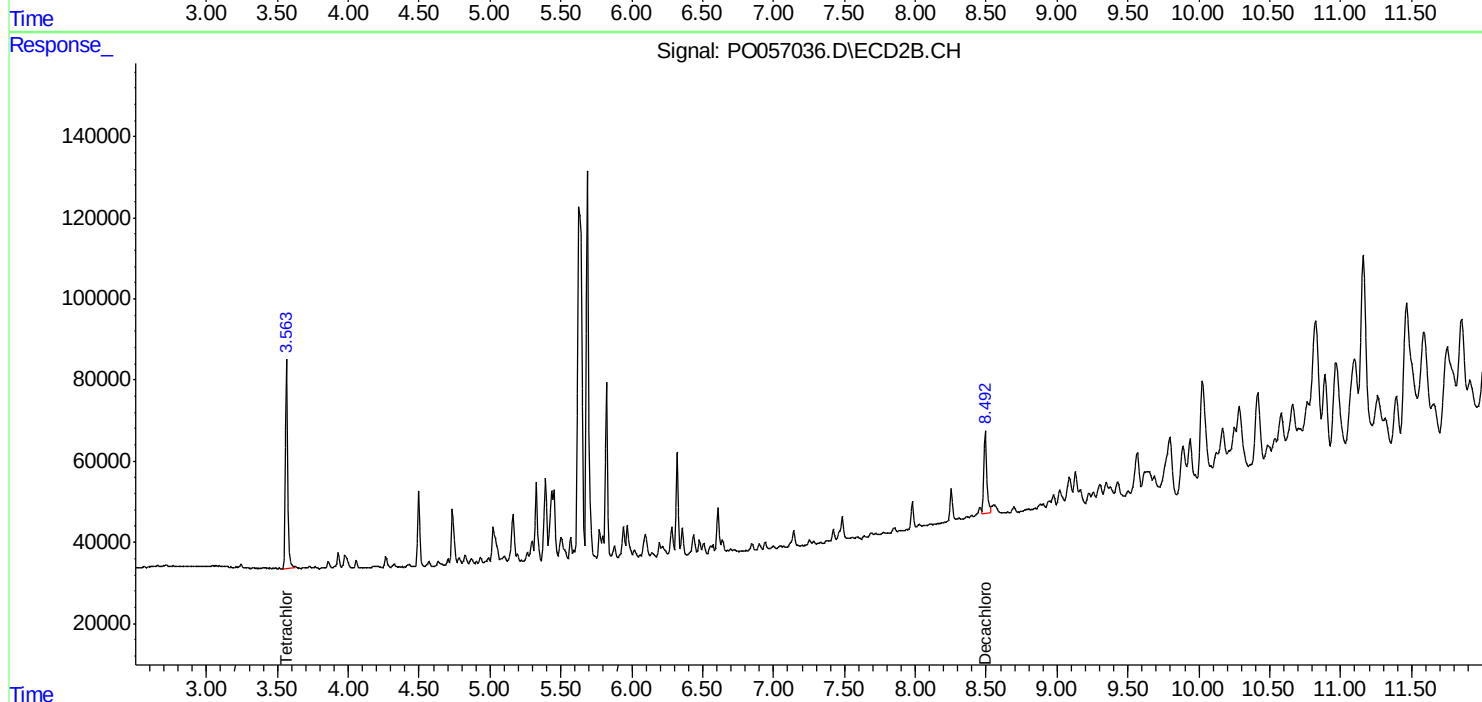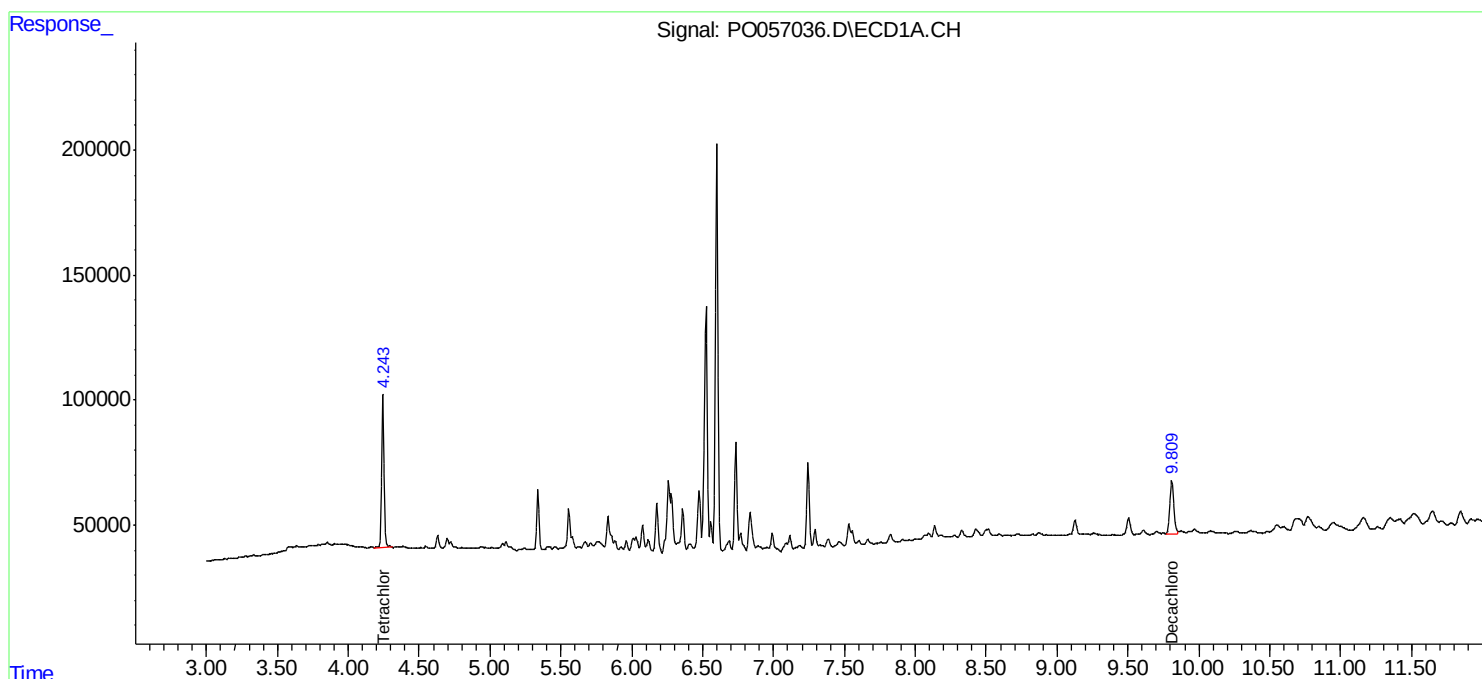

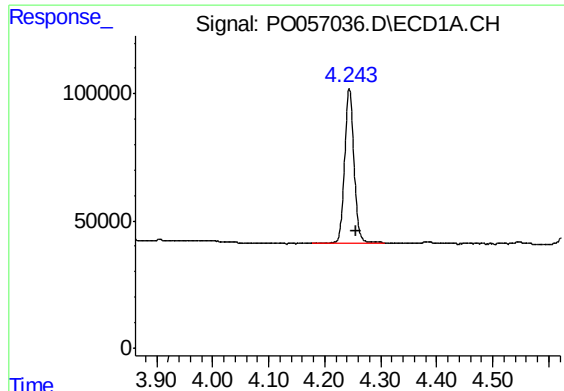


#1 Tetrachloro-m-xylene

R.T.: 4.244 min
Delta R.T.: -0.012 min
Response: 712576
Conc: 18.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
Q115-4ARE


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:19 PM

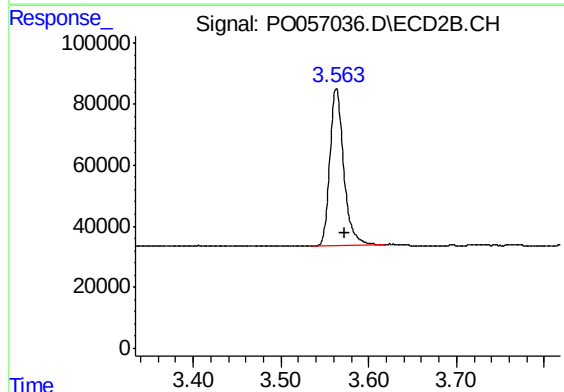


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.010 min
Response: 566637
Conc: 17.18 ng/ml

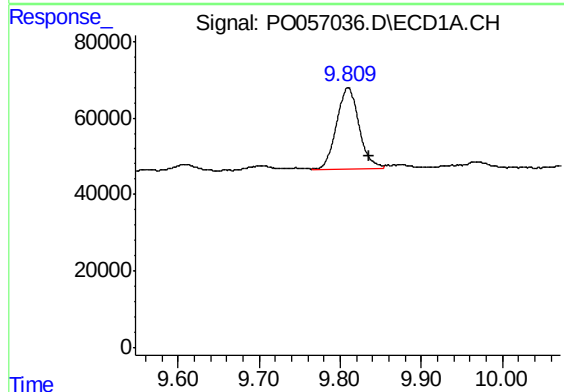

#2 Decachlorobiphenyl

R.T.: 9.809 min
Delta R.T.: -0.027 min
Response: 412047
Conc: 8.39 ng/ml m

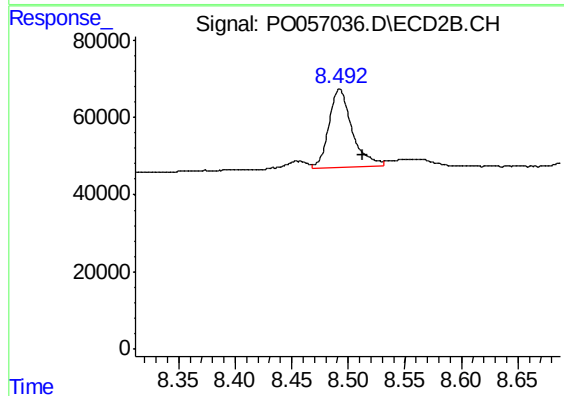

#2 Decachlorobiphenyl

R.T.: 8.492 min
Delta R.T.: -0.021 min
Response: 291937
Conc: 8.19 ng/ml m