

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061019\
 Data File : P0057043.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2019 17:11
 Operator : SM/SJ
 Sample : K3160-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 EO-02-060619-A

Manual Integrations
 APPROVED

Ankita
 6/11/2019 2:44:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 05:52:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0052319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 24 00:11:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.245	3.564	951801	803940	24.862m	24.378
2)	SA Decachlor...	9.814	8.494	962179	602081	19.603	16.885

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO061019\
Data File : PO057043.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2019 17:11
Operator : SM/SJ
Sample : K3160-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
EO-02-060619-A


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 05:52:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO052319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 24 00:11:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

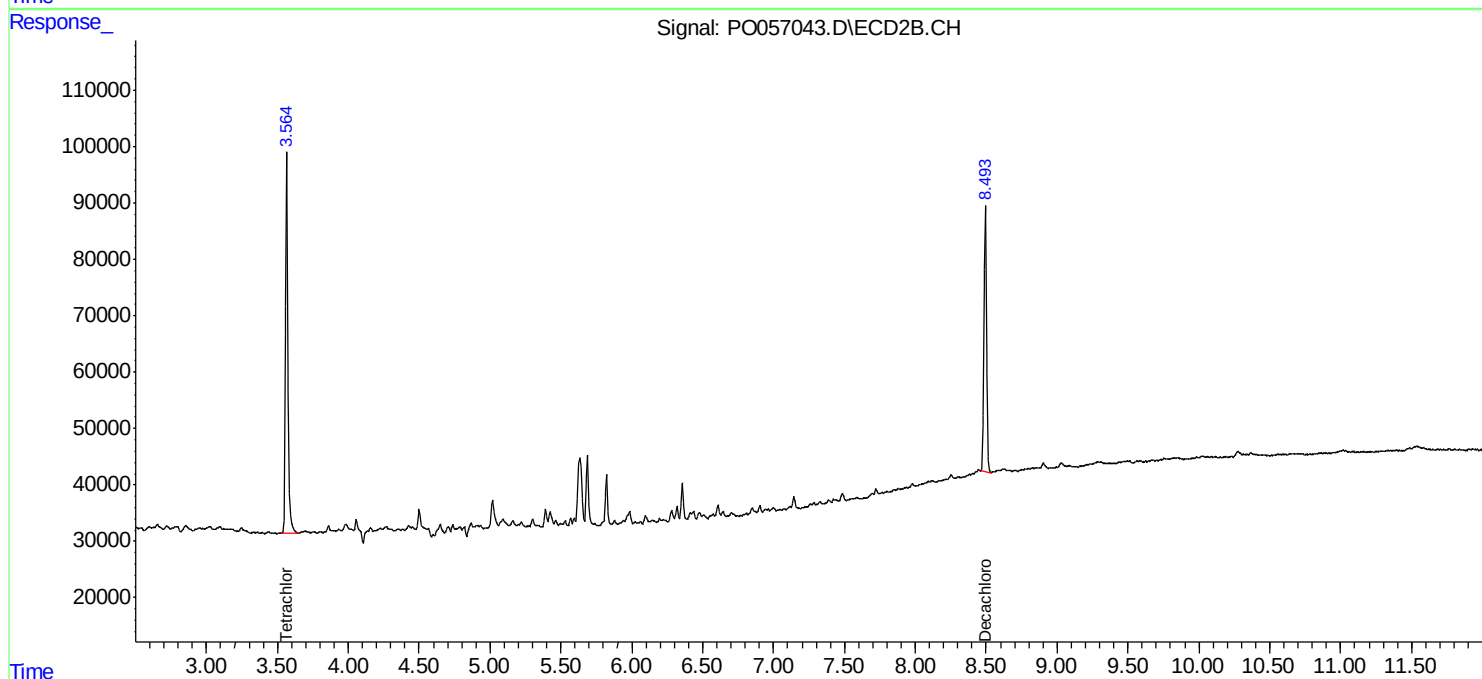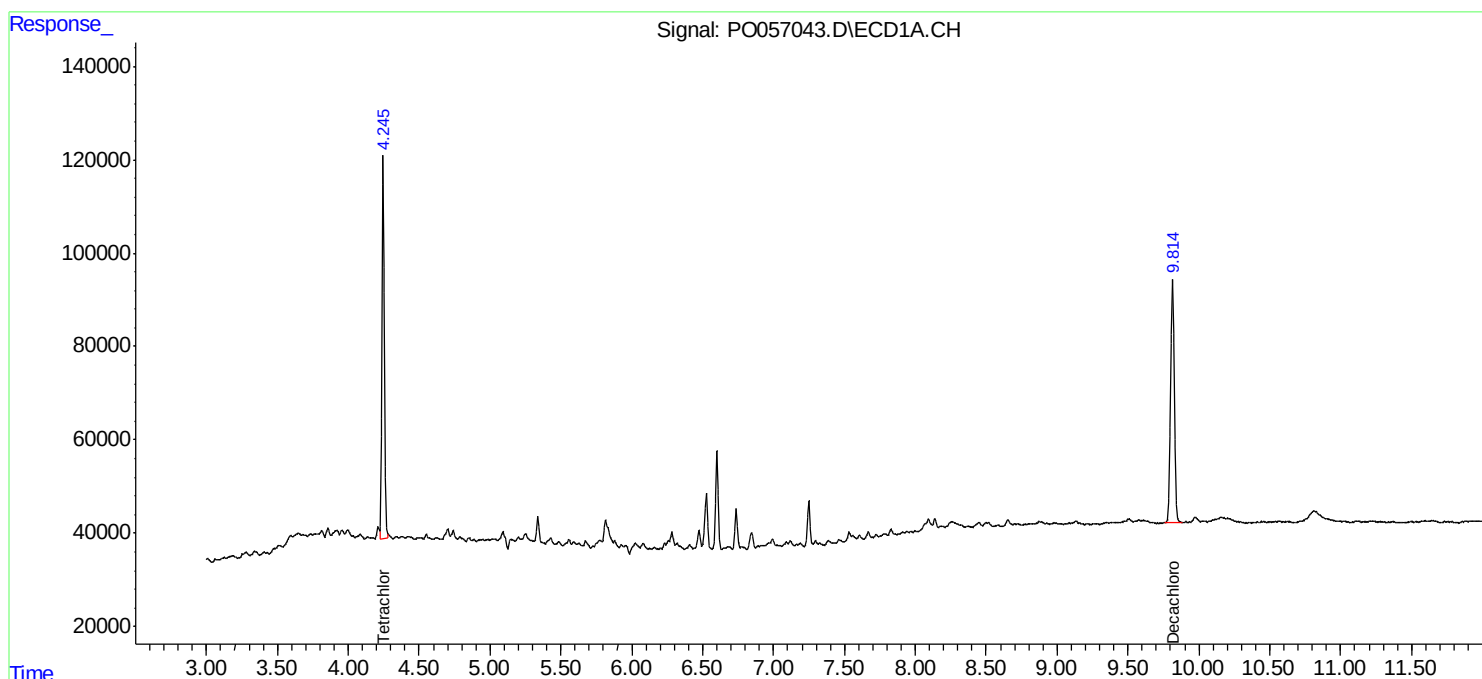

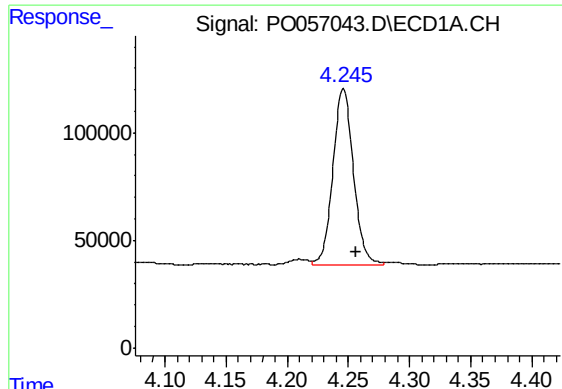


#1 Tetrachloro-m-xylene

R.T.: 4.245 min
Delta R.T.: -0.011 min
Response: 951801
Conc: 24.86 ng/ml m

Instrument :
ECD_O
ClientSampleId :
EO-02-060619-A


Manual Integrations
APPROVED

Ankita
6/11/2019 2:44:27 PM

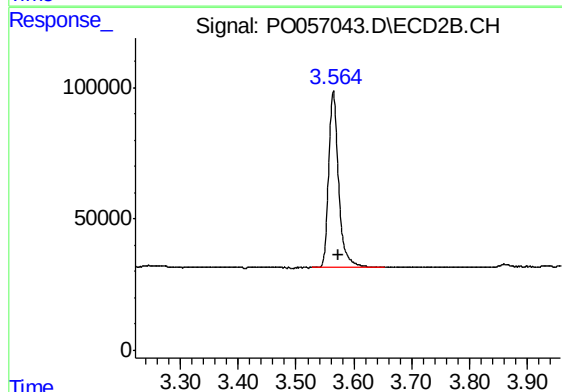


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.009 min
Response: 803940
Conc: 24.38 ng/ml

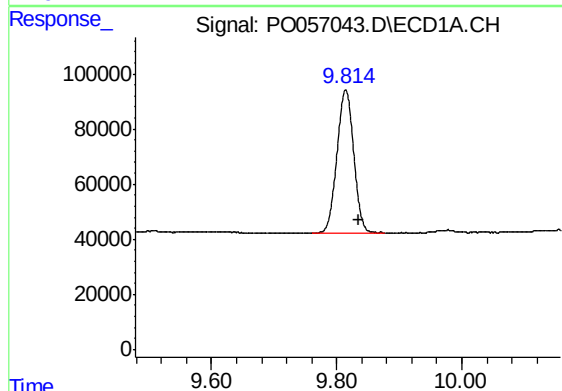

#2 Decachlorobiphenyl

R.T.: 9.814 min
Delta R.T.: -0.022 min
Response: 962179
Conc: 19.60 ng/ml

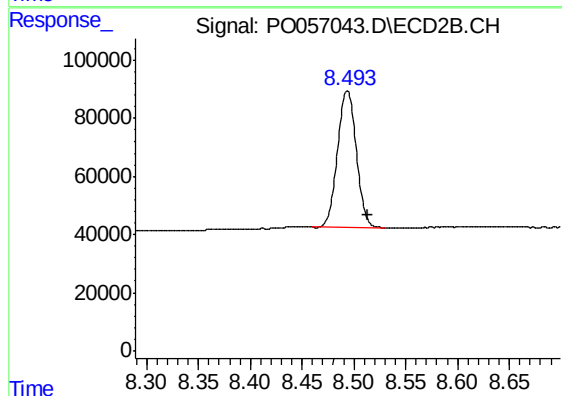

#2 Decachlorobiphenyl

R.T.: 8.494 min
Delta R.T.: -0.019 min
Response: 602081
Conc: 16.89 ng/ml