

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
 Data File : P0078606.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jun 2021 11:00
 Operator : DD\AJ
 Sample : M2641-03 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMA727F-END-1-1

Manual Integrations
 APPROVED

Ankita
 6/11/2021 1:42:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 11 02:13:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 08 05:39:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.337	3.612	52979	25541	0.694	0.808m
2) SA Decachlor...	9.945	8.797	60447	37220	1.491	1.548

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0061021\
Data File : P0078606.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jun 2021 11:00
Operator : DD\AJ
Sample : M2641-03 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMA727F-END-1-1


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 11 02:13:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0060721.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 08 05:39:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

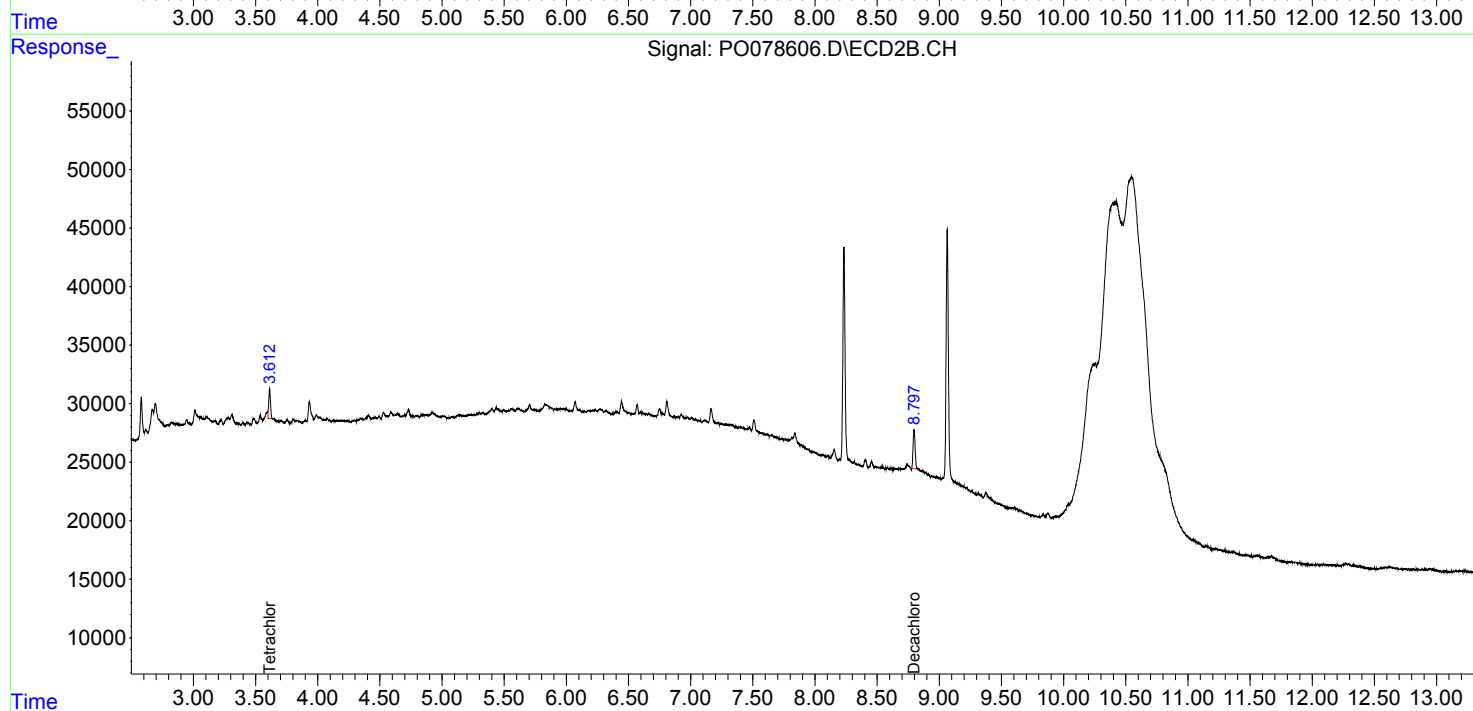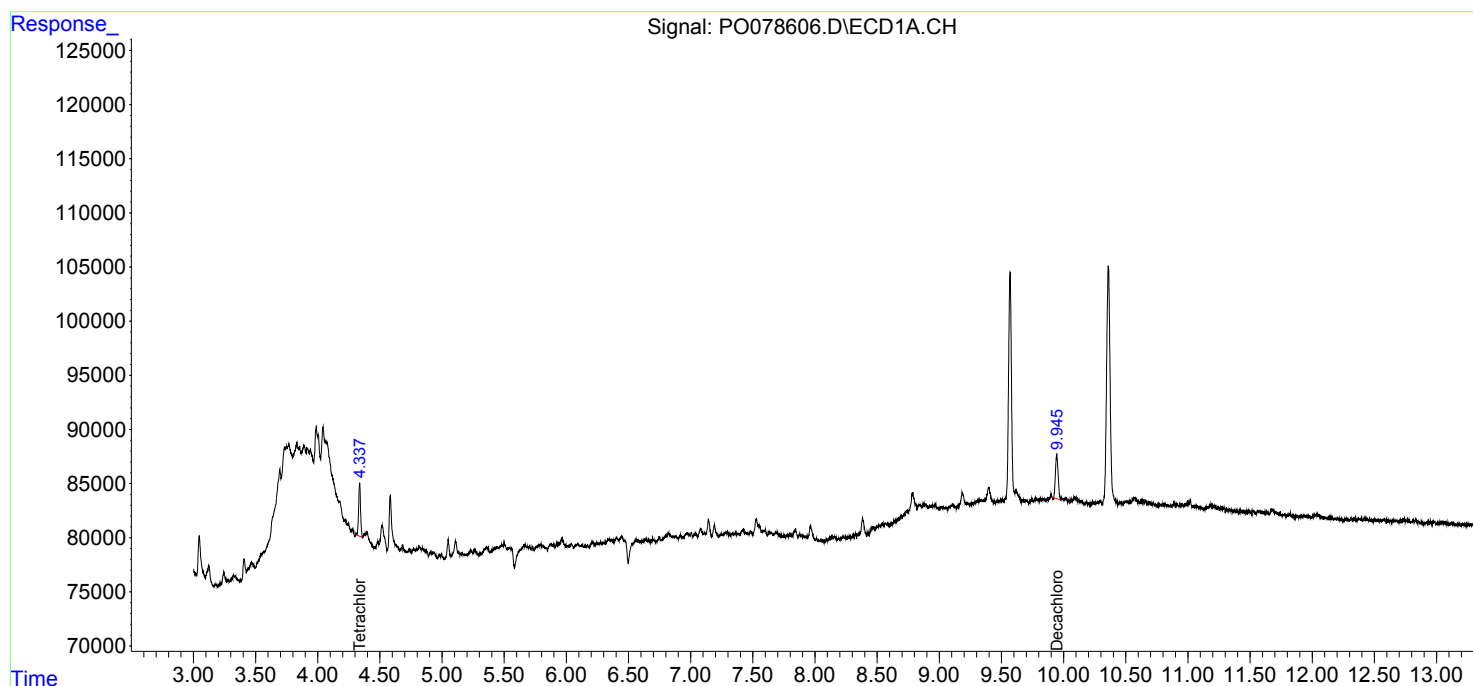

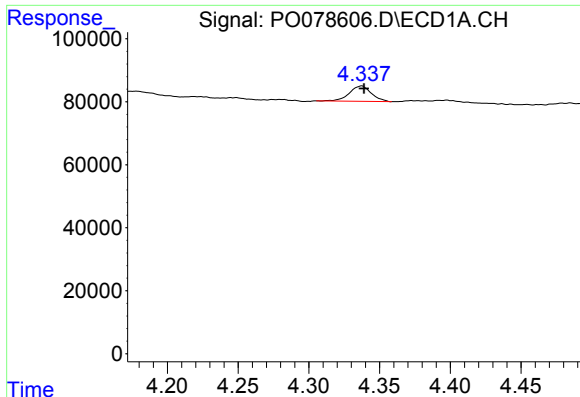


#1 Tetrachloro-m-xylene

R.T.: 4.337 min
Delta R.T.: -0.002 min
Response: 52979
Conc: 0.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMA727F-END-1-1


Manual Integrations
APPROVED

Ankita
6/11/2021 1:42:37 PM

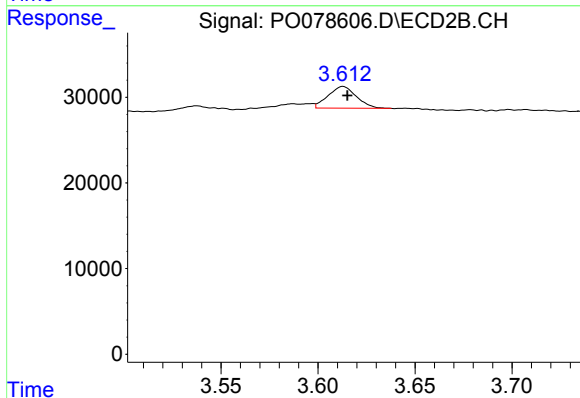


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.003 min
Response: 25541
Conc: 0.81 ng/ml m

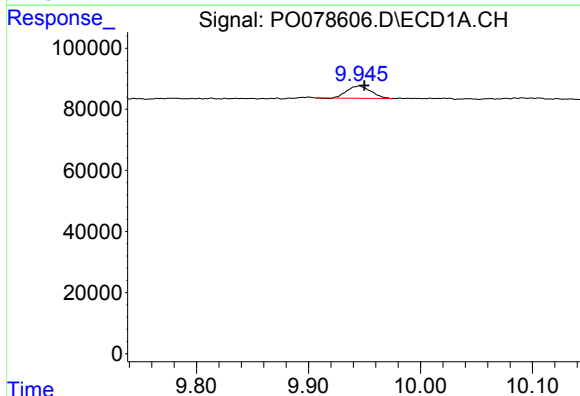

#2 Decachlorobiphenyl

R.T.: 9.945 min
Delta R.T.: -0.005 min
Response: 60447
Conc: 1.49 ng/ml

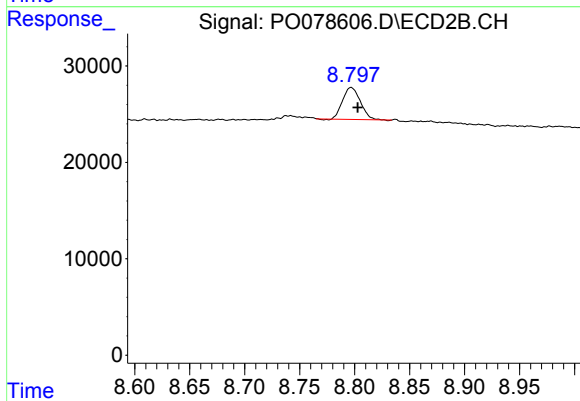

#2 Decachlorobiphenyl

R.T.: 8.797 min
Delta R.T.: -0.006 min
Response: 37220
Conc: 1.55 ng/ml